



Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111225\
Data File : VX048574.D
Acq On : 12 Nov 2025 13:21
Operator : JC/MD
Sample : Q3549-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RT4922

Quant Time: Nov 14 00:27:35 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 08 05:08:11 2025
Response via : Initial Calibration




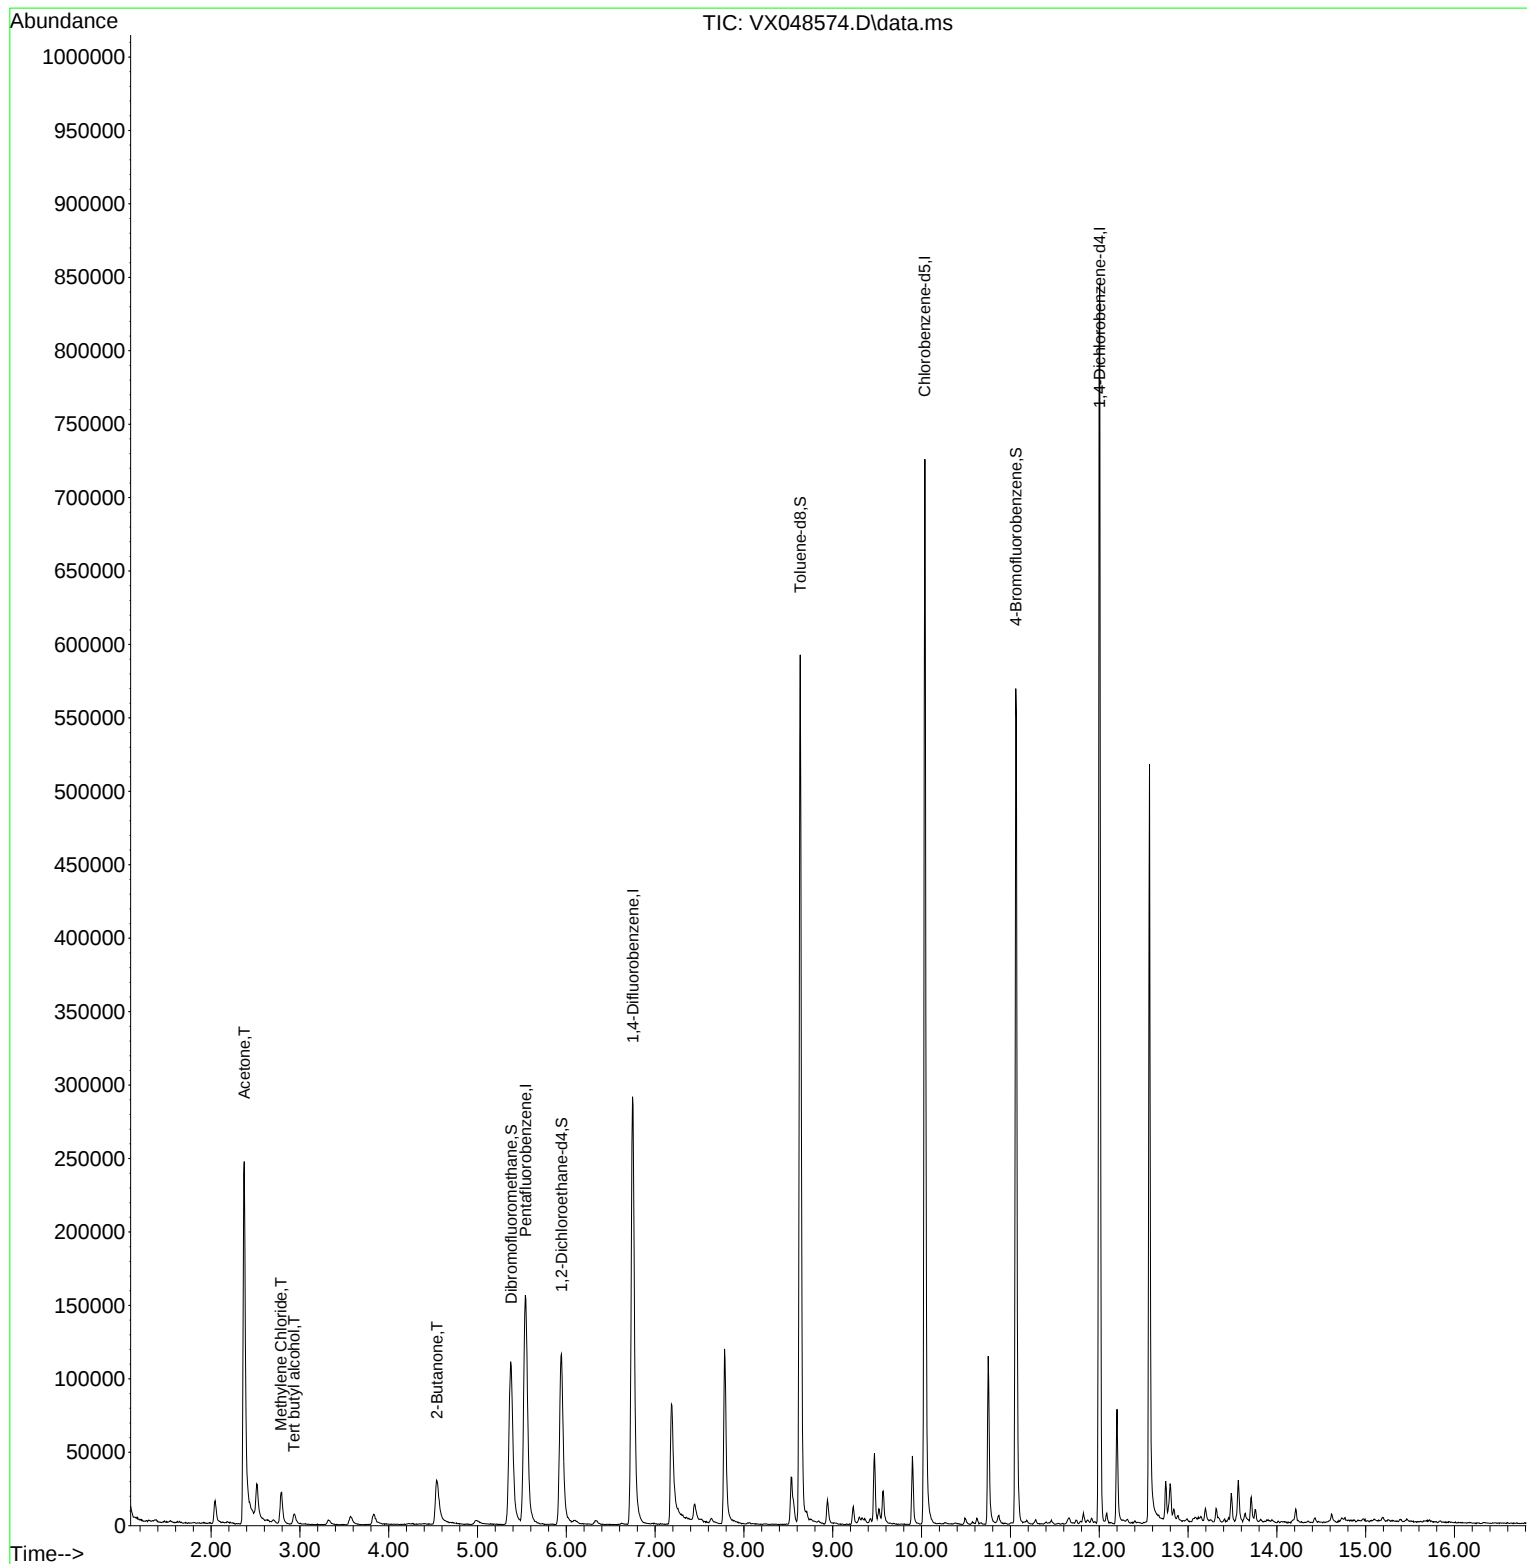


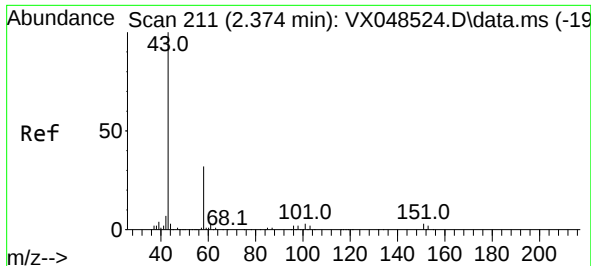

#16
Acetone
Concen: 287.446 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX048574.D
Acq: 12 Nov 2025 13:21

Instrument :
MSVOA_X
ClientSampleId :
RT4922

Tgt Ion: 43 Resp: 325415
Ion Ratio Lower Upper
43 100
58 33.5 25.8 38.6

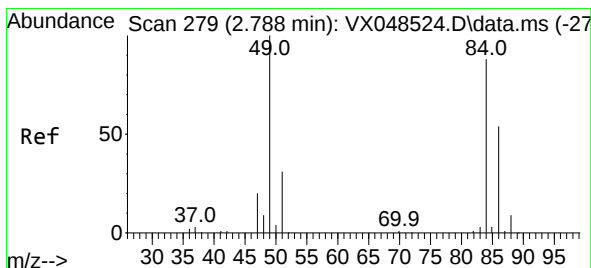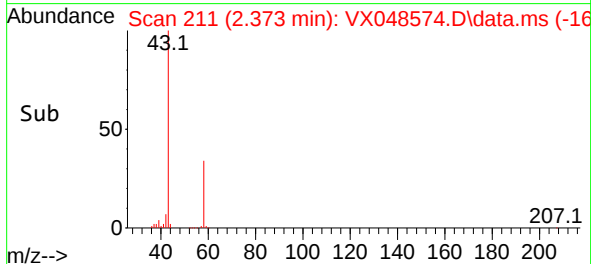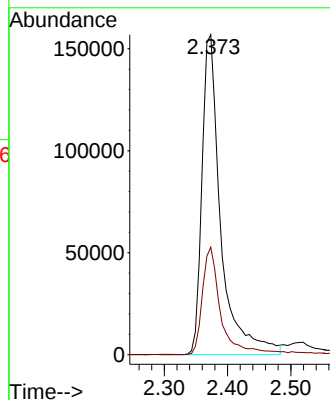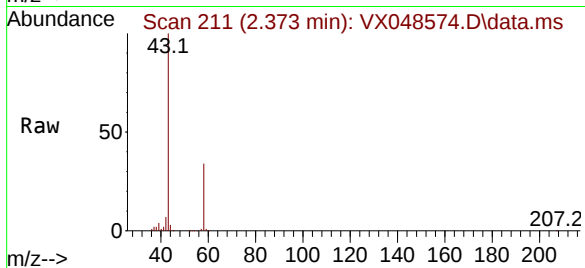

#20
Methylene Chloride
Concen: 4.943 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX048574.D
Acq: 12 Nov 2025 13:21

Tgt Ion: 84 Resp: 11504
Ion Ratio Lower Upper
84 100
49 106.0 91.2 136.8
51 33.6 28.3 42.5
86 55.9 49.4 74.2

