

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111225\
 Data File : VX048578.D
 Acq On : 12 Nov 2025 15:05
 Operator : JC/MD
 Sample : Q2893-07 0.2PPB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Quant Time: Nov 14 00:33:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 08 05:08:11 2025
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : John Carlone 11/14/2025
 Supervised By : Mahesh Dadoda 11/17/2025

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	182202	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	304522	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	281055	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	143278	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	110125	43.376	ug/l	0.00
Spiked Amount 50.000	Range 78 - 117		Recovery =	86.760%		
35) Dibromofluoromethane	5.373	113	92090	39.956	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery =	79.920%		
50) Toluene-d8	8.635	98	332301	46.228	ug/l	0.00
Spiked Amount 50.000	Range 92 - 112		Recovery =	92.460%		
62) 4-Bromofluorobenzene	11.061	95	131896	49.236	ug/l	0.00
Spiked Amount 50.000	Range 83 - 123		Recovery =	98.480%		
Target Compounds					Qvalue	
3) Chloromethane	1.307	50	397	0.203	ug/l #	80
5) Bromomethane	1.618	94	484	0.346	ug/l #	61
10) Methyl Iodide	2.465	142	1000	0.333	ug/l	95
11) Tert butyl alcohol	2.947	59	410m	0.852	ug/l	
13) Acrolein	2.239	56	221	3.175	ug/l	84
15) Acrylonitrile	3.075	53	732	0.521	ug/l #	89
16) Acetone	2.380	43	1723	1.434	ug/l #	67
18) Methyl Acetate	2.703	43	799	0.242	ug/l #	51
20) Methylene Chloride	2.788	84	1094	0.443	ug/l	91
23) Vinyl Acetate	3.739	43	3545	0.534	ug/l #	83
25) 2-Butanone	4.562	43	1515m	0.852	ug/l	
26) 2,2-Dichloropropane	4.471	77	1005m	0.283	ug/l	
29) Tetrahydrofuran	5.001	42	911m	0.718	ug/l	
36) 1,1-Dichloropropene	5.684	75	627	0.203	ug/l #	52
38) Carbon Tetrachloride	5.611	117	1113m	0.317	ug/l	
49) 1,4-Dioxane	7.671	88	19m	0.459	ug/l	
51) 4-Methyl-2-Pentanone	8.561	43	2454	0.706	ug/l	95
58) 2-Chloroethyl Vinyl ether	8.238	63	1419	0.788	ug/l	96
59) 2-Hexanone	9.433	43	1771	0.685	ug/l	97
68) m/p-Xylenes	10.287	106	1207	0.286	ug/l	96
71) Bromoform	10.787	173	449	0.218	ug/l #	28
76) 1,2,3-Trichloropropane	11.220	75	723m	0.209	ug/l	
88) 1,4-Dichlorobenzene	12.018	146	1128m	0.217	ug/l	
89) n-Butylbenzene	12.317	91	1925	0.225	ug/l	79
96) 1,2,3-Trichlorobenzene	13.945	180	608	0.204	ug/l #	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111225\
Data File : VX048578.D
Acq On : 12 Nov 2025 15:05
Operator : JC/MD
Sample : Q2893-07 0.2PPB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Quant Time: Nov 14 00:33:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 08 05:08:11 2025
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By : John Carlone 11/14/2025
Supervised By : Mahesh Dadoda 11/17/2025

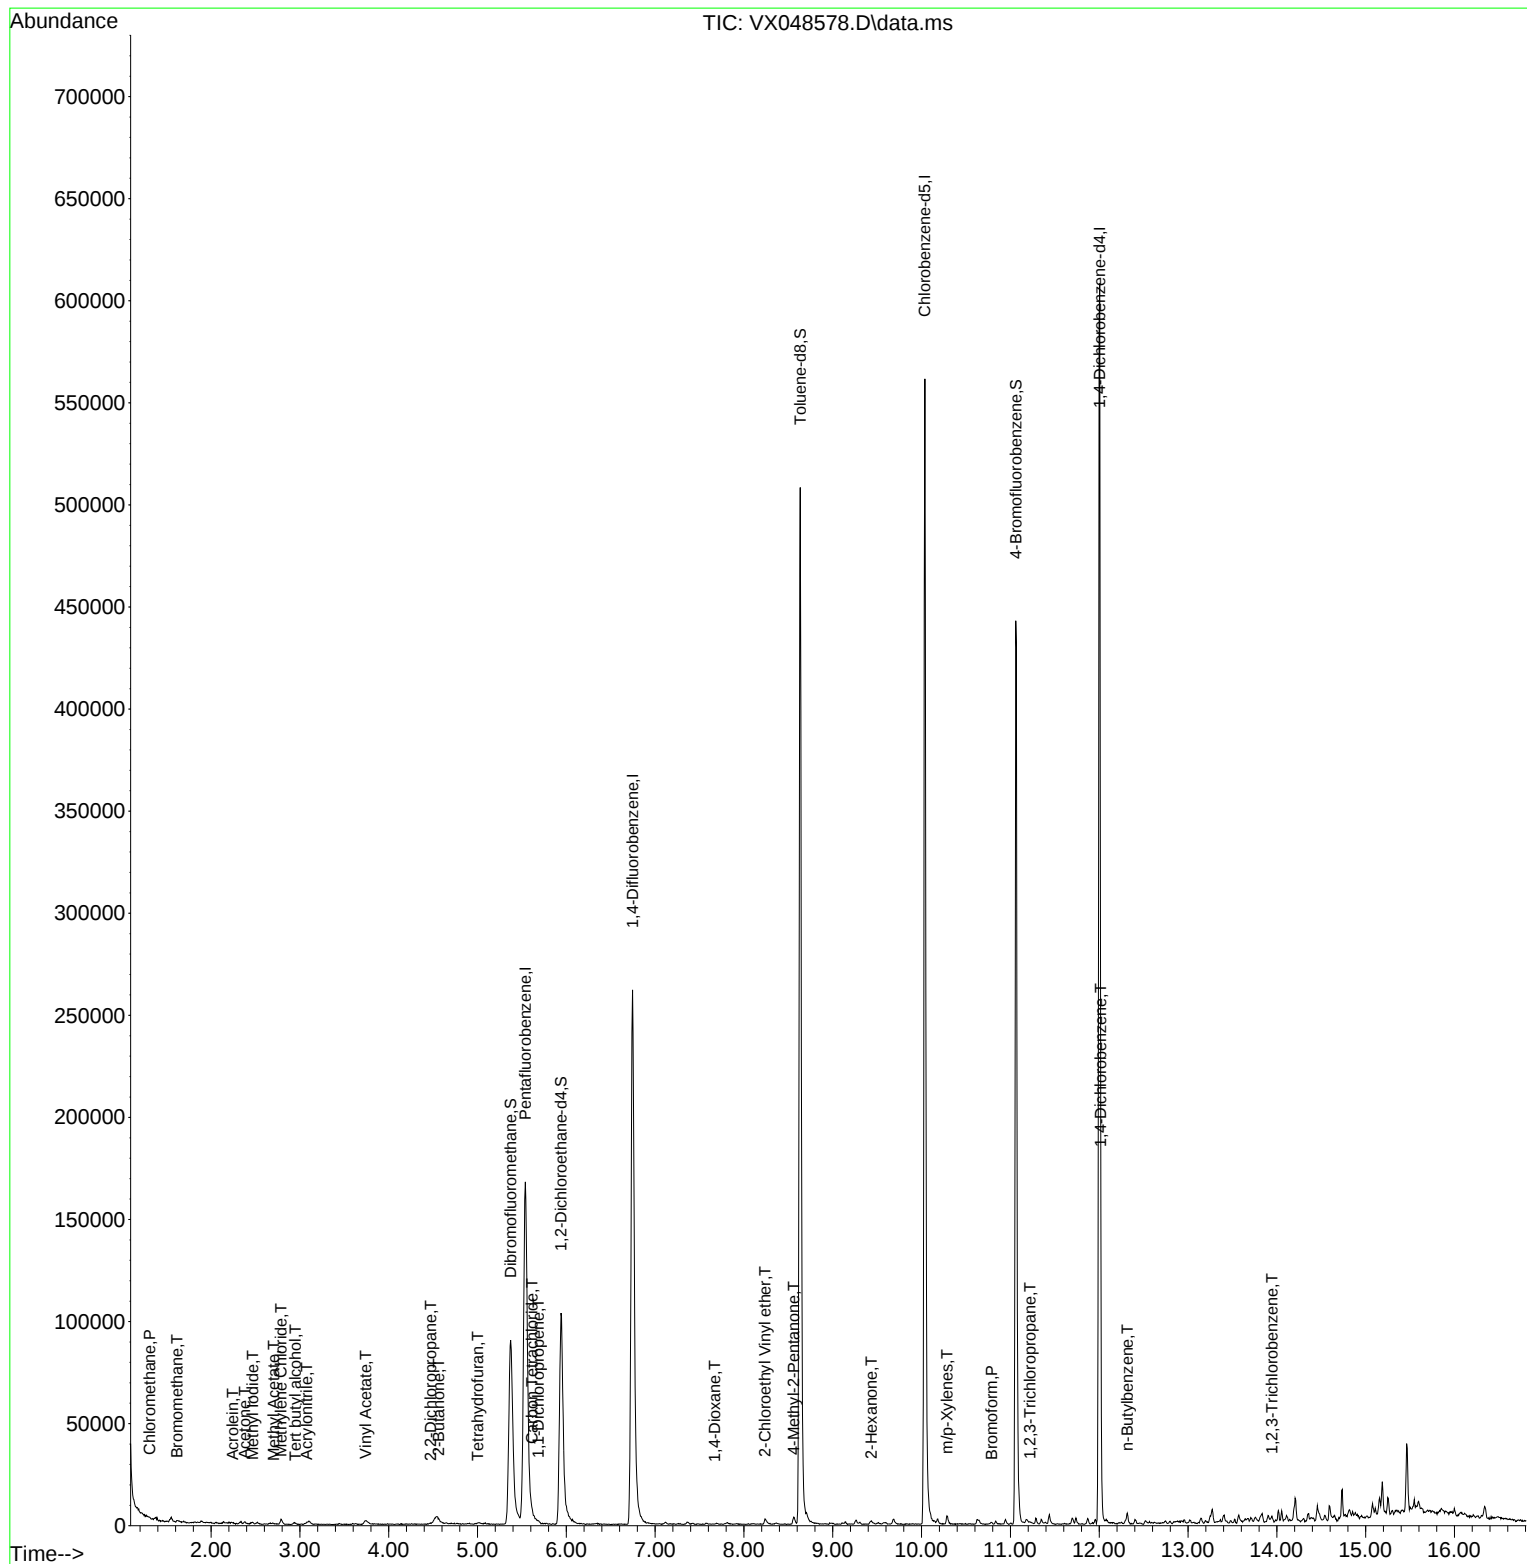







#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Instrument : MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Tgt Ion:168 Resp: 18220
Ion Ratio Lower Upper
168 100
99 59.1 45.2 67.8




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

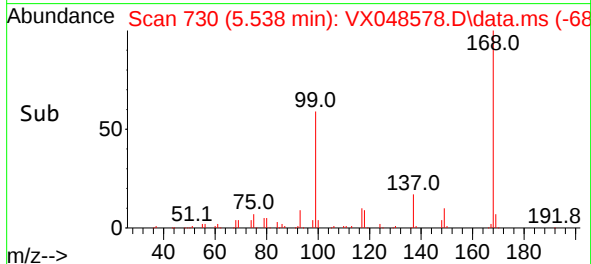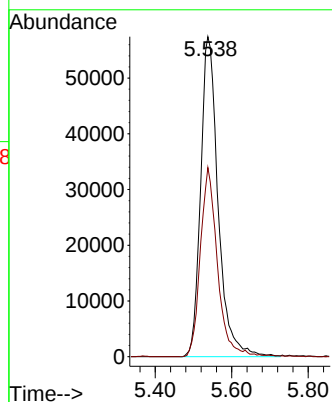

#3
Chloromethane
Concen: 0.203 ug/l
RT: 1.307 min Scan# 36
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion: 50 Resp: 397
Ion Ratio Lower Upper
50 100
52 21.1 26.0 39.0#

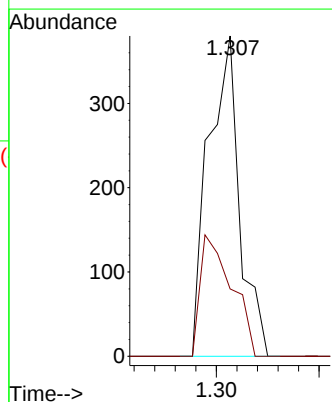

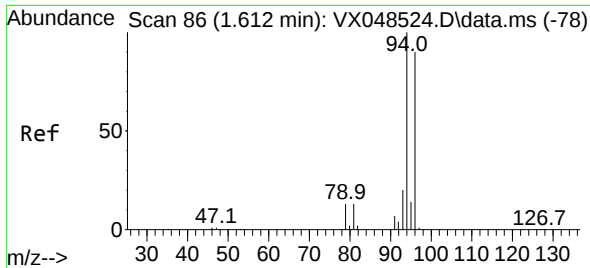

#5
Bromomethane
Concen: 0.346 ug/l
RT: 1.618 min Scan# 81
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

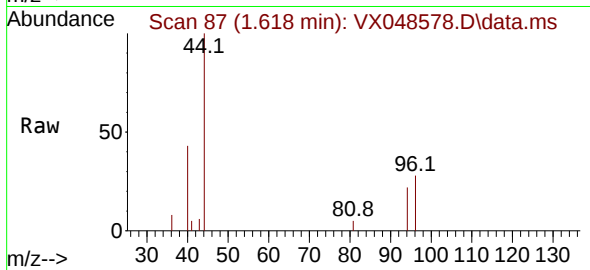

Tgt Ion: 94 Resp: 484
Ion Ratio Lower Upper
94 100
96 127.7 72.3 108.5




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

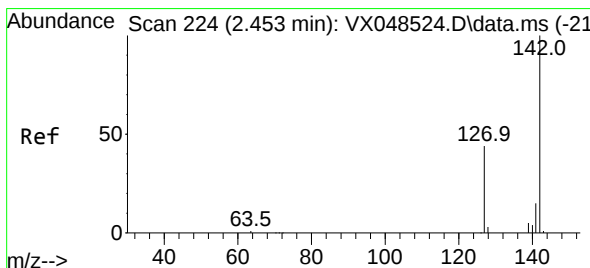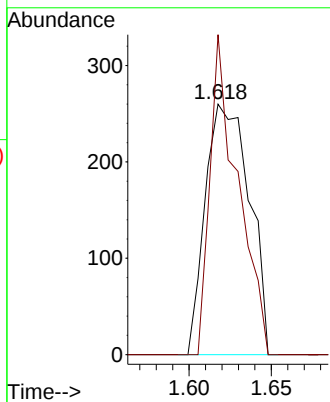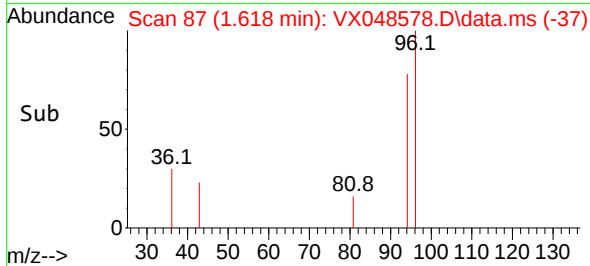

#10
Methyl Iodide
Concen: 0.333 ug/l
RT: 2.465 min Scan# 226
Delta R.T. 0.012 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion:142 Resp: 1000
Ion Ratio Lower Upper
142 100
127 48.1 35.8 53.6
141 12.3 11.4 17.0

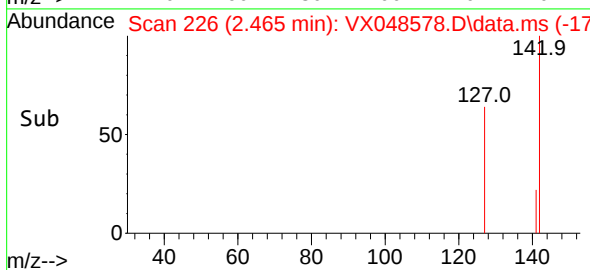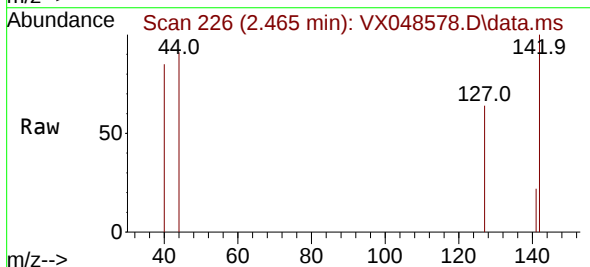



#11
Tert butyl alcohol
Concen: 0.852 ug/l m
RT: 2.947 min Scan# 304
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05




Instrument : MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025



Tgt Ion: 59 Resp: 410
Ion Ratio Lower Upper
59 100
57 0.0 8.6 13.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

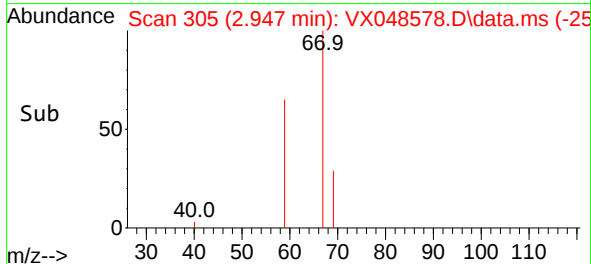

#13
Acrolein
Concen: 3.175 ug/l
RT: 2.239 min Scan# 189
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Tgt Ion: 56 Resp: 221
Ion Ratio Lower Upper
56 100
55 55.7 54.9 82.3









#15
Acrylonitrile
Concen: 0.521 ug/l
RT: 3.075 min Scan# 31
Delta R.T. 0.018 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Tgt Ion: 53 Resp: 732
Ion Ratio Lower Upper
53 100
52 79.5 65.3 97.9
51 16.0 27.8 41.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

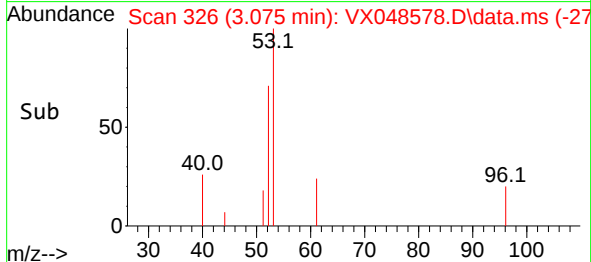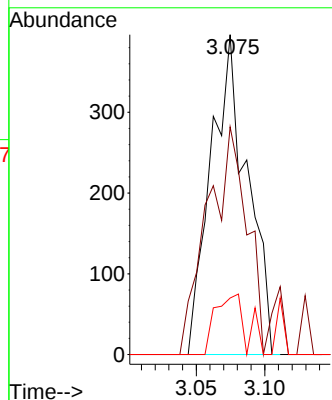

#16
Acetone
Concen: 1.434 ug/l
RT: 2.380 min Scan# 212
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion: 43 Resp: 1723
Ion Ratio Lower Upper
43 100
58 50.9 25.8 38.6

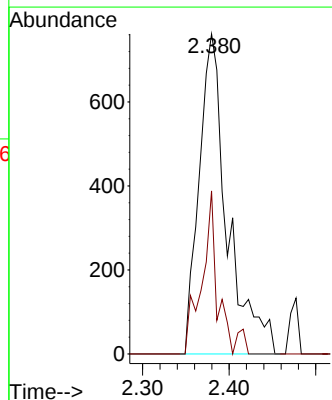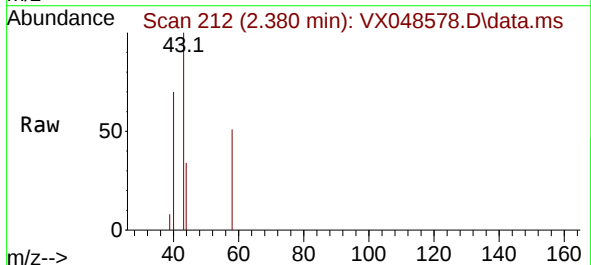



#18
Methyl Acetate
Concen: 0.242 ug/l
RT: 2.703 min Scan# 20
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025



Tgt Ion: 43 Resp: 799
Ion Ratio Lower Upper
43 100
74 0.0 19.1 28.7




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

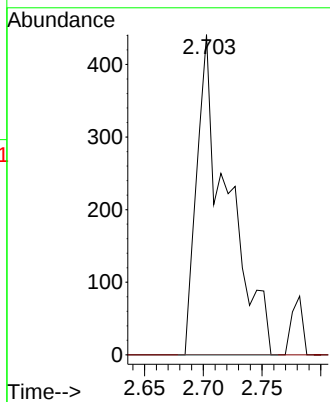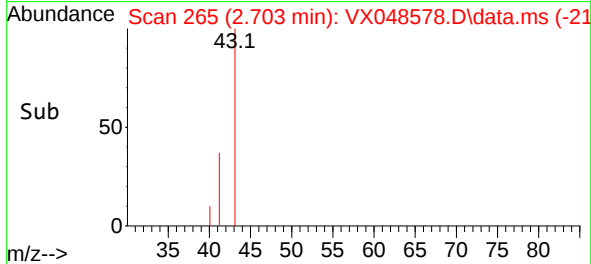

#20
Methylene Chloride
Concen: 0.443 ug/l
RT: 2.788 min Scan# 279
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion: 84 Resp: 1094
Ion Ratio Lower Upper
84 100
49 126.2 91.2 136.8
51 41.7 28.3 42.5
86 64.3 49.4 74.2

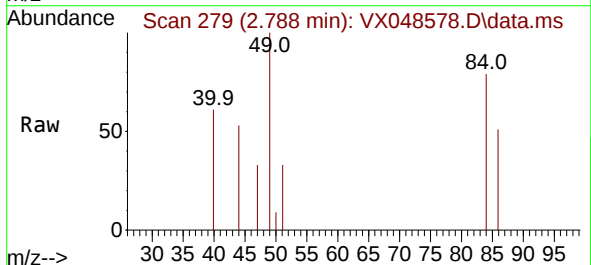



#23
 Vinyl Acetate
 Concen: 0.534 ug/l
 RT: 3.739 min Scan# 41
 Delta R.T. 0.024 min
 Lab File: VX048578.D
 Acq: 12 Nov 2025 15:05




Instrument :
 MSVOA_X
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025



Tgt Ion: 43 Resp: 354
 Ion Ratio Lower Upper
 43 100
 86 4.9 9.0 13.6




Manual Integrations
 APPROVED


Reviewed By :John Carlone 11/14/2025
 Supervised By :Mahesh Dadoda 11/17/2025



#25
 2-Butanone
 Concen: 0.852 ug/l m
 RT: 4.562 min Scan# 570
 Delta R.T. 0.024 min
 Lab File: VX048578.D
 Acq: 12 Nov 2025 15:05

Tgt Ion: 43 Resp: 1515
 Ion Ratio Lower Upper
 43 100
 72 16.8 21.5 32.3

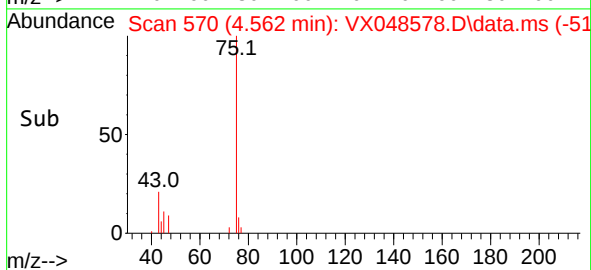



#26

2,2-Dichloropropane

Concen: 0.283 ug/l m

RT: 4.471 min Scan# 5

Delta R.T. 0.006 min

Lab File: VX048578.D

Acq: 12 Nov 2025 15:05

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT3-2025

Tgt Ion: 77 Resp: 100

Ion Ratio Lower Upper

77 100





97 2.1 11.7 35.1

Manual Integrations

APPROVED

Reviewed By :John Carlone 11/14/2025

Supervised By :Mahesh Dadoda 11/17/2025



#29

Tetrahydrofuran

Concen: 0.718 ug/l m

RT: 5.001 min Scan# 642

Delta R.T. 0.012 min

Lab File: VX048578.D

Acq: 12 Nov 2025 15:05




Tgt Ion: 42 Resp: 911


Ion Ratio Lower Upper

42 100

72 22.7 36.3 54.5#

71 26.1 34.1 51.1#

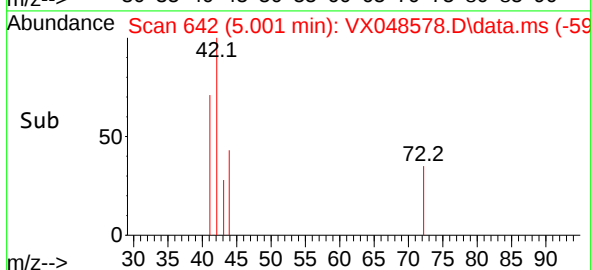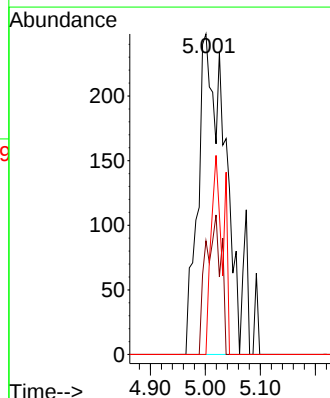







#33
 1,2-Dichloroethane-d4
 Concen: 43.376 ug/l
 RT: 5.940 min Scan# 797
 Delta R.T. -0.006 min
 Lab File: VX048578.D
 Acq: 12 Nov 2025 15:05

Instrument : MSVOA_X
 ClientSampleId : LOD-MDL-WATER-01-QT3-2025

Tgt Ion: 65 Resp: 110125
 Ion Ratio Lower Upper
 65 100
 67 53.3 0.0 106.2




Manual Integrations
 APPROVED


Reviewed By :John Carlone 11/14/2025
 Supervised By :Mahesh Dadoda 11/17/2025

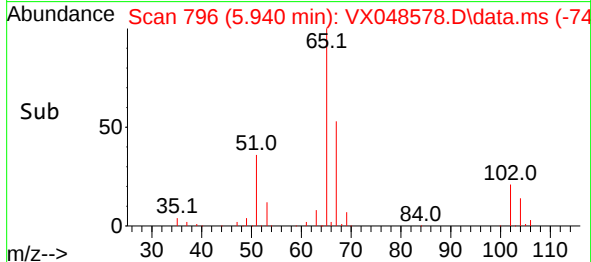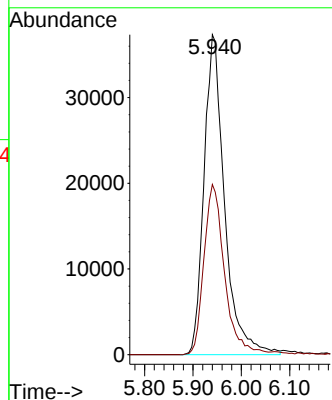

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.745 min Scan# 928
 Delta R.T. -0.000 min
 Lab File: VX048578.D
 Acq: 12 Nov 2025 15:05


Tgt Ion:114 Resp: 304522
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 41.2
 88 16.3 0.0 32.2

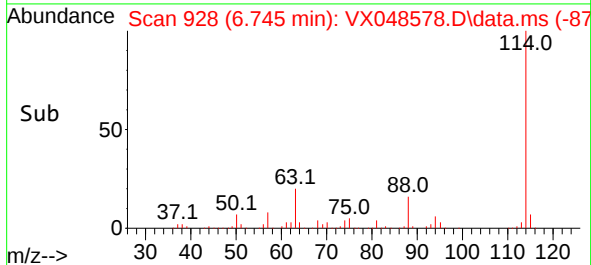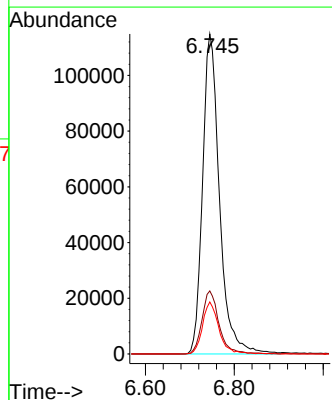

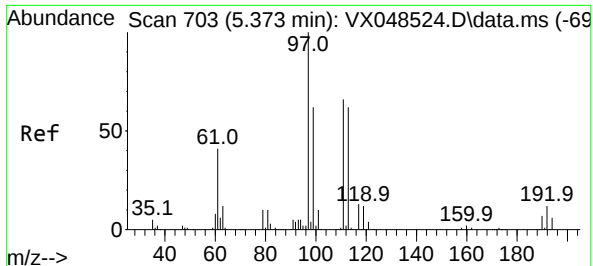

#35
Dibromofluoromethane
Concen: 39.956 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05




Instrument : MSVOA_X
ClientSampleId : LOD-MDL-WATER-01-QT3-2025

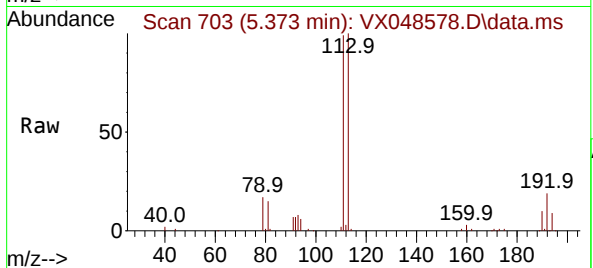

Tgt Ion: 113 Resp: 92090
Ion Ratio Lower Upper
113 100
111 103.7 81.9 122.9
192 19.8 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

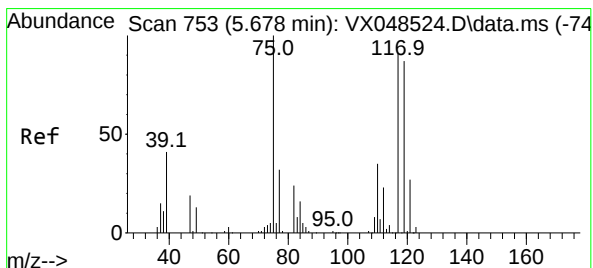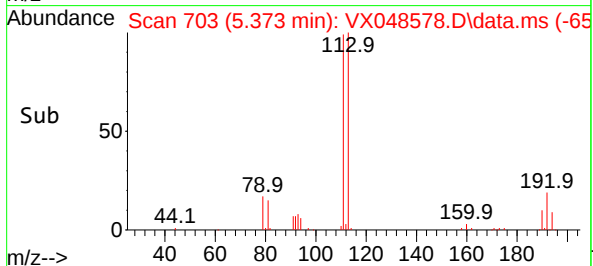

#36
1,1-Dichloropropene
Concen: 0.203 ug/l
RT: 5.684 min Scan# 754
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion: 75 Resp: 627
Ion Ratio Lower Upper
75 100
110 9.7 18.4 55.4#
77 3.0 24.6 37.0#

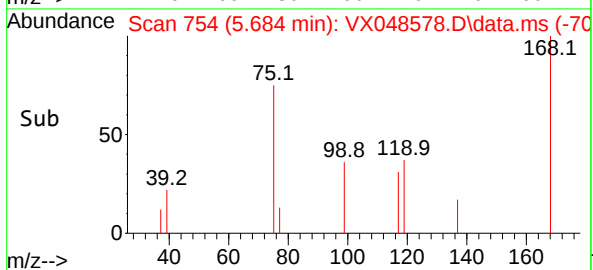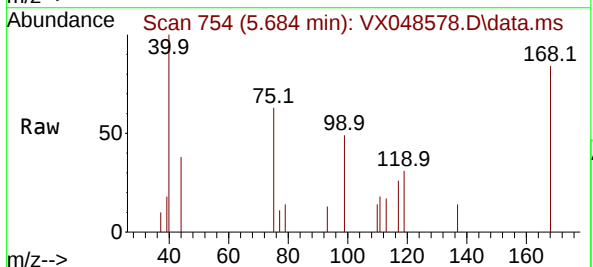



#38
Carbon Tetrachloride
Concen: 0.317 ug/l m
RT: 5.611 min Scan# 74
Delta R.T. -0.055 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05




Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025



Tgt Ion: 117 Resp: 111
Ion Ratio Lower Upper
117 100
119 0.0 74.5 111.7#
121 0.0 24.8 37.2#




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

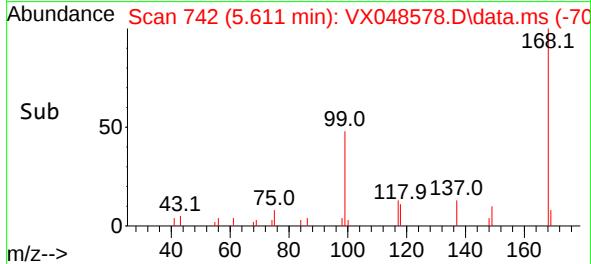

#49
1,4-Dioxane
Concen: 0.459 ug/l m
RT: 7.671 min Scan# 1080
Delta R.T. 0.024 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Tgt Ion: 88 Resp: 19
Ion Ratio Lower Upper
88 100
43 0.0 25.1 37.7#
58 0.0 56.7 85.1#

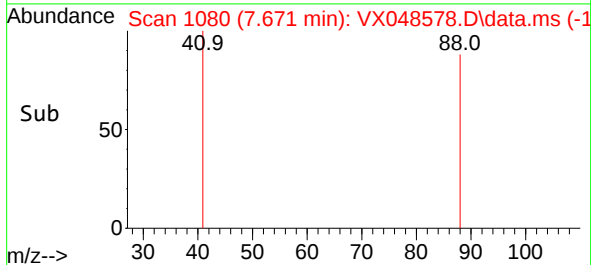







#50
Toluene-d8
Concen: 46.228 ug/l
RT: 8.635 min Scan# 1238
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Instrument :
MSVOA_X
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Tgt Ion: 98 Resp: 33230
Ion Ratio Lower Upper
98 100
100 65.8 53.6 80.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

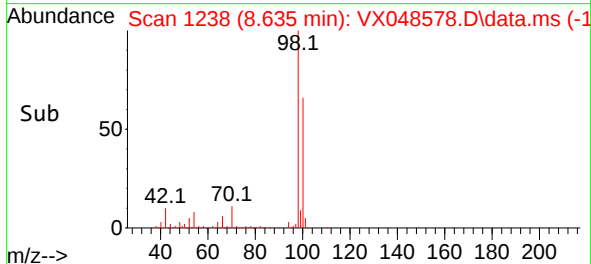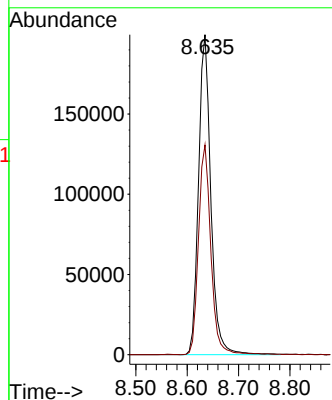

#51
4-Methyl-2-Pentanone
Concen: 0.706 ug/l
RT: 8.561 min Scan# 1226
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Tgt Ion: 43 Resp: 2454
Ion Ratio Lower Upper
43 100
58 43.3 32.3 48.5

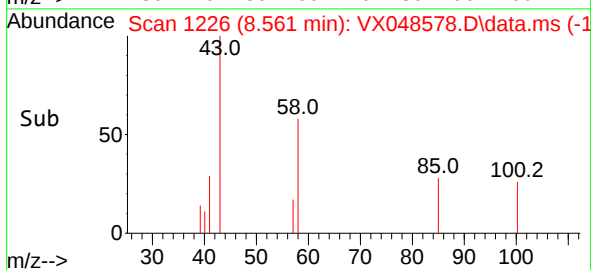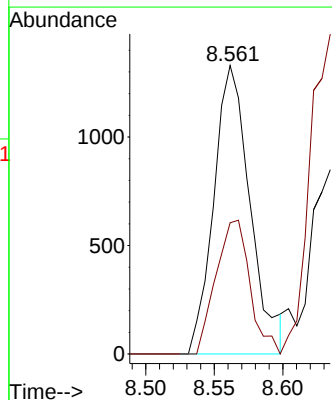

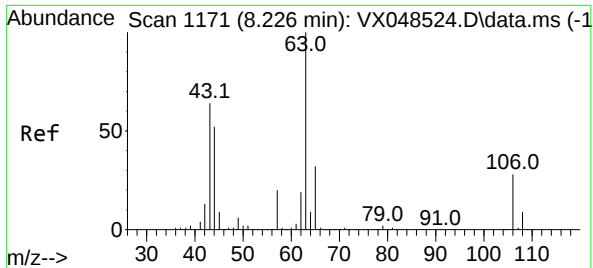





#58
2-Chloroethyl Vinyl ether
Concen: 0.788 ug/l
RT: 8.238 min Scan# 1173
Delta R.T. 0.012 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Instrument : MSVOA_X
ClientSampleId : LOD-MDL-WATER-01-QT3-2025

Tgt Ion: 63 Resp: 1419
Ion Ratio Lower Upper
63 100
106 26.5 23.0 34.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

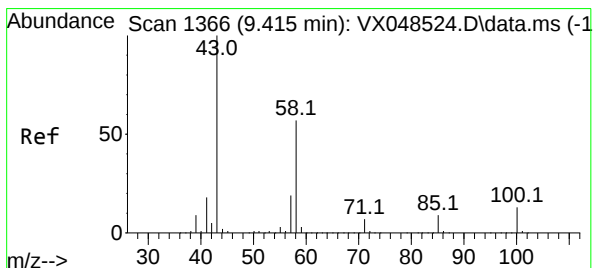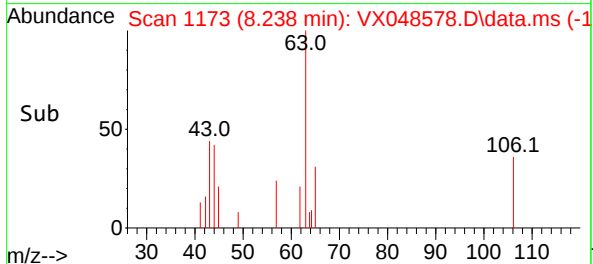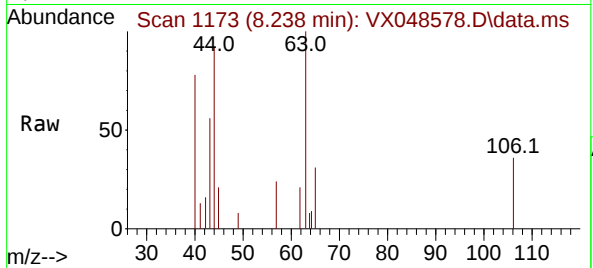

#59
2-Hexanone
Concen: 0.685 ug/l
RT: 9.433 min Scan# 1369
Delta R.T. 0.018 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Tgt Ion: 43 Resp: 1771
Ion Ratio Lower Upper
43 100
58 54.2 28.1 84.2

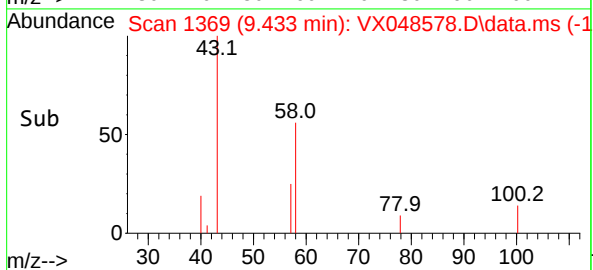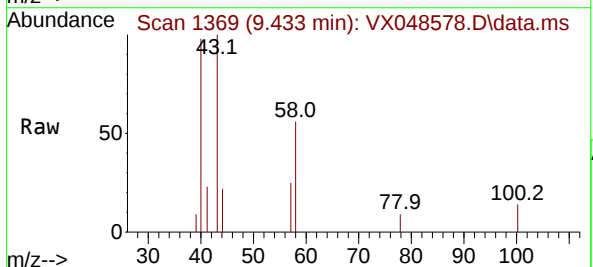



#62

4-Bromofluorobenzene

Concen: 49.236 ug/l

RT: 11.061 min Scan# 1

Delta R.T. -0.000 min

Lab File: VX048578.D

Acq: 12 Nov 2025 15:05

Instrument :

MSVOA_X

ClientSampleId :

LOD-MDL-WATER-01-QT3-2025

Tgt Ion: 95 Resp: 131890

Ion Ratio Lower Upper

95 100

174 81.7 0.0 161.8





176 77.9 0.0 153.6

Manual Integrations

APPROVED

Reviewed By :John Carlone 11/14/2025

Supervised By :Mahesh Dadoda 11/17/2025



#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.037 min Scan# 1468

Delta R.T. -0.000 min

Lab File: VX048578.D

Acq: 12 Nov 2025 15:05




Tgt Ion:117 Resp: 281055


Ion Ratio Lower Upper

117 100

82 55.5 44.4 66.6

119 31.3 25.1 37.7

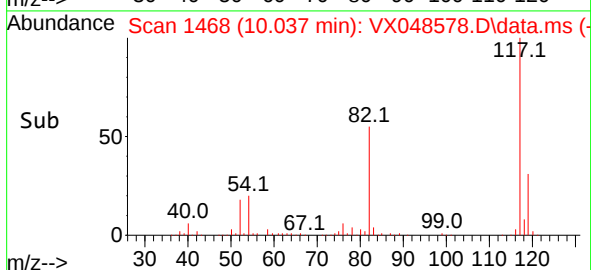







#68
m/p-Xylenes
Concen: 0.286 ug/l
RT: 10.287 min Scan# 1509
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Instrument : MSVOA_X
ClientSampleId : LOD-MDL-WATER-01-QT3-2025

Tgt Ion:106 Resp: 120
Ion Ratio Lower Upper
106 100
91 205.8 159.6 239.4




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

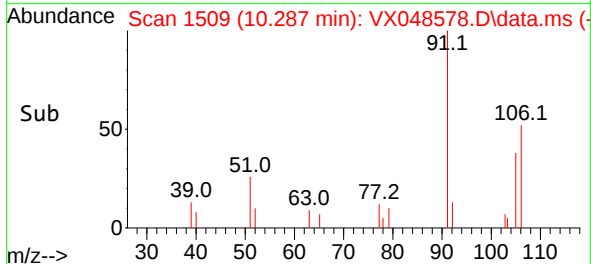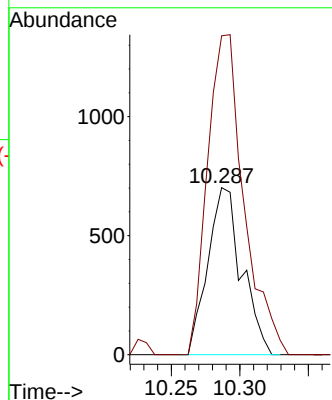

#71
Bromoform
Concen: 0.218 ug/l
RT: 10.787 min Scan# 1591
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion:173 Resp: 449
Ion Ratio Lower Upper
173 100
175 0.0 24.4 73.4#
254 0.0 0.1 0.1#

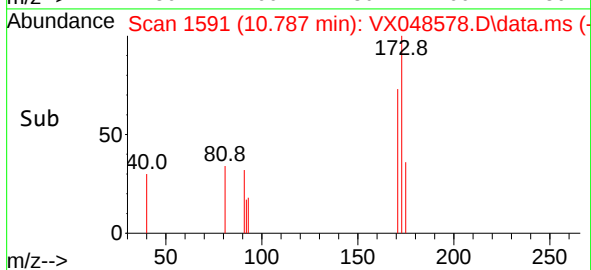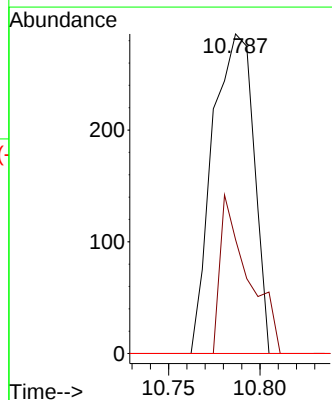



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05




Instrument : MSVOA_X
ClientSampleId : LOD-MDL-WATER-01-QT3-2025



Tgt Ion:152 Resp: 143278
Ion Ratio Lower Upper
152 100
115 56.7 39.2 117.6
150 154.0 0.0 347.0




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

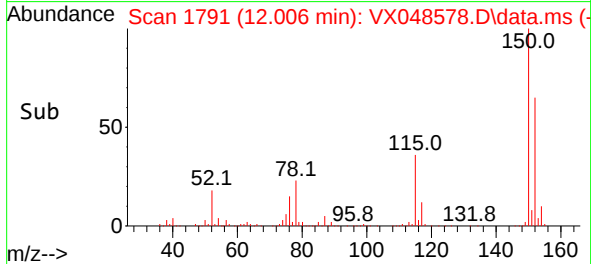

#76
1,2,3-Trichloropropane
Concen: 0.209 ug/l m
RT: 11.220 min Scan# 1662
Delta R.T. -0.000 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Tgt Ion: 75 Resp: 723
Ion Ratio Lower Upper
75 100
77 114.0 24.3 72.8#

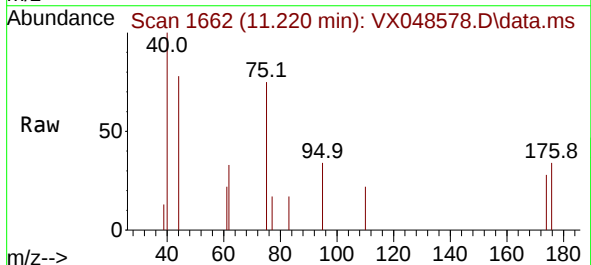







#88
1,4-Dichlorobenzene
Concen: 0.217 ug/l m
RT: 12.018 min Scan# 1793
Delta R.T. -0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05

Instrument : MSVOA_X
ClientSampleId : LOD-MDL-WATER-01-QT3-2025

Tgt Ion:146 Resp: 1128
Ion Ratio Lower Upper
146 100
111 28.7 19.2 57.6
148 33.6 31.9 95.9




Manual Integrations
APPROVED


Reviewed By :John Carlone 11/14/2025
Supervised By :Mahesh Dadoda 11/17/2025

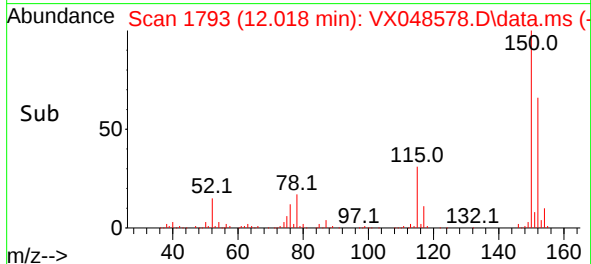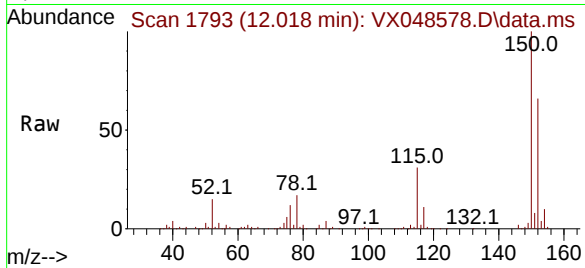

#89
n-Butylbenzene
Concen: 0.225 ug/l
RT: 12.317 min Scan# 1842
Delta R.T. 0.006 min
Lab File: VX048578.D
Acq: 12 Nov 2025 15:05


Tgt Ion: 91 Resp: 1925
Ion Ratio Lower Upper
91 100
92 40.8 27.2 81.5
134 38.4 13.0 39.0

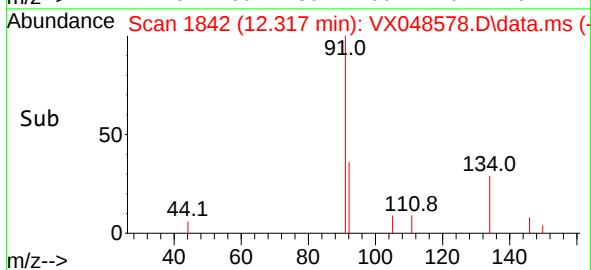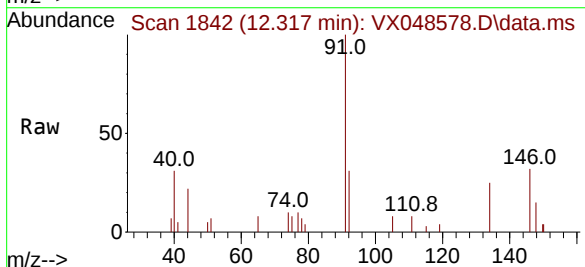

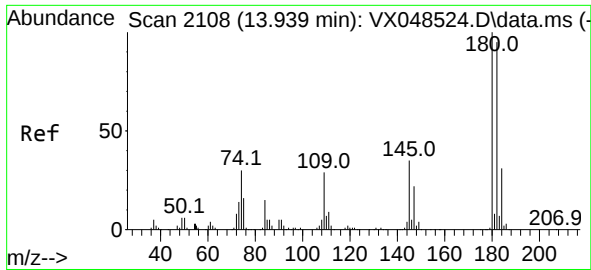

#96
 1,2,3-Trichlorobenzene
 Concen: 0.204 ug/l
 RT: 13.945 min Scan# 2109
 Delta R.T. 0.006 min
 Lab File: VX048578.D
 Acq: 12 Nov 2025 15:05

Instrument : MSVOA_X
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

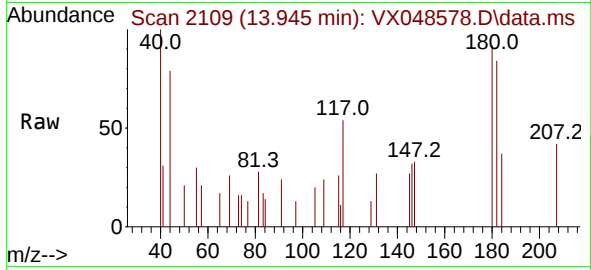

Tgt Ion:180 Resp: 608
 Ion Ratio Lower Upper
 180 100
 182 91.9 47.3 142.0
 145 50.2 16.7 50.0

Manual Integrations
 APPROVED

Reviewed By :John Carlone 11/14/2025
 Supervised By :Mahesh Dadoda 11/17/2025

