
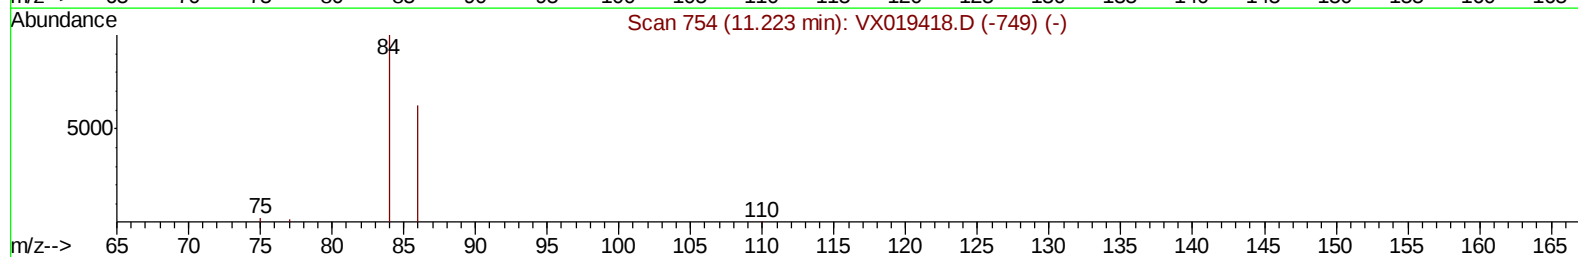
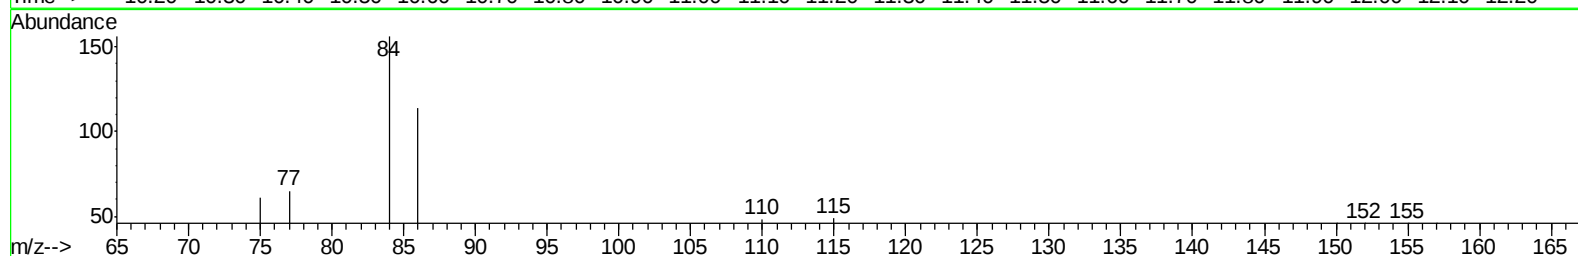


Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX111320\
 Data File : VX019422.D
 Acq On : 13 Nov 2020 12:15
 Operator : JC/MD
 Sample : VSTD0.0503
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Nov 17 04:15:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 17 04:13:39 2020
 Response via : Initial Calibration

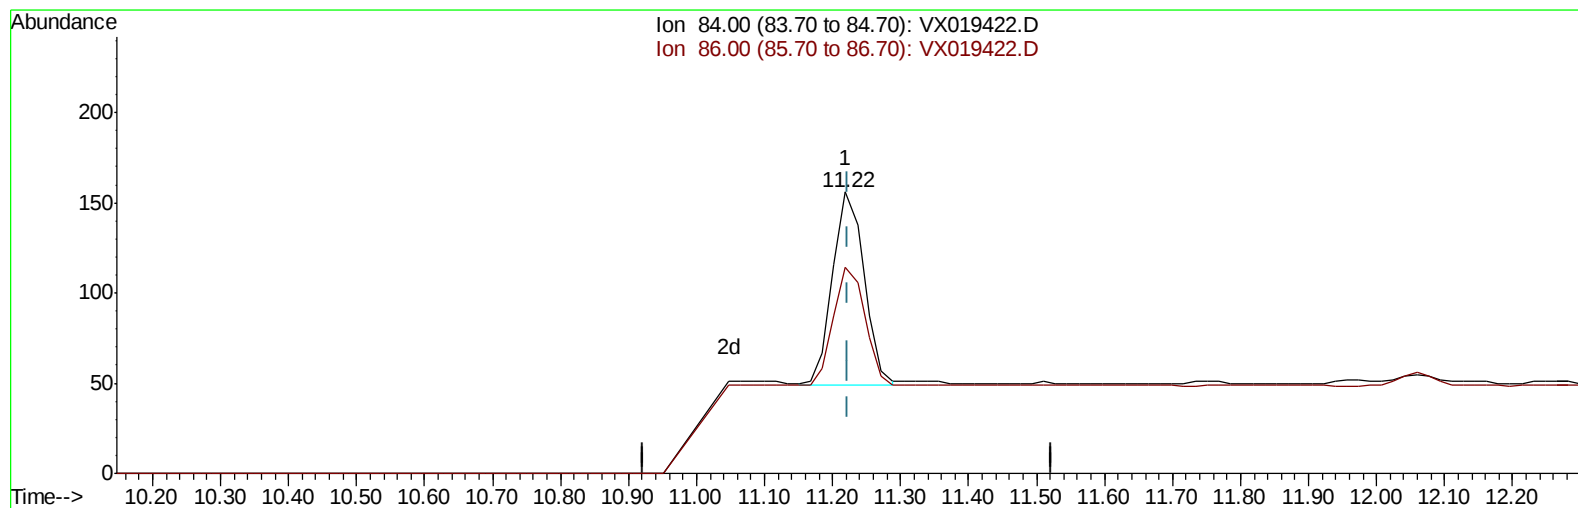

TIC: VX019422.D

(10) 1,1,2,2-Tetrachloroethane-d2 (S)

11.219min (-0.004) 0.04ug/L m

response 340

Ion	Exp%	Act%
84.00	100	100
86.00	65.10	140.29#
0.00	0.00	0.00
0.00	0.00	0.00