

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX111320\
 Data File : VX019418.D
 Acq On : 13 Nov 2020 10:04
 Operator : JC/MD
 Sample : VSTD0.505
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VSTD0.5305

Quant Time: Nov 17 04:15:03 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 17 04:13:39 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.82	114	18135	0.50	ug/L	0.00
5) Chlorobenzene-d5	10.09	117	15969	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	12.06	152	7664	0.50	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.39	65	9835	0.55	ug/L	0.00
4) 1,2-Dichloroethane-d4	6.03	65	7820	0.42	ug/L	0.00
7) 1,2-Dichloropropane-d6	7.37	67	7912	0.58	ug/L	0.00
8) Toluene-d8	8.68	98	20010	0.40	ug/L	0.00
10) 1,1,2,2-Tetrachloroethane-	11.22	84	5779	0.62	ug/L	0.00
Target Compounds						
3) Vinyl chloride	1.39	62	9028	0.533	ug/L	100
6) Trichloroethene	7.18	95	6962	0.562	ug/L	100
9) 1,2-Dibromoethane	9.66	107	4082	0.562	ug/L	100
12) 1,2,3-Trichloropropane	11.27	75	3935	0.589	ug/L	100
13) 1,2-Dibromo-3-chloropropan	12.97	75	674	0.579	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX111320\
Data File : VX019418.D
Acq On : 13 Nov 2020 10:04
Operator : JC/MD
Sample : VSTD0.505
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VSTD0.5305

Quant Time: Nov 17 04:15:03 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 17 04:13:39 2020
Response via : Initial Calibration

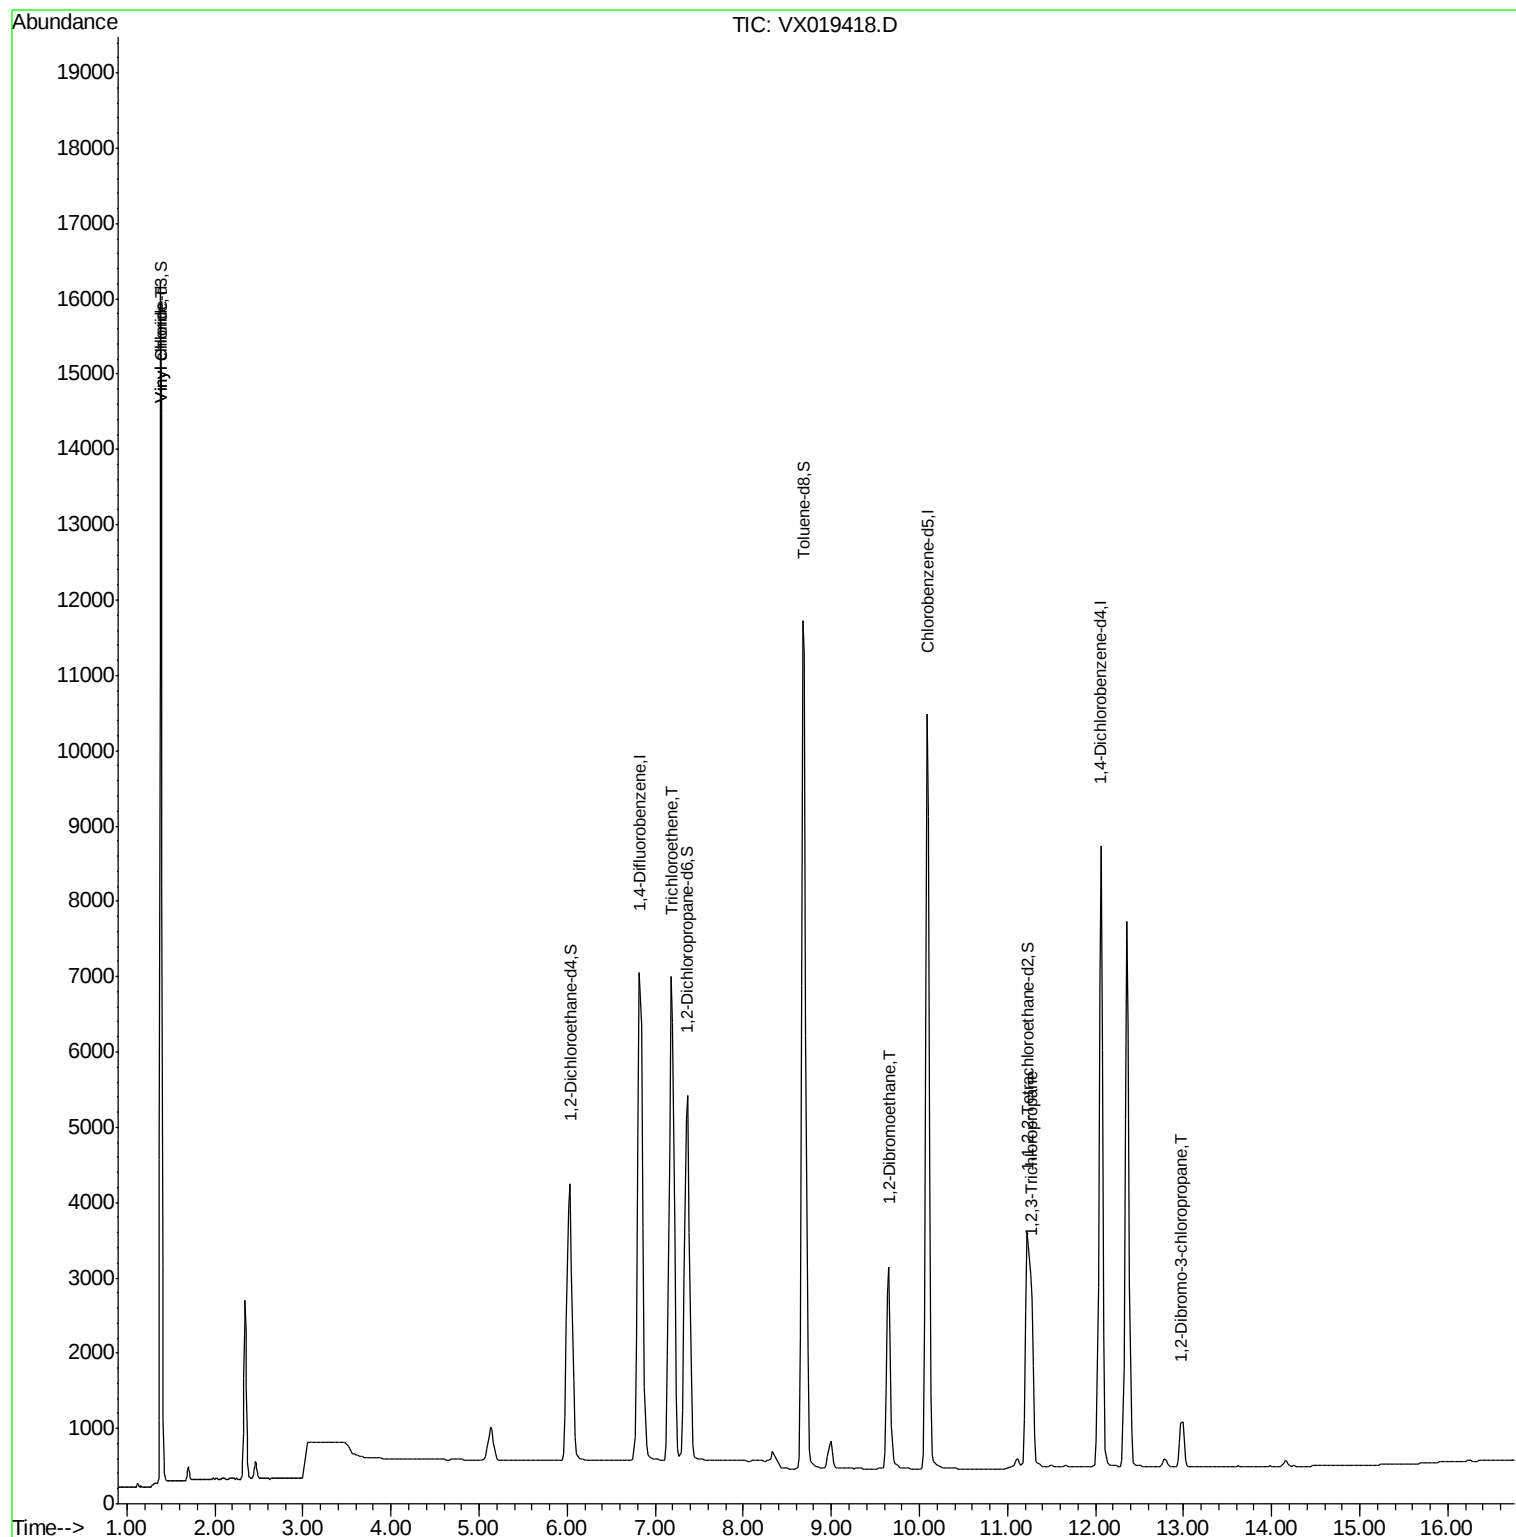

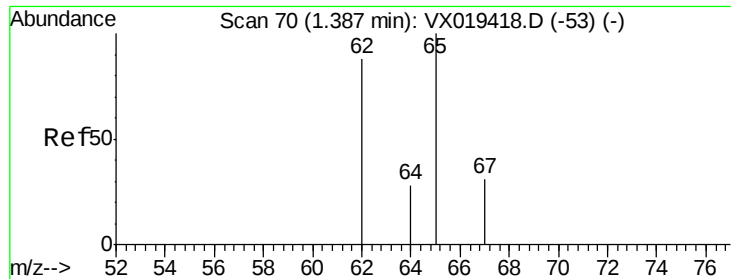

#3

Vinyl chloride

Concen: 0.533 ug/L

RT: 1.39 min Scan# 70

Delta R.T. 0.00 min

Lab File: VX019418.D

Acq: 13 Nov 2020 10:04

Instrument :

MSVOA_X

ClientSampleId :





VSTD0.5305

Tot Ion: 62 Resp: 9028

Ion Ratio Lower Upper

62 100

64 32.1 22.5 41.7

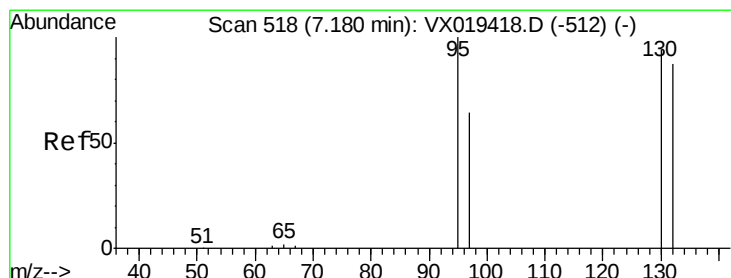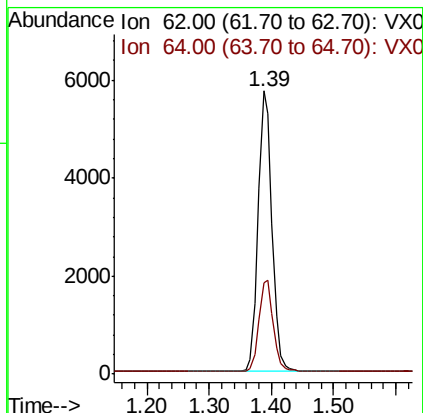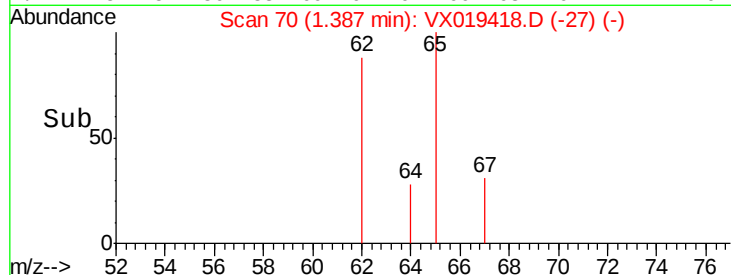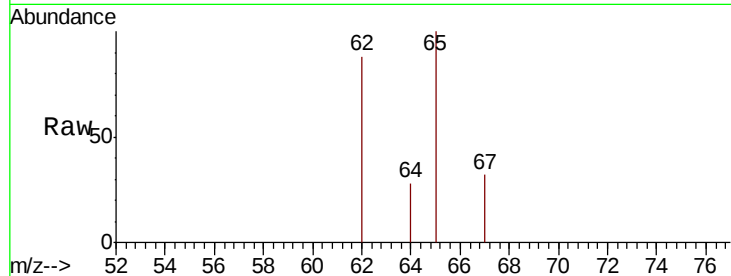

#6

Trichloroethene

Concen: 0.562 ug/L

RT: 7.18 min Scan# 518

Delta R.T. 0.00 min

Lab File: VX019418.D

Acq: 13 Nov 2020 10:04

Tgt Ion: 95 Resp: 6962




Ion Ratio Lower Upper


95 100

97 64.6 45.2 84.0

132 87.2 61.0 113.4

130 93.7 65.6 121.8

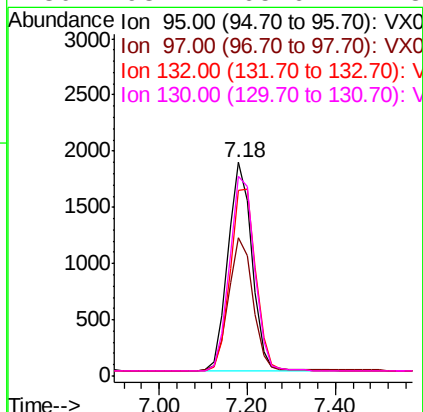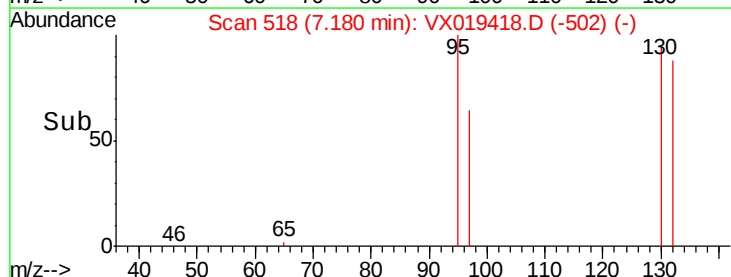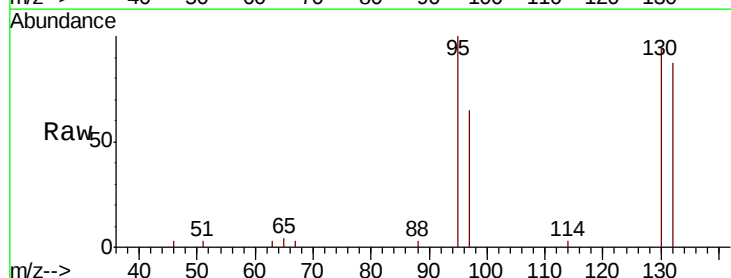

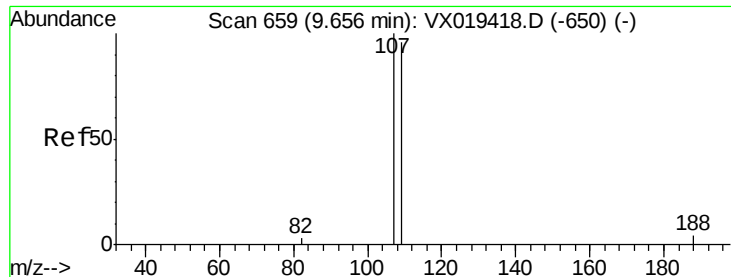

#9

1,2-Dibromoethane

Concen: 0.562 ug/L

RT: 9.66 min Scan# 659

Delta R.T. 0.00 min

Lab File: VX019418.D

Acq: 13 Nov 2020 10:04

Instrument :

MSVOA_X

ClientSampleId :

VSTD0.5305


Tot Ion:107 Resp: 4082

Ion Ratio Lower Upper

107 100

109 96.4 67.5 125.3




188 6.9 5.5 8.3

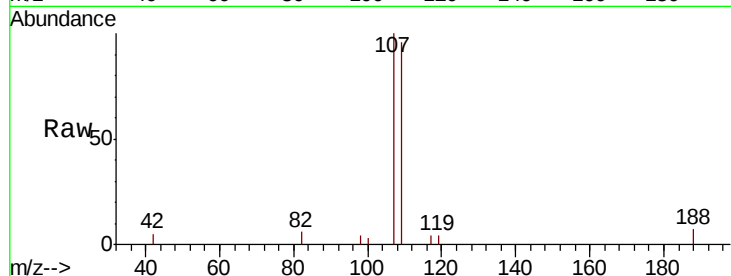

Abundance Ion 107.00 (106.70 to 107.70): V

Ion 109.00 (108.70 to 109.70): V

Ion 188.00 (187.70 to 188.70): V

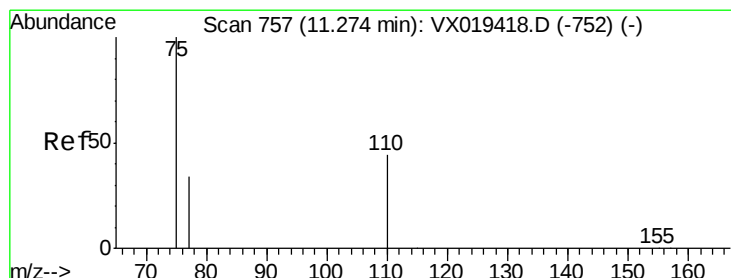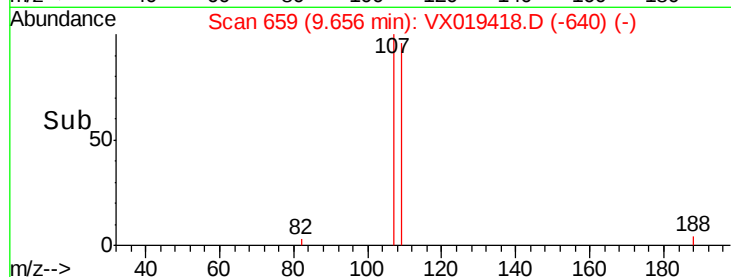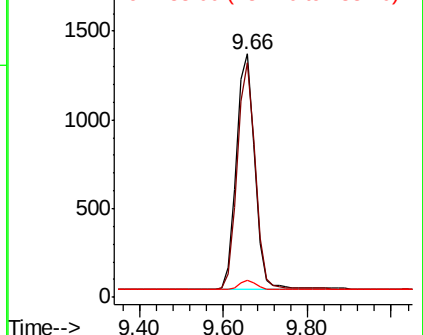

#12

1,2,3-Trichloropropane

Concen: 0.589 ug/L

RT: 11.27 min Scan# 757

Delta R.T. 0.00 min

Lab File: VX019418.D

Acq: 13 Nov 2020 10:04


Tgt Ion: 75 Resp: 3935

Ion Ratio Lower Upper

75 100

110 41.2 33.0 49.4



77 33.2 26.6 39.8

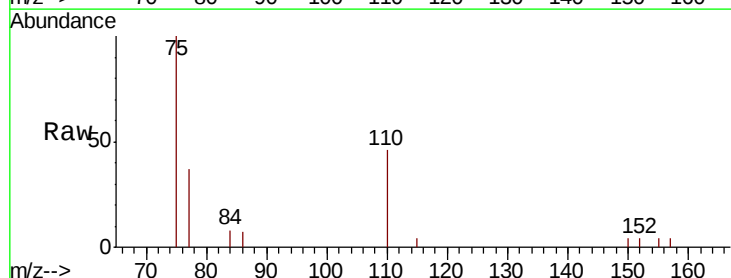


Abundance Ion 75.00 (74.70 to 75.70): VX0

Ion 110.00 (109.70 to 110.70): V

Ion 77.00 (76.70 to 77.70): VX0

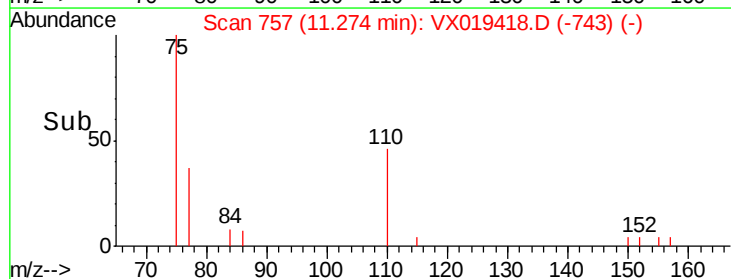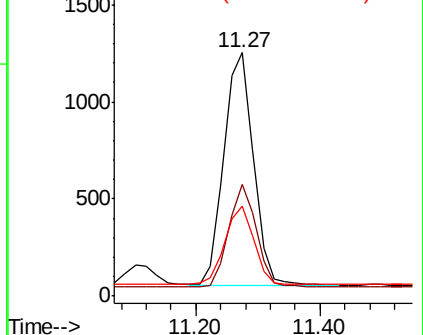

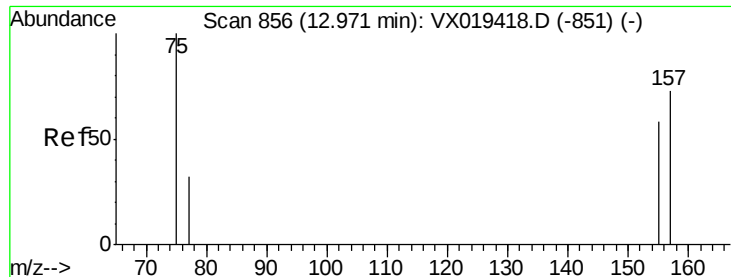

#13

1,2-Dibromo-3-chloropropane

Concen: 0.579 ug/L

RT: 12.97 min Scan# 856

Delta R.T. 0.00 min

Lab File: VX019418.D

Acq: 13 Nov 2020 10:04

Instrument :

MSVOA_X

ClientSampleId :

VSTD0.5305

Tot Ion: 75 Resp: 674

Ion Ratio Lower Upper

75 100

157 74.5 59.6 89.4

155 63.3 50.6 76.0

