


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX111320\
 Data File : VX019415.D
 Acq On : 13 Nov 2020 08:45
 Operator : JC/MD
 Sample : BFB03
 Misc : 25.0mL/MSVOA X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB303

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 17 04:26:19 2020

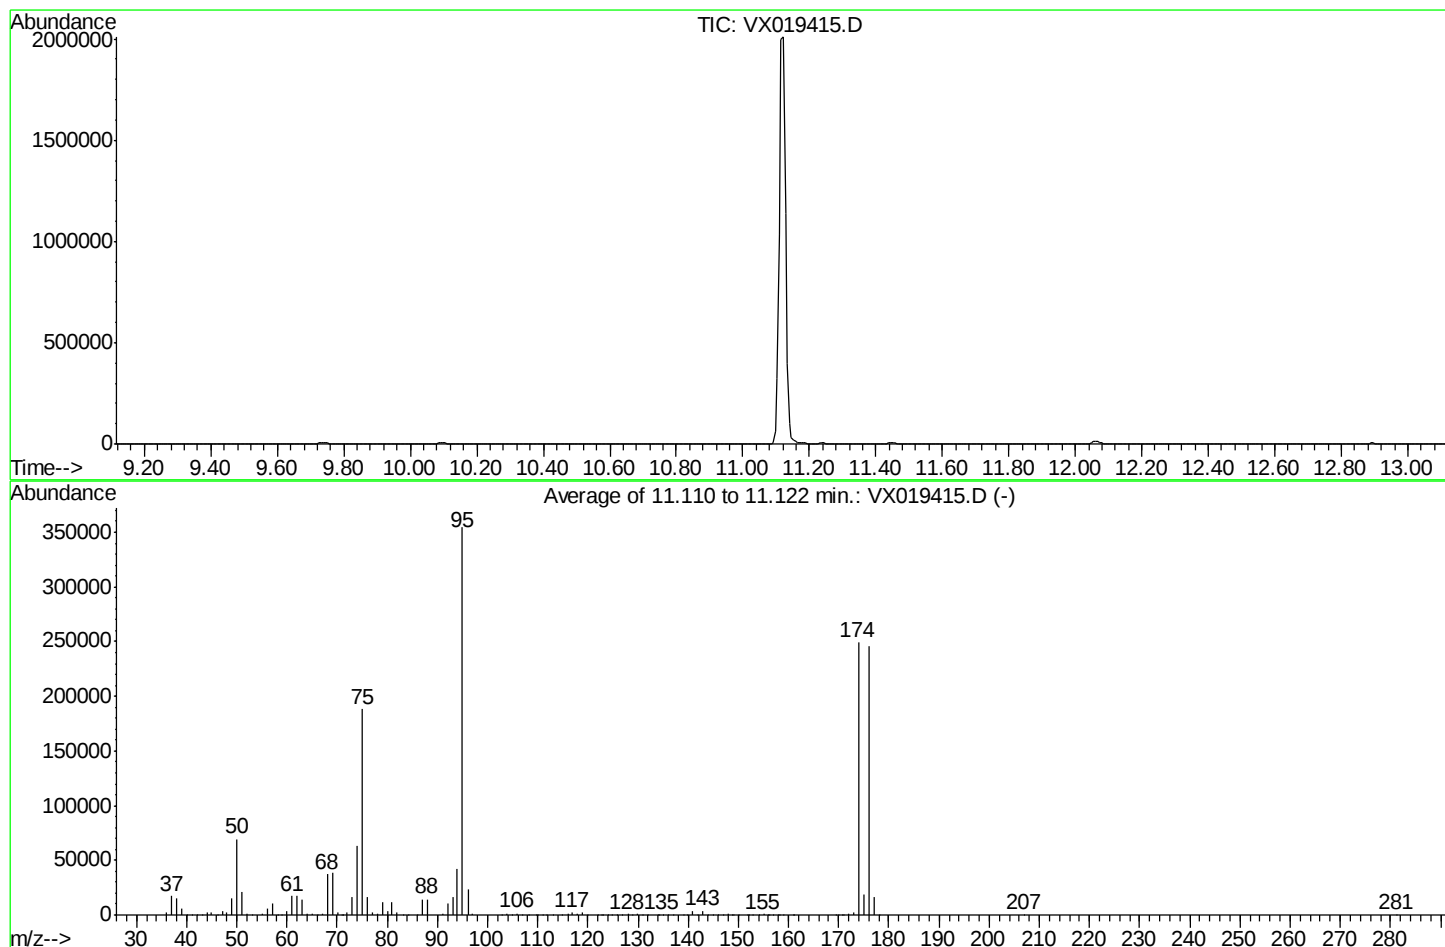

AutoFind: Scans 1644, 1645, 1646; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	69389	PASS
75	95	30	80	53.1	188242	PASS
95	95	100	100	100.0	354474	PASS
96	95	5	9	6.8	24014	PASS
173	174	0.00	2	0.9	2190	PASS
174	95	50	120	70.3	249050	PASS
175	174	5	9	7.7	19090	PASS
176	174	95	101	98.9	246314	PASS
177	176	5	9	6.4	15877	PASS

m/z	Abundance
36.00	2160.0
37.00	12552.0
38.00	10822.0
39.10	4437.0
40.10	363.0
41.20	88.0
43.00	179.0
44.10	2125.0
45.00	2225.0
46.00	299.0
47.10	2556.0
48.00	1692.0
49.00	10362.0
50.00	49416.0
51.10	15239.0
52.00	664.0
53.00	195.0
55.00	755.0
56.00	4086.0
57.00	7182.0
58.00	373.0
60.00	2239.0
61.00	12396.0
62.10	12257.0
63.00	9603.0
64.00	1071.0
65.00	1569.0
66.00	217.0
67.10	635.0
68.00	24360.0
69.00	26656.0
70.00	1908.0
70.90	81.0
72.00	1281.0
73.00	11238.0
74.00	42432.0
75.00	125048.0
76.00	11749.0
77.00	1413.0
77.90	908.0
78.90	7784.0
80.00	2158.0
80.90	8132.0
81.90	2115.0
83.10	274.0
85.90	371.0
87.00	9550.0
88.00	9071.0
91.00	993.0
92.00	6959.0
93.00	10400.0
94.00	26904.0
95.00	225216.0
96.10	16027.0
97.10	601.0
103.00	130.0
103.90	1044.0
104.90	237.0
105.90	1028.0
107.00	282.0
108.10	72.0
109.70	148.0
110.90	212.0
111.80	195.0
112.90	198.0
115.00	211.0
116.00	694.0
117.00	1552.0
117.90	799.0
118.90	1367.0
122.00	59.0
123.00	54.0
124.00	176.0
124.80	113.0
126.00	109.0
127.10	59.0
128.00	602.0
129.00	328.0
130.00	636.0
131.00	402.0
133.90	98.0
135.00	344.0
135.90	105.0
137.00	380.0
139.00	66.0
140.00	131.0
141.00	2134.0
142.00	242.0
143.00	2111.0
144.00	153.0
145.00	550.0
145.90	231.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303

147.00	160.0
148.00	450.0
148.80	138.0
150.00	135.0
153.00	200.0
154.00	119.0
155.10	453.0
156.20	95.0
157.00	308.0
157.80	68.0
159.00	243.0
160.90	285.0
170.70	94.0
172.10	1315.0
173.10	1036.0
174.00	129488.0
175.00	10391.0
176.00	127040.0
177.00	8103.0
178.10	268.0
207.10	102.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303

m/z	Abundance
36.00	3670.0
37.00	21104.0
38.00	18688.0
39.00	7601.0
40.10	563.0
41.10	75.0
42.20	66.0
43.10	184.0
44.00	3516.0
45.00	3592.0
46.10	429.0
47.00	4919.0
48.00	2794.0
49.00	17800.0
50.00	84808.0
51.10	25344.0
52.10	1081.0
53.10	204.0
55.00	1234.0
56.00	6365.0
57.00	12714.0
58.10	687.0
58.90	91.0
60.00	4098.0
61.00	20752.0
62.00	21640.0
63.00	16560.0
64.00	1989.0
65.10	1785.0
66.10	158.0
67.00	1074.0
68.00	46056.0
69.00	46168.0
70.00	3570.0
71.10	265.0
72.00	2446.0
73.00	19400.0
74.00	75592.0
75.00	227200.0
76.00	19656.0
77.00	2948.0
77.90	1493.0
79.00	13900.0
80.00	4467.0
80.90	14290.0
82.00	3097.0
83.00	287.0
84.20	56.0
86.00	505.0
87.00	17664.0
88.00	17896.0
91.00	1610.0
92.00	13382.0
93.00	19696.0
94.00	49592.0
95.00	427904.0
96.10	29384.0
97.00	852.0
102.90	190.0
104.00	1792.0
104.90	588.0
106.00	1971.0
107.00	456.0
108.10	80.0
109.90	339.0
111.00	427.0
111.90	253.0
113.00	372.0
114.80	361.0
116.00	1589.0
116.90	2733.0
117.90	1611.0
119.00	2251.0
119.90	85.0
122.00	169.0
122.70	89.0
123.90	299.0
124.80	96.0
125.80	147.0
126.90	151.0
128.00	1570.0
128.90	772.0
129.90	1313.0
131.00	514.0
131.90	137.0
133.90	188.0
134.90	695.0
135.90	173.0
137.00	735.0
139.10	132.0
139.90	249.0
141.00	4176.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303

141.90	512.0
143.00	4579.0
143.90	309.0
145.00	692.0
146.00	555.0
146.80	303.0
147.80	787.0
149.00	291.0
150.00	374.0
151.70	106.0
152.10	115.0
153.00	274.0
154.00	290.0
155.00	1049.0
155.80	224.0
156.90	558.0
157.90	110.0
158.90	405.0
161.10	337.0
169.30	55.0
171.00	300.0
172.00	2189.0
173.00	2457.0
174.00	285056.0
175.00	21904.0
176.00	282304.0
177.00	18632.0
178.00	574.0
207.00	227.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303

m/z	Abundance
36.00	2945.0
37.00	17800.0
38.00	15516.0
39.10	6593.0
40.10	558.0
41.30	63.0
42.10	74.0
42.90	169.0
44.00	2854.0
45.00	3049.0
46.10	295.0
47.10	4422.0
48.00	2350.0
49.00	16215.0
50.00	73944.0
51.00	23016.0
52.10	939.0
53.20	179.0
55.00	1053.0
56.10	5945.0
57.00	10577.0
58.00	374.0
60.00	4012.0
61.00	19200.0
62.00	20040.0
63.10	14970.0
64.10	1641.0
65.00	1382.0
66.00	138.0
67.00	1176.0
68.00	41584.0
69.00	43712.0
70.10	2863.0
71.00	164.0
72.00	2371.0
73.00	19032.0
74.00	71848.0
75.00	212480.0
76.10	18040.0
77.00	2315.0
78.00	1731.0
78.90	13266.0
80.00	4041.0
80.90	13835.0
81.90	2989.0
83.00	374.0
84.20	55.0
85.90	513.0
87.00	16480.0
88.00	16928.0
91.00	1669.0
92.00	12753.0
93.00	18680.0
94.00	49032.0
95.00	410304.0
96.10	26632.0
97.00	757.0
102.80	242.0
103.90	1799.0
104.90	491.0
105.90	1803.0
107.00	493.0
109.90	252.0
110.90	365.0
111.80	379.0
112.90	480.0
115.00	455.0
115.90	1882.0
116.90	2709.0
117.90	1619.0
119.00	2273.0
119.90	108.0
121.90	131.0
122.70	88.0
123.00	94.0
123.90	288.0
124.80	95.0
125.80	189.0
126.80	106.0
127.00	106.0
128.00	1319.0
128.80	609.0
130.00	1380.0
131.00	609.0
132.00	65.0
134.10	67.0
135.00	731.0
135.80	91.0
137.00	723.0
139.00	142.0
139.80	315.0
140.90	4493.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303

142.00	482.0
142.90	4777.0
144.00	285.0
144.90	610.0
145.80	612.0
146.90	301.0
147.90	1077.0
149.00	263.0
149.90	399.0
151.90	234.0
152.90	365.0
154.00	316.0
154.90	1075.0
156.00	193.0
157.10	754.0
158.10	151.0
159.00	500.0
160.90	433.0
169.30	62.0
169.90	89.0
170.60	140.0
172.00	1891.0
173.00	3077.0
174.00	332608.0
175.00	24976.0
176.00	329600.0
177.00	20896.0
178.10	576.0
207.10	139.0
281.20	80.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303

Scan 1637 (11.067 min): VX019415.D
BFB03

m/z	Abundance
39.90	276.0
41.10	63.0
43.00	77.0
44.00	738.0
207.10	133.0
280.90	54.0

Instrument :
MSVOA_X
ClientSampleId :
BFB303