

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111323\
 Data File : VX038782.D
 Acq On : 13 Nov 2023 15:30
 Operator : JC/MD
 Sample : 05350-10DL 50X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE115D2-20231107DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M

Title : SW846 8260

Signal : TIC: VX038782.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	198	204	210	rBV4	12451	24003	1.61%	0.287%
2	4.550	560	568	581	rBV2	5517	18863	1.27%	0.226%
3	5.385	694	705	721	rBV2	163962	479360	32.17%	5.738%
4	5.550	721	732	751	rVV	262269	744376	49.95%	8.910%
5	5.958	787	799	815	rBV	154266	412895	27.71%	4.942%
6	6.763	921	931	948	rBV	393533	967929	64.95%	11.586%
7	7.129	982	991	1009	rBV	201386	457137	30.68%	5.472%
8	8.647	1233	1240	1262	rBV	853812	1355694	90.98%	16.227%
9	10.055	1465	1471	1491	rBV	931159	1305992	87.64%	15.632%
10	11.079	1634	1639	1656	rBV	836054	1098105	73.69%	13.144%
11	12.018	1788	1793	1815	rBV	1144636	1490156	100.00%	17.837%




Sum of corrected areas: 8354510

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111323\
Data File : VX038782.D
Acq On : 13 Nov 2023 15:30
Operator : JC/MD
Sample : 05350-10DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE115D2-20231107DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

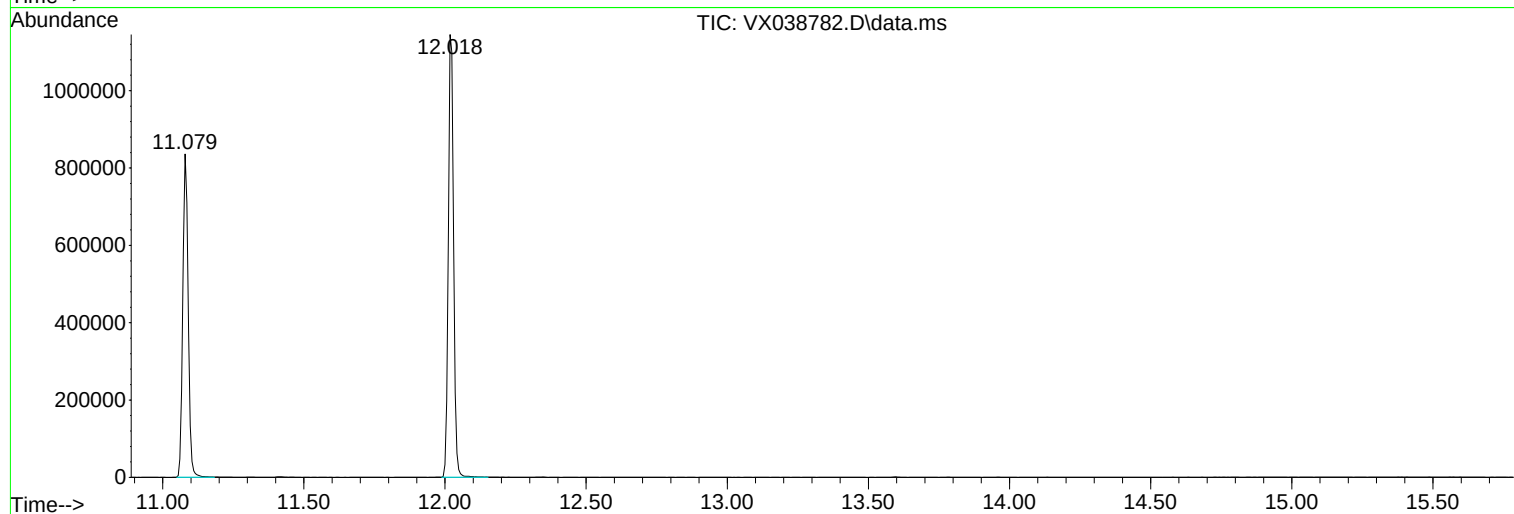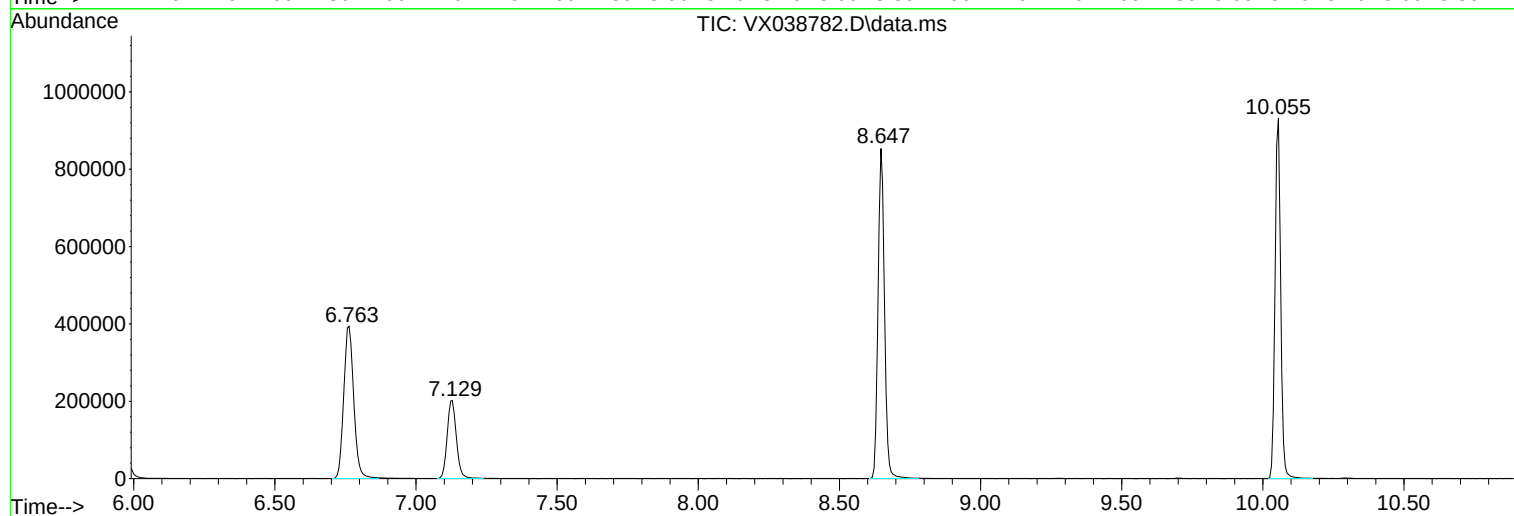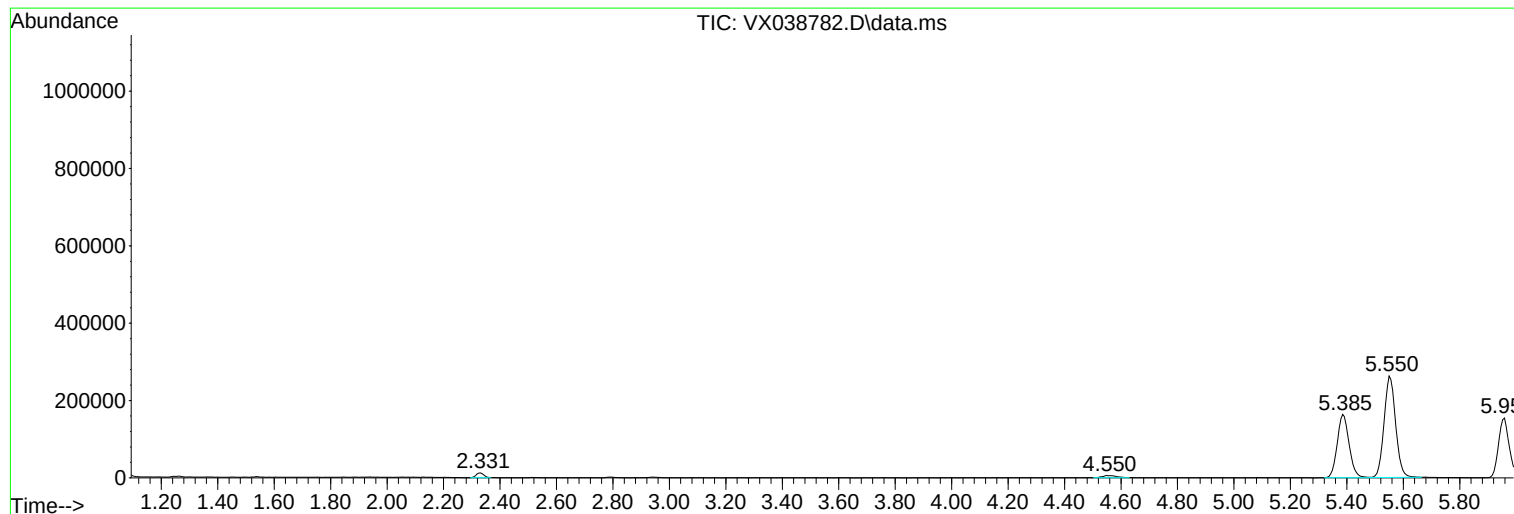

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111323\
Data File : VX038782.D
Acq On : 13 Nov 2023 15:30
Operator : JC/MD
Sample : 05350-10DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE115D2-20231107DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111323\
Data File : VX038782.D
Acq On : 13 Nov 2023 15:30
Operator : JC/MD
Sample : 05350-10DL 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE115D2-20231107DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110723W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------