

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043833.D
 Acq On : 13 Nov 2024 15:06
 Operator : JC/MD
 Sample : P4785-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L9

Quant Time: Nov 14 04:29:58 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Nov 13 02:04:29 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		6.757	114	262358	50.000	ug/L	0.00
28) Chlorobenzene-d5		10.049	117	222437	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		12.018	152	100267	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		1.368	65	74612	53.383	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	= 106.760%		
7) Chloroethane-d5		1.642	69	47255	78.656	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	= 157.320%#		
11) 1,1-Dichloroethene-d2		2.294	65	34023	52.731	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 105.460%		
21) 2-Butanone-d5		4.465	46	80967	88.476	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	= 88.480%		
24) Chloroform-d		5.056	84	148535	49.297	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 98.600%		
26) 1,2-Dichloroethane-d4		5.946	65	96637	50.487	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 100.980%		
32) Benzene-d6		5.964	84	303558	52.784	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	= 105.560%		
36) 1,2-Dichloropropane-d6		7.306	67	85225	48.710	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	= 97.420%		
41) Toluene-d8		8.647	98	270907	51.856	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 103.720%		
43) trans-1,3-Dichloroprop...		8.952	79	39513	47.223	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	= 94.440%		
47) 2-Hexanone-d5		9.384	63	63646	91.918	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	= 91.920%		
56) 1,1,2,2-Tetrachloroeth...		11.189	84	115788	51.579	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	= 103.160%		
66) 1,2-Dichlorobenzene-d4		12.317	152	101243	58.278	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	= 116.560%		
Target Compounds							Qvalue
13) Acetone		2.386	43	11374	13.363	ug/L	95
15) Methyl Acetate		2.715	43	1539	0.855	ug/L #	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043833.D
Acq On : 13 Nov 2024 15:06
Operator : JC/MD
Sample : P4785-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L9

Quant Time: Nov 14 04:29:58 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Nov 13 02:04:29 2024
Response via : Initial Calibration

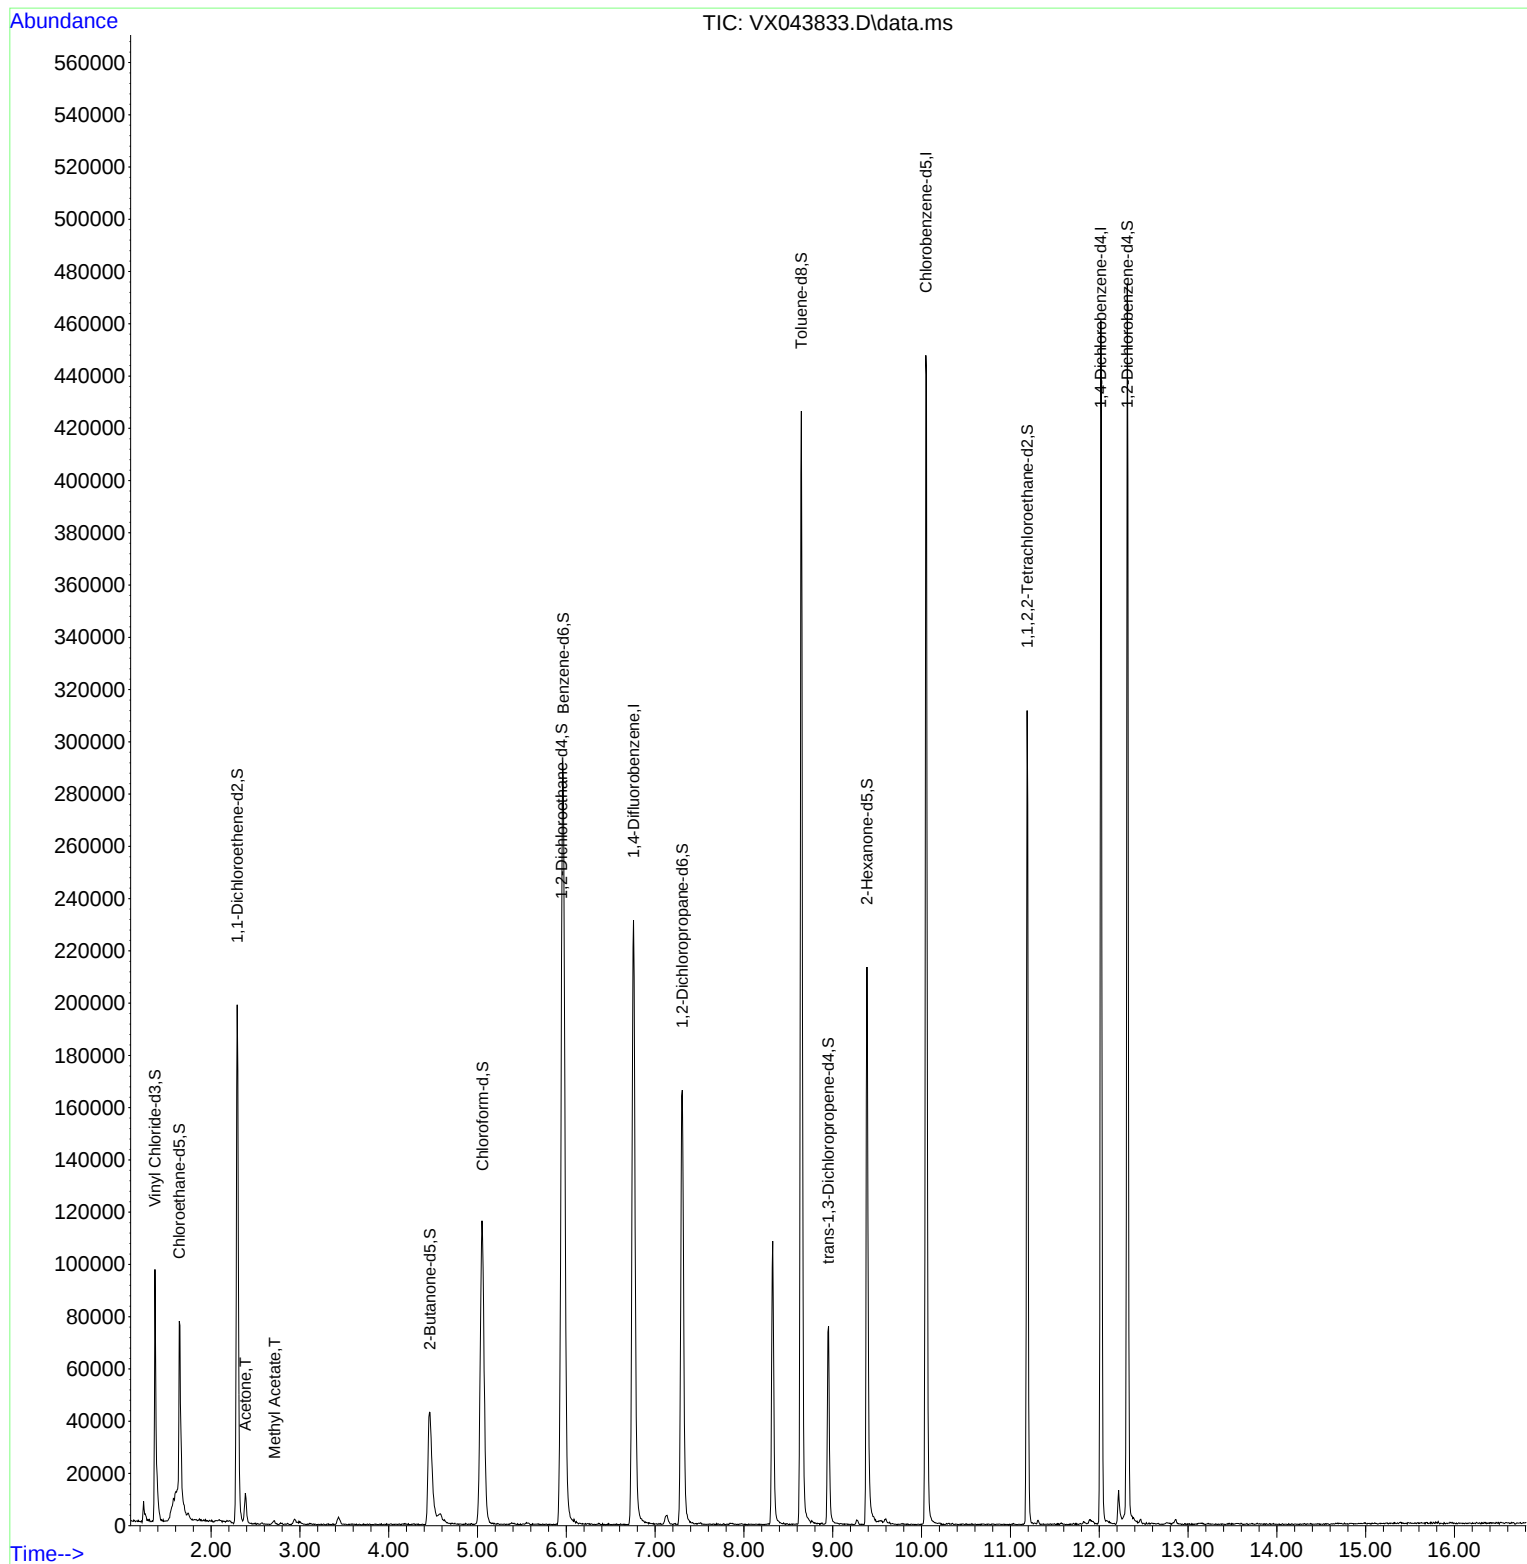

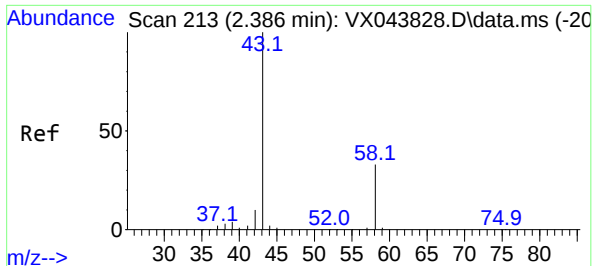

#13

Acetone

Concen: 13.363 ug/L

RT: 2.386 min Scan# 21

Delta R.T. 0.000 min

Lab File: VX043833.D

Acq: 13 Nov 2024 15:06

Instrument :

MSVOA_X

ClientSampleId :





E27L9

Tgt Ion: 43 Resp: 11374

Ion Ratio Lower Upper

43 100

58 34.8 0.0 63.6

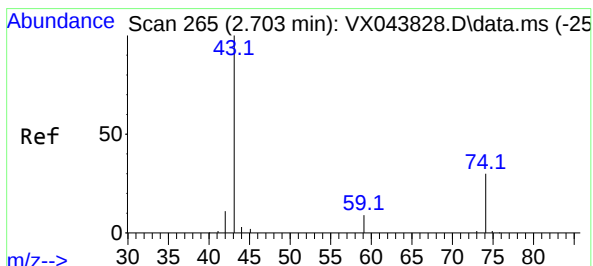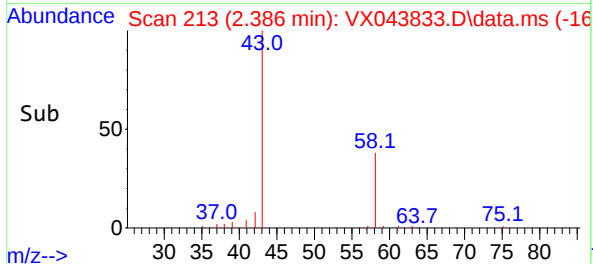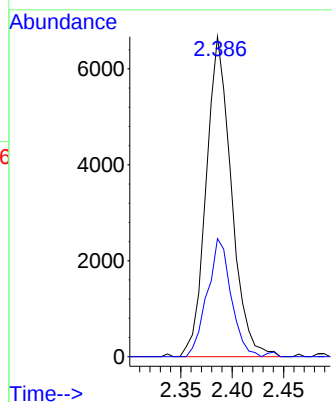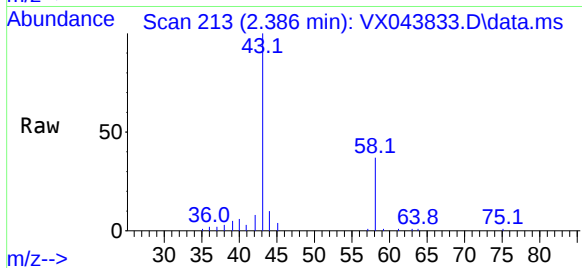

#15

Methyl Acetate

Concen: 0.855 ug/L

RT: 2.715 min Scan# 267

Delta R.T. 0.012 min

Lab File: VX043833.D

Acq: 13 Nov 2024 15:06

Tgt Ion: 43 Resp: 1539

Ion Ratio Lower Upper

43 100

74 32.4 18.9 28.3#

