

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043830.D
 Acq On : 13 Nov 2024 12:21
 Operator : JC/MD
 Sample : VX1113WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043830.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	33	rBV2	5324	8205	1.14%	0.140%
2	1.368	43	46	57	rVB	58036	76657	10.64%	1.307%
3	1.648	89	92	104	rVB	55505	85792	11.90%	1.463%
4	2.294	192	198	211	rVV	139583	219382	30.44%	3.740%
5	2.386	211	213	217	rVB3	874	1003	0.14%	0.017%
6	2.489	228	230	231	rBV2	819	668	0.09%	0.011%
7	2.782	275	278	283	rBV3	1035	1574	0.22%	0.027%
8	2.947	296	305	314	rVB2	4358	10595	1.47%	0.181%
9	3.075	324	326	327	rBV	523	419	0.06%	0.007%
10	3.166	339	341	343	rVB2	313	314	0.04%	0.005%
11	3.239	351	353	356	rVV2	365	374	0.05%	0.006%
12	3.312	363	365	368	rBV2	297	316	0.04%	0.005%
13	3.434	379	385	393	rBV4	3416	7701	1.07%	0.131%
14	3.690	425	427	431	rBV2	354	391	0.05%	0.007%
15	3.800	443	445	447	rVV	320	302	0.04%	0.005%
16	4.111	494	496	499	rVB	438	323	0.04%	0.006%
17	4.190	508	509	514	rVB2	325	312	0.04%	0.005%
18	4.257	519	520	523	rVB	475	370	0.05%	0.006%
19	4.458	546	553	571	rBV	45751	143867	19.96%	2.453%
20	4.654	584	585	587	rVB	801	323	0.04%	0.006%
21	4.733	597	598	604	rVB	522	434	0.06%	0.007%
22	4.794	604	608	610	rBV2	407	393	0.05%	0.007%
23	5.050	638	650	667	rBV	101011	305947	42.45%	5.216%
24	5.251	681	683	685	rBV	286	338	0.05%	0.006%
25	5.367	698	702	705	rBV4	700	1195	0.17%	0.020%
26	5.531	728	729	730	rBV	613	299	0.04%	0.005%
27	5.672	749	752	753	rBV	598	607	0.08%	0.010%
28	5.879	783	786	787	rBV2	296	325	0.05%	0.006%
29	5.964	787	800	817	rBV2	240001	720648	100.00%	12.286%
30	6.214	839	841	844	rVB2	414	441	0.06%	0.008%
31	6.257	844	848	851	rBV2	266	462	0.06%	0.008%
32	6.537	890	894	896	rVB3	269	314	0.04%	0.005%
33	6.604	903	905	909	rVB2	274	299	0.04%	0.005%
34	6.757	921	930	947	rVV	227225	566023	78.54%	9.650%
35	7.129	982	991	999	rVB6	4911	12473	1.73%	0.213%
36	7.232	1006	1008	1011	rVB3	559	492	0.07%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043830.D
 Acq On : 13 Nov 2024 12:21
 Operator : JC/MD
 Sample : VX1113WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

37	7.306	1011	1020	1032	rBV	146298	331142	45.95%	5.646%
38	7.586	1065	1066	1069	rBV2	397	402	0.06%	0.007%
39	7.824	1103	1105	1108	rVB2	419	346	0.05%	0.006%
40	7.958	1125	1127	1133	rVB4	702	813	0.11%	0.014%
41	8.324	1180	1187	1208	rBV	95320	165052	22.90%	2.814%
42	8.586	1226	1230	1231	rBV2	667	560	0.08%	0.010%
43	8.647	1233	1240	1254	rBV	343175	560225	77.74%	9.551%
44	8.952	1285	1290	1299	rBV	64155	103713	14.39%	1.768%
45	9.159	1322	1324	1325	rBV2	364	320	0.04%	0.005%
46	9.208	1330	1332	1333	rBV	422	287	0.04%	0.005%
47	9.275	1339	1343	1349	rVB6	1747	2825	0.39%	0.048%
48	9.384	1356	1361	1377	rBV	215855	328213	45.54%	5.596%
49	9.616	1394	1399	1404	rVB5	678	1335	0.19%	0.023%
50	9.695	1408	1412	1420	rVV3	1051	1969	0.27%	0.034%
51	9.769	1422	1424	1429	rVB4	346	465	0.06%	0.008%
52	9.811	1429	1431	1436	rVB2	370	349	0.05%	0.006%
53	9.988	1457	1460	1461	rVV	356	298	0.04%	0.005%
54	10.049	1465	1470	1488	rVV	457493	658537	91.38%	11.227%
55	10.195	1491	1494	1501	rVV4	1821	2709	0.38%	0.046%
56	10.256	1502	1504	1508	rVV3	436	614	0.09%	0.010%
57	10.311	1508	1513	1521	rVV5	1523	2943	0.41%	0.050%
58	10.640	1565	1567	1569	rBV2	1333	1604	0.22%	0.027%
59	10.811	1593	1595	1598	rVB3	384	338	0.05%	0.006%
60	10.915	1611	1612	1615	rBV2	370	351	0.05%	0.006%
61	10.963	1615	1620	1623	rBV3	1196	1967	0.27%	0.034%
62	11.189	1652	1657	1671	rBV	316357	394115	54.69%	6.719%
63	11.311	1675	1677	1681	rVB3	445	607	0.08%	0.010%
64	11.457	1697	1701	1705	rVB3	1432	1863	0.26%	0.032%
65	11.524	1709	1712	1714	rBV	410	440	0.06%	0.008%
66	11.561	1717	1718	1721	rVB2	425	294	0.04%	0.005%
67	11.604	1721	1725	1726	rBV2	351	468	0.06%	0.008%
68	11.750	1746	1749	1756	rBV3	1614	2507	0.35%	0.043%
69	11.975	1779	1786	1788	rBV2	1889	2801	0.39%	0.048%
70	12.018	1788	1793	1802	rBV	453624	583069	80.91%	9.941%
71	12.317	1837	1842	1852	rVV	412647	521245	72.33%	8.887%
72	12.646	1893	1896	1898	rBV2	241	286	0.04%	0.005%
73	12.689	1901	1903	1906	rBV2	295	351	0.05%	0.006%
74	12.762	1912	1915	1918	rVV3	762	838	0.12%	0.014%
75	12.811	1922	1923	1926	rBV	313	312	0.04%	0.005%
76	12.914	1935	1940	1941	rBV2	419	504	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043830.D
 Acq On : 13 Nov 2024 12:21
 Operator : JC/MD
 Sample : VX1113WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK726

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	13.122	1969	1974	1977	rBV4	1212	1840	0.26%	0.031%
78	13.158	1977	1980	1983	rVV2	398	525	0.07%	0.009%
79	13.567	2043	2047	2048	rVB	305	322	0.04%	0.005%
80	13.597	2048	2052	2057	rBV3	1131	1706	0.24%	0.029%
81	13.737	2072	2075	2078	rVB3	367	503	0.07%	0.009%
82	13.786	2078	2083	2089	rBV5	1855	3097	0.43%	0.053%
83	13.890	2096	2100	2101	rVB	310	395	0.05%	0.007%
84	13.969	2108	2113	2117	rBV3	1127	1969	0.27%	0.034%
85	14.121	2136	2138	2143	rVB3	1257	1842	0.26%	0.031%
86	14.243	2156	2158	2161	rVB	413	348	0.05%	0.006%
87	14.292	2163	2166	2169	rBV2	408	502	0.07%	0.009%
88	14.768	2242	2244	2246	rBV2	408	354	0.05%	0.006%
89	15.005	2280	2283	2284	rVB3	543	474	0.07%	0.008%
90	15.024	2284	2286	2288	rVB2	453	308	0.04%	0.005%
91	15.079	2294	2295	2300	rBV2	565	596	0.08%	0.010%
92	15.524	2366	2368	2372	rVB4	677	670	0.09%	0.011%
93	15.560	2372	2374	2377	rBV2	508	606	0.08%	0.010%
94	15.603	2380	2381	2383	rBV	578	402	0.06%	0.007%
95	15.645	2387	2388	2391	rBV3	683	572	0.08%	0.010%
96	15.688	2393	2395	2398	rVV2	450	393	0.05%	0.007%
97	15.822	2415	2417	2419	rBV2	660	472	0.07%	0.008%
98	15.926	2432	2434	2435	rBV	479	317	0.04%	0.005%
99	16.273	2489	2491	2492	rBV2	565	354	0.05%	0.006%
100	16.584	2541	2542	2544	rBV2	516	299	0.04%	0.005%




Sum of corrected areas: 5865521

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043830.D
Acq On : 13 Nov 2024 12:21
Operator : JC/MD
Sample : VX1113WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK726

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

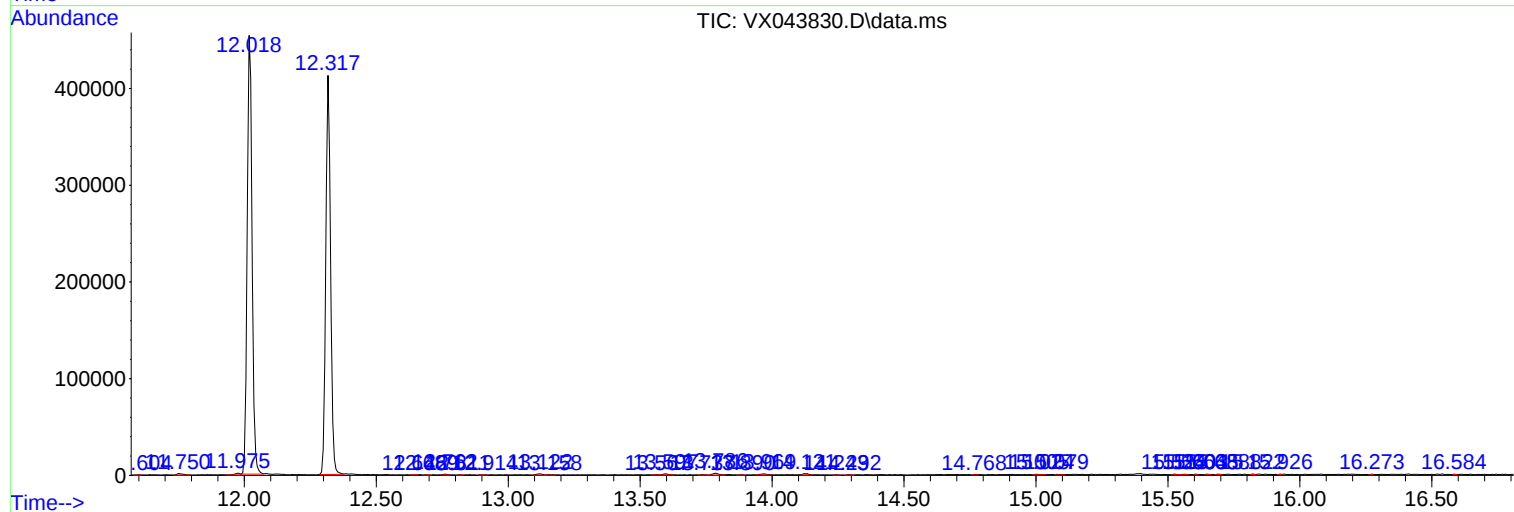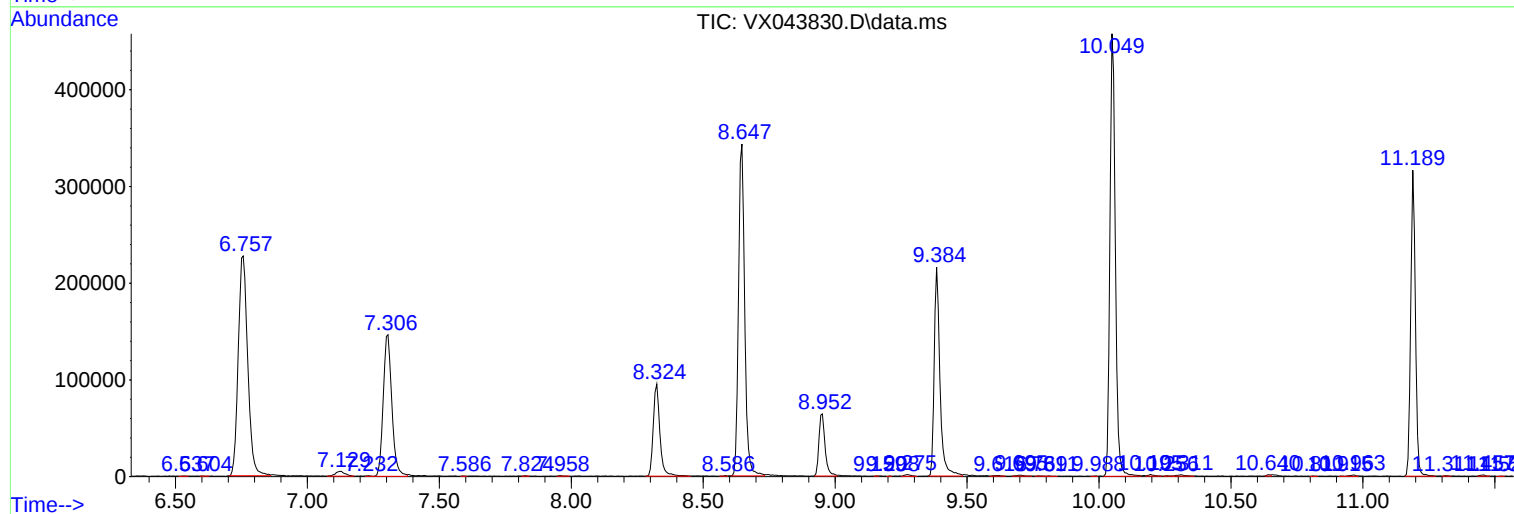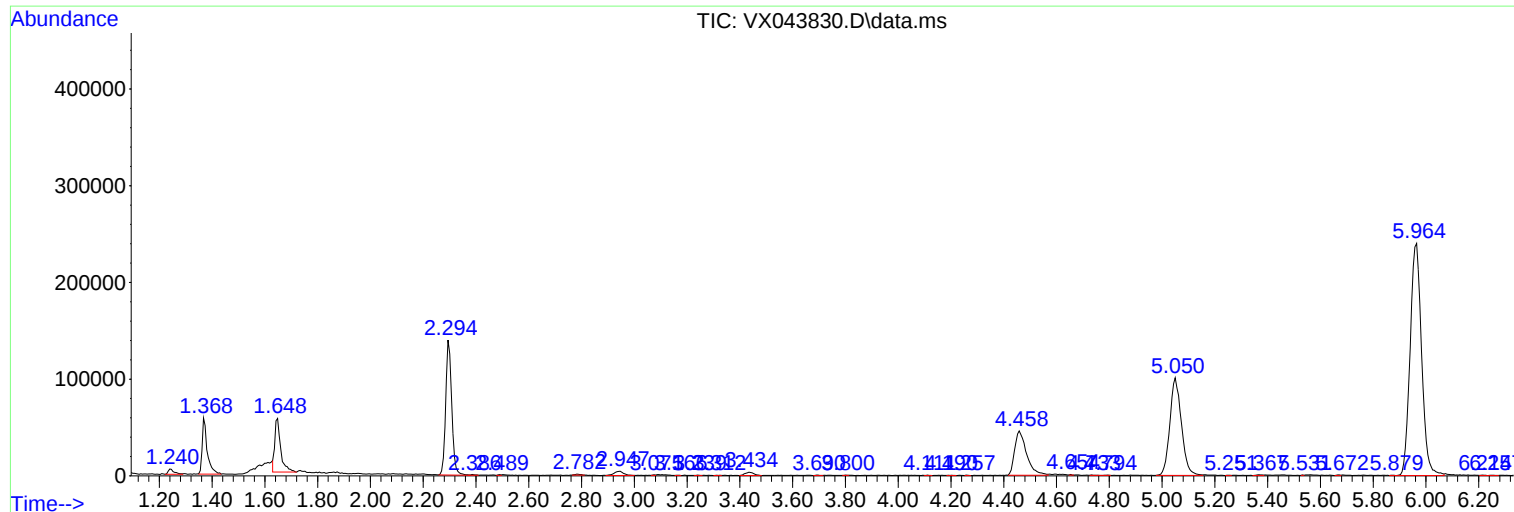

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043830.D
Acq On : 13 Nov 2024 12:21
Operator : JC/MD
Sample : VX1113WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK726

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043830.D
Acq On : 13 Nov 2024 12:21
Operator : JC/MD
Sample : VX1113WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK726

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc