

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043840.D
 Acq On : 13 Nov 2024 17:48
 Operator : JC/MD
 Sample : P4785-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043840.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.142	6	9	13	rVB	2824	2501	0.00%	0.001%
2	1.239	21	25	28	rBV	11424	13763	0.00%	0.004%
3	1.374	42	47	61	rBV2	373491	487614	0.17%	0.150%
4	1.617	71	87	88	rBV4	11585	39219	0.01%	0.012%
5	1.642	88	91	102	rVB	86260	120240	0.04%	0.037%
6	1.904	131	134	137	rBV3	1500	1984	0.00%	0.001%
7	2.099	161	166	168	rBV	9427	14429	0.00%	0.004%
8	2.130	168	171	179	rVB3	21003	37999	0.01%	0.012%
9	2.306	192	200	231	rBV2	566672	1176665	0.40%	0.361%
10	2.569	239	243	245	rBV3	427	458	0.00%	0.000%
11	2.648	251	256	261	rVB3	838	1676	0.00%	0.001%
12	2.782	273	278	288	rBV	5691	11347	0.00%	0.003%
13	2.934	299	303	305	rBV2	730	1083	0.00%	0.000%
14	3.001	312	314	316	rVB3	425	406	0.00%	0.000%
15	3.087	320	328	346	rVV	192604	397140	0.14%	0.122%
16	3.257	355	356	359	rVB	532	421	0.00%	0.000%
17	3.434	375	385	386	rBV3	2954	4594	0.00%	0.001%
18	3.605	402	413	432	rBV	317916	813132	0.28%	0.250%
19	3.843	449	452	454	rBV3	354	422	0.00%	0.000%
20	4.300	525	527	532	rVV3	647	561	0.00%	0.000%
21	4.483	541	557	593	rBV	7111486	21093432	7.20%	6.480%
22	5.056	639	651	667	rBV2	102379	331528	0.11%	0.102%
23	5.172	668	670	673	rVB3	987	900	0.00%	0.000%
24	5.385	690	705	727	rBV	399655	1397672	0.48%	0.429%
25	5.611	740	742	747	rVB2	550	619	0.00%	0.000%
26	5.757	765	766	769	rVB2	575	436	0.00%	0.000%
27	5.976	788	802	829	rBV2	232411	859276	0.29%	0.264%
28	6.379	865	868	870	rBV3	443	519	0.00%	0.000%
29	6.684	910	918	920	rBV2	409	984	0.00%	0.000%
30	6.775	920	933	951	rBV	161034	597633	0.20%	0.184%
31	6.909	954	955	959	rBV3	386	597	0.00%	0.000%
32	7.019	968	973	974	rBV2	274	493	0.00%	0.000%
33	7.190	978	1001	1010	rBV5	42246091	292887636	100.00%	89.981%
34	7.360	1024	1029	1040	rVB	158967	309338	0.11%	0.095%
35	8.208	1166	1168	1169	rBV2	1841	1592	0.00%	0.000%
36	8.330	1182	1188	1201	rVB	108041	182840	0.06%	0.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043840.D
 Acq On : 13 Nov 2024 17:48
 Operator : JC/MD
 Sample : P4785-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	8.580	1225	1229	1234	rBV	18036	28702	0.01%	0.009%
38	8.653	1235	1241	1247	rVV	380349	617656	0.21%	0.190%
39	8.720	1247	1252	1270	rVB	234742	368673	0.13%	0.113%
40	8.952	1285	1290	1301	rBV	86868	127155	0.04%	0.039%
41	9.049	1303	1306	1312	rVB3	4632	6257	0.00%	0.002%
42	9.153	1318	1323	1333	rVB	40711	65478	0.02%	0.020%
43	9.275	1336	1343	1356	rBV	520852	764373	0.26%	0.235%
44	9.384	1356	1361	1372	rBV	197540	283447	0.10%	0.087%
45	9.549	1386	1388	1391	rVB2	1101	804	0.00%	0.000%
46	10.055	1465	1471	1486	rBV	485037	672667	0.23%	0.207%
47	10.195	1490	1494	1502	rVB	7954	12817	0.00%	0.004%
48	10.305	1507	1512	1522	rVB	14721	23072	0.01%	0.007%
49	10.640	1563	1567	1574	rBV2	8021	12215	0.00%	0.004%
50	10.738	1579	1583	1588	rVB5	557	1285	0.00%	0.000%
51	10.774	1588	1589	1592	rBV3	494	524	0.00%	0.000%
52	10.957	1617	1619	1623	rVB5	742	1157	0.00%	0.000%
53	11.018	1626	1629	1632	rBV3	377	477	0.00%	0.000%
54	11.104	1639	1643	1644	rBV2	589	605	0.00%	0.000%
55	11.189	1652	1657	1664	rVV	288084	373513	0.13%	0.115%
56	11.238	1664	1665	1669	rVB3	2389	2053	0.00%	0.001%
57	11.299	1673	1675	1676	rBV	823	461	0.00%	0.000%
58	11.384	1685	1689	1692	rBV3	2145	3169	0.00%	0.001%
59	11.451	1697	1700	1705	rVB3	1609	2438	0.00%	0.001%
60	11.494	1705	1707	1709	rVB2	828	713	0.00%	0.000%
61	11.524	1711	1712	1714	rVV2	469	439	0.00%	0.000%
62	11.616	1724	1727	1731	rVV3	1516	1838	0.00%	0.001%
63	11.652	1731	1733	1736	rVB3	624	716	0.00%	0.000%
64	11.756	1746	1750	1755	rVB	3994	4955	0.00%	0.002%
65	11.829	1759	1762	1763	rBV2	402	554	0.00%	0.000%
66	11.969	1782	1785	1788	rBV5	846	861	0.00%	0.000%
67	12.018	1788	1793	1801	rBV	524710	689183	0.24%	0.212%
68	12.317	1837	1842	1852	rBV	483192	621790	0.21%	0.191%
69	12.536	1876	1878	1880	rVB2	652	509	0.00%	0.000%
70	12.634	1892	1894	1898	rVB4	363	469	0.00%	0.000%
71	12.762	1913	1915	1917	rBV3	413	485	0.00%	0.000%
72	12.835	1922	1927	1928	rBV3	497	657	0.00%	0.000%
73	12.865	1928	1932	1933	rBV3	353	448	0.00%	0.000%
74	13.006	1951	1955	1957	rBV3	229	434	0.00%	0.000%
75	13.237	1991	1993	1996	rBV3	343	415	0.00%	0.000%
76	13.603	2050	2053	2054	rBV2	383	429	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043840.D
 Acq On : 13 Nov 2024 17:48
 Operator : JC/MD
 Sample : P4785-16
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.804	2084	2086	2088	rVB2	558	484	0.00%	0.000%
78	13.877	2096	2098	2102	rBV3	406	581	0.00%	0.000%
79	14.030	2121	2123	2127	rVB3	341	481	0.00%	0.000%
80	14.140	2137	2141	2144	rBV3	405	548	0.00%	0.000%
81	14.603	2213	2217	2220	rBV4	650	949	0.00%	0.000%
82	14.640	2221	2223	2227	rVB2	733	661	0.00%	0.000%
83	14.700	2230	2233	2234	rBV2	482	637	0.00%	0.000%
84	14.963	2274	2276	2277	rBV2	554	449	0.00%	0.000%
85	14.993	2277	2281	2283	rVV2	352	478	0.00%	0.000%
86	15.139	2303	2305	2309	rVB2	625	705	0.00%	0.000%
87	15.170	2309	2310	2314	rBV2	399	470	0.00%	0.000%
88	15.249	2322	2323	2326	rBV2	364	396	0.00%	0.000%
89	15.414	2348	2350	2353	rBV3	354	406	0.00%	0.000%
90	15.450	2353	2356	2359	rVV5	446	581	0.00%	0.000%
91	15.560	2372	2374	2379	rVB3	531	649	0.00%	0.000%
92	15.688	2393	2395	2397	rVV2	523	405	0.00%	0.000%
93	15.908	2430	2431	2434	rBV3	316	390	0.00%	0.000%
94	16.060	2454	2456	2458	rVB3	589	573	0.00%	0.000%
95	16.090	2458	2461	2463	rBV4	540	645	0.00%	0.000%
96	16.286	2489	2493	2494	rBV3	415	533	0.00%	0.000%
97	16.359	2502	2505	2506	rBV2	914	721	0.00%	0.000%
98	16.444	2517	2519	2521	rVV3	574	608	0.00%	0.000%
99	16.505	2526	2529	2533	rVB2	523	712	0.00%	0.000%
100	16.706	2559	2562	2566	rBV3	465	786	0.00%	0.000%




Sum of corrected areas: 325498890

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043840.D
Acq On : 13 Nov 2024 17:48
Operator : JC/MD
Sample : P4785-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

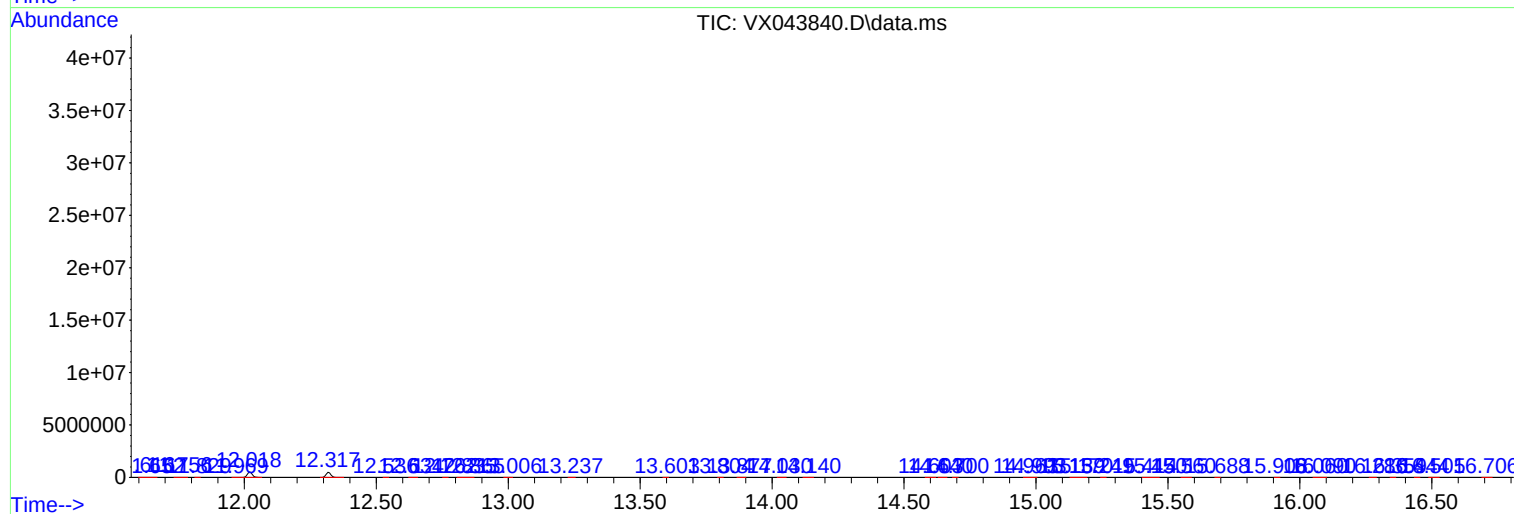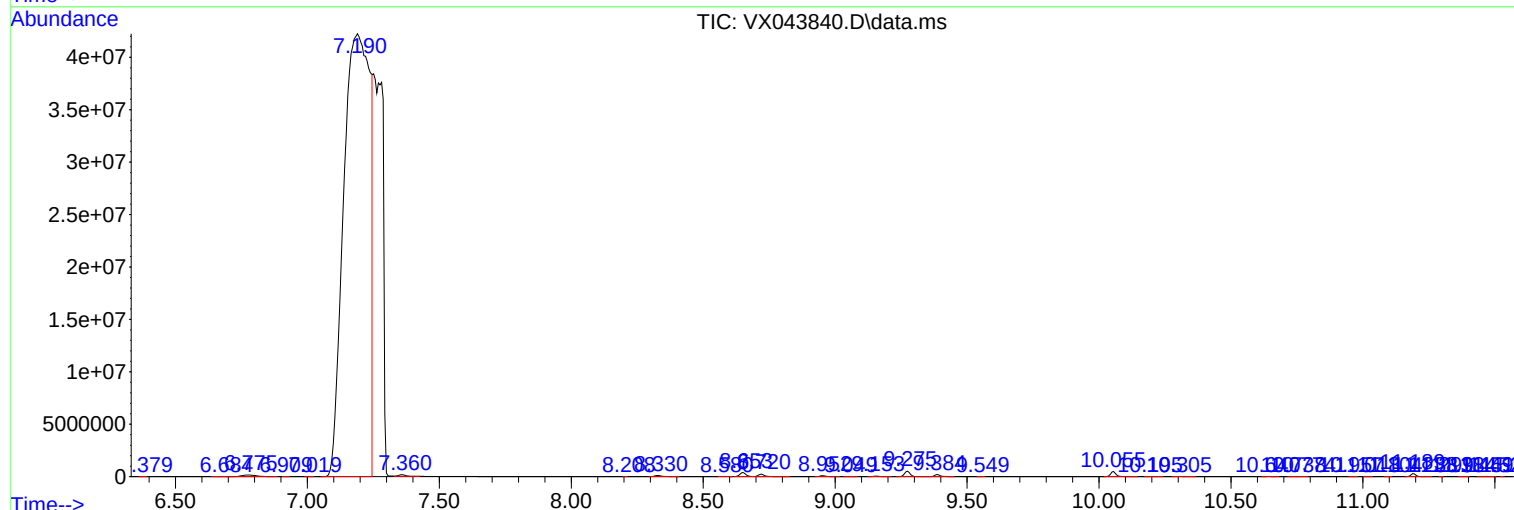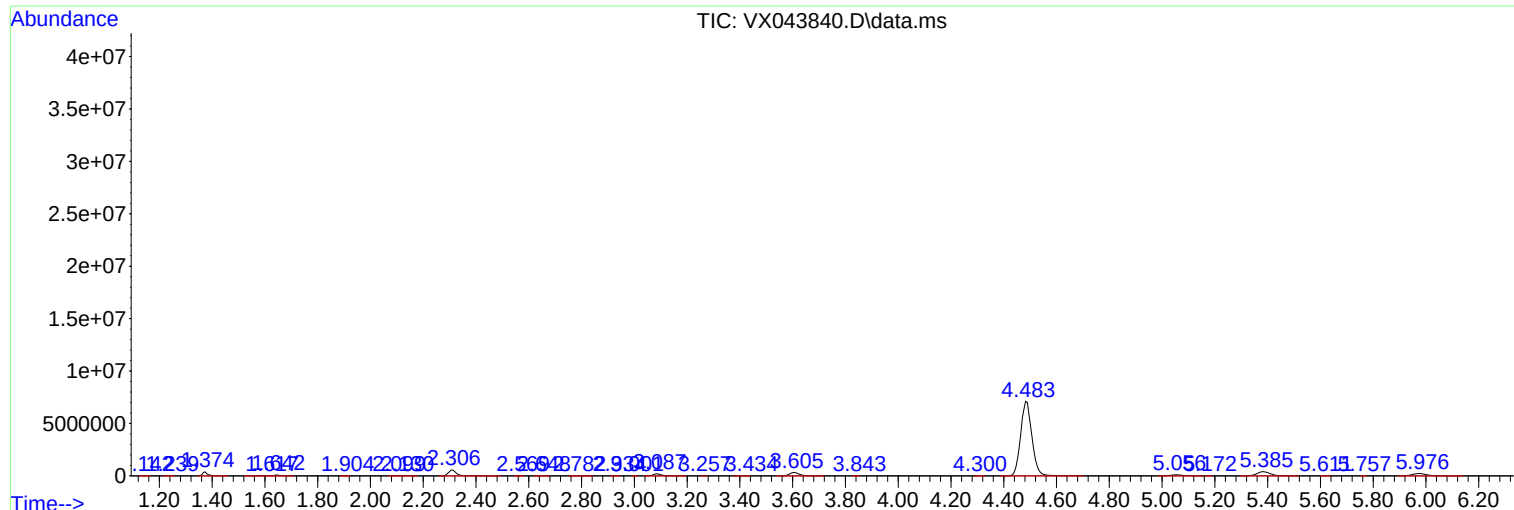

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043840.D
Acq On : 13 Nov 2024 17:48
Operator : JC/MD
Sample : P4785-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043840.D
Acq On : 13 Nov 2024 17:48
Operator : JC/MD
Sample : P4785-16
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc