

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043841.D
 Acq On : 13 Nov 2024 18:11
 Operator : JC/MD
 Sample : P4785-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043841.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	27	rBV	9007	9949	0.00%	0.003%
2	1.374	43	47	59	rBV2	324646	426053	0.13%	0.116%
3	1.642	88	91	102	rVB	80983	125978	0.04%	0.034%
4	2.099	162	166	168	rBV	8645	12062	0.00%	0.003%
5	2.239	187	189	192	rVB3	1130	1230	0.00%	0.000%
6	2.306	192	200	225	rBV2	472219	1005697	0.30%	0.274%
7	2.562	241	242	243	rBV	693	397	0.00%	0.000%
8	2.623	250	252	253	rBV2	405	344	0.00%	0.000%
9	2.642	253	255	257	rBV3	635	716	0.00%	0.000%
10	2.727	265	269	271	rBV3	326	476	0.00%	0.000%
11	2.782	272	278	288	rVV3	5080	10548	0.00%	0.003%
12	2.922	299	301	302	rBV2	504	489	0.00%	0.000%
13	3.087	320	328	341	rBV	184542	381563	0.11%	0.104%
14	3.215	348	349	351	rVB2	512	343	0.00%	0.000%
15	3.282	359	360	361	rBV	325	176	0.00%	0.000%
16	3.385	375	377	380	rVB3	319	251	0.00%	0.000%
17	3.440	380	386	395	rBV7	2142	5783	0.00%	0.002%
18	3.605	404	413	434	rBV	282534	724984	0.22%	0.198%
19	3.843	450	452	453	rVB2	355	219	0.00%	0.000%
20	3.861	453	455	456	rBV	341	183	0.00%	0.000%
21	3.922	463	465	467	rBV2	220	150	0.00%	0.000%
22	4.001	476	478	480	rVB3	329	201	0.00%	0.000%
23	4.062	486	488	489	rBV2	208	184	0.00%	0.000%
24	4.080	489	491	492	rVV2	405	257	0.00%	0.000%
25	4.111	492	496	497	rVB2	296	291	0.00%	0.000%
26	4.154	502	503	506	rBV	269	242	0.00%	0.000%
27	4.202	509	511	512	rBV	338	235	0.00%	0.000%
28	4.306	525	528	531	rBV4	537	575	0.00%	0.000%
29	4.385	539	541	544	rVB2	293	262	0.00%	0.000%
30	4.483	544	557	592	rBV	6766522	19706031	5.86%	5.378%
31	5.050	640	650	668	rVB	98366	327913	0.10%	0.089%
32	5.385	691	705	726	rBV	357308	1265458	0.38%	0.345%
33	5.611	741	742	744	rBV2	427	351	0.00%	0.000%
34	5.800	772	773	776	rVB3	248	153	0.00%	0.000%
35	5.824	776	777	778	rBV	395	164	0.00%	0.000%
36	5.976	789	802	820	rBV2	222276	814813	0.24%	0.222%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043841.D
 Acq On : 13 Nov 2024 18:11
 Operator : JC/MD
 Sample : P4785-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	6.190	836	837	840	rBV2	471	436	0.00%	0.000%
38	6.348	861	863	864	rVB2	295	209	0.00%	0.000%
39	6.373	864	867	869	rBV4	432	612	0.00%	0.000%
40	6.434	875	877	878	rBV	224	184	0.00%	0.000%
41	6.464	878	882	884	rVB3	330	380	0.00%	0.000%
42	6.531	891	893	895	rBV	154	193	0.00%	0.000%
43	6.556	895	897	898	rVV	209	149	0.00%	0.000%
44	6.653	912	913	916	rBV2	335	221	0.00%	0.000%
45	6.684	916	918	921	rBV2	353	225	0.00%	0.000%
46	6.775	921	933	949	rBV2	149932	534548	0.16%	0.146%
47	7.019	971	973	974	rVB2	289	174	0.00%	0.000%
48	7.190	978	1001	1013	rBV8	42426337	336077041	100.00%	91.715%
49	7.354	1025	1028	1041	rVB	164153	302125	0.09%	0.082%
50	8.330	1183	1188	1199	rVB	105525	181078	0.05%	0.049%
51	8.580	1225	1229	1234	rBV	18607	29334	0.01%	0.008%
52	8.647	1235	1240	1247	rVV	375870	616355	0.18%	0.168%
53	8.720	1247	1252	1264	rVB	215691	346203	0.10%	0.094%
54	8.952	1285	1290	1300	rBV	82400	127640	0.04%	0.035%
55	9.153	1318	1323	1330	rVB	41004	62469	0.02%	0.017%
56	9.275	1337	1343	1354	rBV	469453	714175	0.21%	0.195%
57	9.384	1356	1361	1373	rBV	193736	284213	0.08%	0.078%
58	9.933	1447	1451	1456	rBV2	11123	17154	0.01%	0.005%
59	10.055	1465	1471	1489	rVB	432198	622554	0.19%	0.170%
60	10.201	1490	1495	1500	rVV3	7040	10920	0.00%	0.003%
61	10.305	1507	1512	1519	rVB	13679	20678	0.01%	0.006%
62	10.482	1540	1541	1542	rBV	873	418	0.00%	0.000%
63	10.646	1563	1568	1575	rBV	8352	11782	0.00%	0.003%
64	10.878	1604	1606	1607	rBV	692	307	0.00%	0.000%
65	10.963	1619	1620	1622	rBV2	853	572	0.00%	0.000%
66	11.189	1652	1657	1663	rBV	286241	378045	0.11%	0.103%
67	11.427	1694	1696	1697	rBV2	488	404	0.00%	0.000%
68	11.616	1723	1727	1732	rVB3	1416	1887	0.00%	0.001%
69	11.658	1732	1734	1736	rVB3	531	243	0.00%	0.000%
70	11.756	1747	1750	1757	rVB3	2831	4122	0.00%	0.001%
71	12.018	1788	1793	1802	rBV	483338	634561	0.19%	0.173%
72	12.250	1826	1831	1834	rVB5	1184	1583	0.00%	0.000%
73	12.280	1834	1836	1837	rBV	367	263	0.00%	0.000%
74	12.317	1837	1842	1851	rBV	483327	619861	0.18%	0.169%
75	12.646	1894	1896	1899	rBV3	497	506	0.00%	0.000%
76	12.737	1909	1911	1912	rBV2	359	224	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043841.D
 Acq On : 13 Nov 2024 18:11
 Operator : JC/MD
 Sample : P4785-17
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	12.817	1923	1924	1927	rBV3	538	400	0.00%	0.000%
78	12.932	1942	1943	1946	rBV3	335	271	0.00%	0.000%
79	12.993	1949	1953	1954	rBV2	243	242	0.00%	0.000%
80	13.067	1963	1965	1968	rBV2	334	433	0.00%	0.000%
81	13.097	1968	1970	1971	rBV2	289	191	0.00%	0.000%
82	13.128	1974	1975	1978	rBV2	347	344	0.00%	0.000%
83	13.219	1988	1990	1991	rBV2	319	176	0.00%	0.000%
84	13.304	2002	2004	2007	rVB	473	393	0.00%	0.000%
85	13.548	2042	2044	2045	rBV	254	225	0.00%	0.000%
86	13.707	2069	2070	2073	rVB3	451	376	0.00%	0.000%
87	13.945	2106	2109	2110	rBV2	682	473	0.00%	0.000%
88	13.987	2113	2116	2117	rBV2	422	410	0.00%	0.000%
89	14.024	2120	2122	2123	rBV	366	275	0.00%	0.000%
90	14.054	2125	2127	2131	rVB2	554	593	0.00%	0.000%
91	14.164	2142	2145	2146	rBV3	486	477	0.00%	0.000%
92	14.347	2173	2175	2177	rBV2	322	208	0.00%	0.000%
93	14.585	2212	2214	2218	rVB3	515	597	0.00%	0.000%
94	14.774	2243	2245	2247	rBV2	501	494	0.00%	0.000%
95	15.030	2285	2287	2288	rBV2	548	458	0.00%	0.000%
96	15.078	2294	2295	2296	rBV	585	351	0.00%	0.000%
97	15.798	2411	2413	2414	rBV2	502	293	0.00%	0.000%
98	16.261	2487	2489	2492	rVB4	676	455	0.00%	0.000%
99	16.328	2498	2500	2504	rBV5	461	689	0.00%	0.000%
100	16.645	2550	2552	2554	rBV3	720	509	0.00%	0.000%




Sum of corrected areas: 366438102

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043841.D
Acq On : 13 Nov 2024 18:11
Operator : JC/MD
Sample : P4785-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

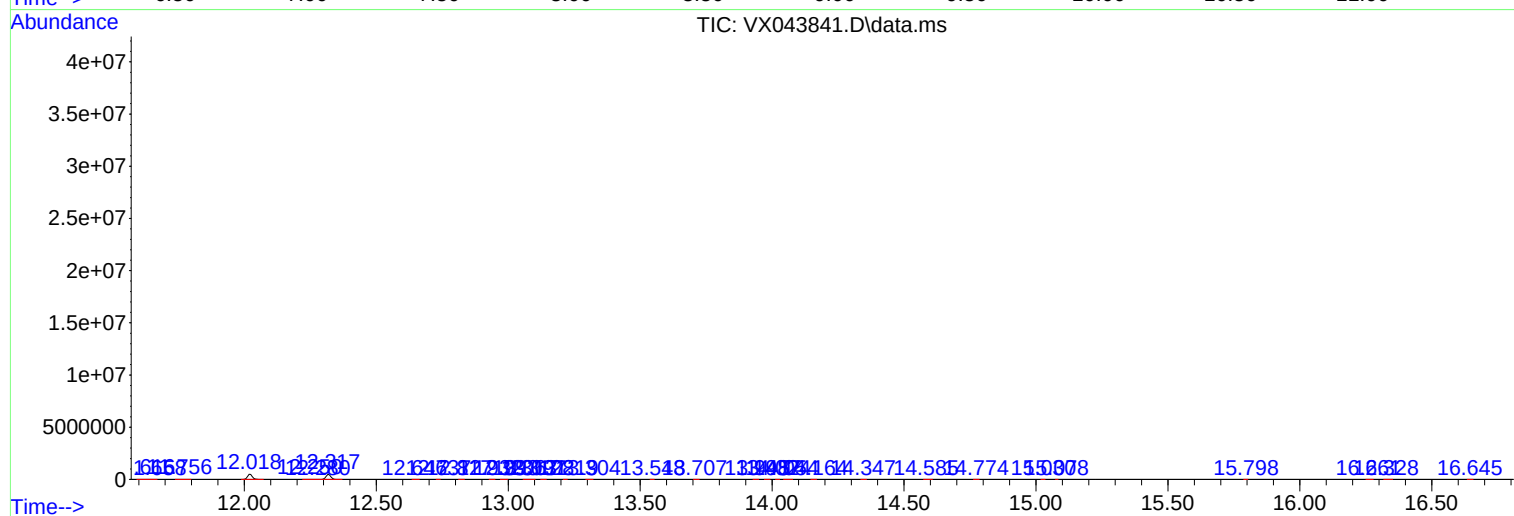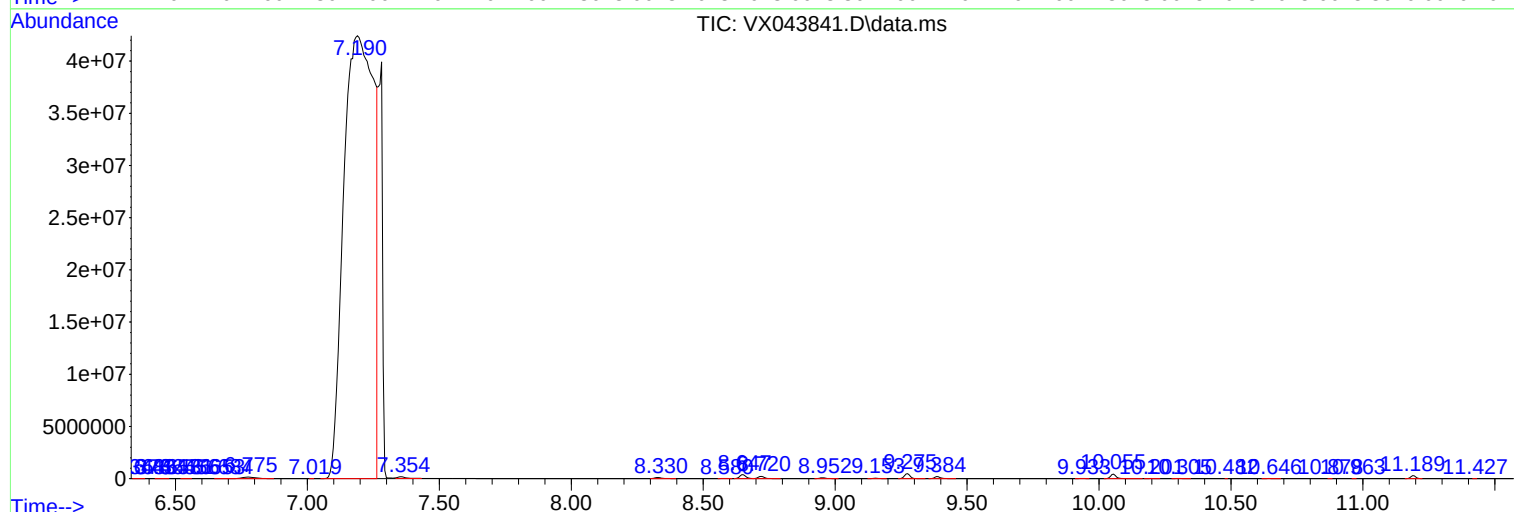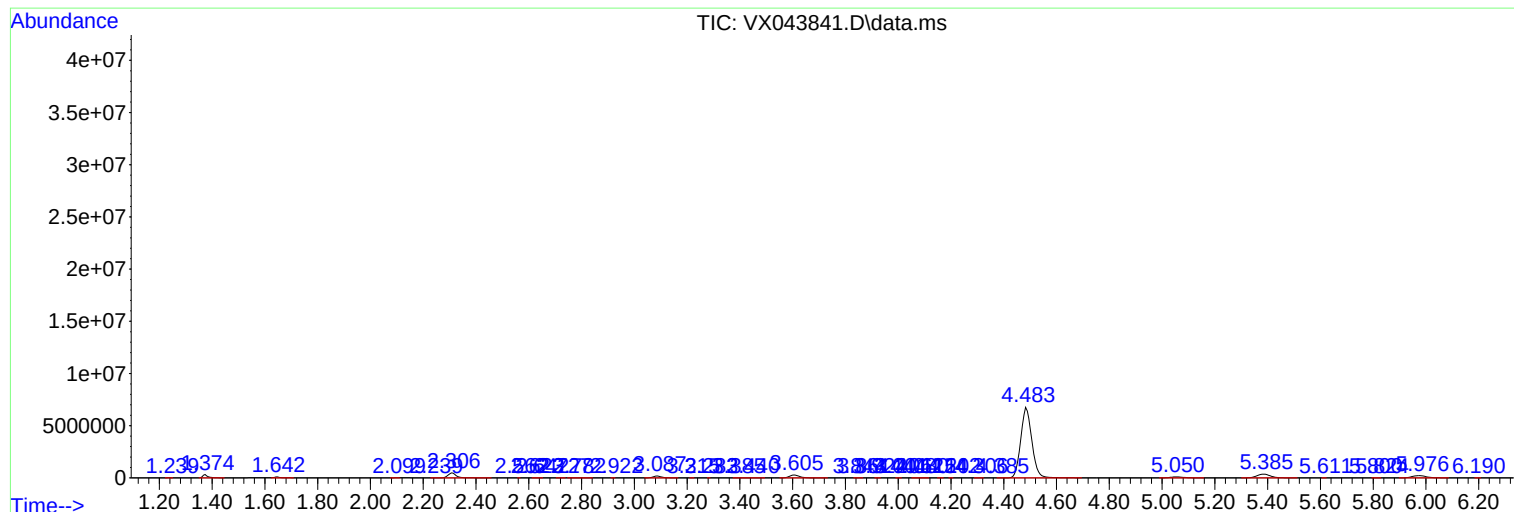

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043841.D
Acq On : 13 Nov 2024 18:11
Operator : JC/MD
Sample : P4785-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043841.D
Acq On : 13 Nov 2024 18:11
Operator : JC/MD
Sample : P4785-17
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------