

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043846.D
 Acq On : 13 Nov 2024 20:06
 Operator : JC/MD
 Sample : P4724-24ME
 Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	43	46	49	rBV	43182	52738	6.57%	0.844%
2	2.276	189	195	208	rBV	156989	262796	32.74%	4.205%
3	2.556	239	241	247	rVB3	452	749	0.09%	0.012%
4	2.636	252	254	256	rBV3	307	259	0.03%	0.004%
5	2.782	273	278	285	rBV3	1109	2870	0.36%	0.046%
6	2.855	289	290	292	rVB	517	249	0.03%	0.004%
7	2.940	297	304	311	rBV	4053	10458	1.30%	0.167%
8	3.099	327	330	331	rBV	258	265	0.03%	0.004%
9	3.233	349	352	353	rBV2	350	310	0.04%	0.005%
10	3.251	353	355	359	rVB3	251	289	0.04%	0.005%
11	3.312	364	365	368	rVB2	309	271	0.03%	0.004%
12	3.416	375	382	391	rVB4	2154	4973	0.62%	0.080%
13	3.556	402	405	407	rVV2	248	252	0.03%	0.004%
14	3.654	417	421	424	rBV2	185	265	0.03%	0.004%
15	3.702	427	429	432	rVV3	333	416	0.05%	0.007%
16	3.776	439	441	444	rVV	293	292	0.04%	0.005%
17	3.806	444	446	450	rVB	359	265	0.03%	0.004%
18	3.934	463	467	468	rBV2	227	286	0.04%	0.005%
19	3.977	472	474	476	rBV	265	281	0.04%	0.004%
20	4.148	500	502	504	rBV2	405	472	0.06%	0.008%
21	4.300	526	527	531	rBV2	325	363	0.05%	0.006%
22	4.483	549	557	575	rBV	29931	122780	15.29%	1.965%
23	5.056	637	651	665	rBV	103955	324106	40.37%	5.186%
24	5.336	694	697	700	rBV	471	523	0.07%	0.008%
25	5.586	736	738	741	rVB	373	254	0.03%	0.004%
26	5.848	779	781	782	rBV2	321	301	0.04%	0.005%
27	5.879	784	786	788	rBV2	278	316	0.04%	0.005%
28	5.958	788	799	816	rBV2	277772	802796	100.00%	12.845%
29	6.269	846	850	854	rBV3	526	964	0.12%	0.015%
30	6.361	862	865	866	rBV	1011	881	0.11%	0.014%
31	6.482	883	885	886	rVB	529	281	0.04%	0.004%
32	6.507	886	889	892	rBV2	327	360	0.04%	0.006%
33	6.653	912	913	918	rVB2	214	263	0.03%	0.004%
34	6.751	921	929	947	rBV	211703	527072	65.65%	8.433%
35	7.117	981	989	1000	rBV	149241	344353	42.89%	5.510%
36	7.306	1011	1020	1034	rBV	152317	348810	43.45%	5.581%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043846.D
 Acq On : 13 Nov 2024 20:06
 Operator : JC/MD
 Sample : P4724-24ME
 Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.714	1084	1087	1088	rBV2	338	384	0.05%	0.006%
38	7.775	1096	1097	1101	rBV2	412	432	0.05%	0.007%
39	7.958	1123	1127	1128	rBV2	566	716	0.09%	0.011%
40	8.238	1170	1173	1174	rBV	402	434	0.05%	0.007%
41	8.324	1181	1187	1200	rBV	99629	172481	21.49%	2.760%
42	8.446	1206	1207	1210	rVB2	590	376	0.05%	0.006%
43	8.525	1218	1220	1221	rBV2	419	251	0.03%	0.004%
44	8.647	1233	1240	1255	rBV	419007	683206	85.10%	10.932%
45	8.891	1278	1280	1282	rVB2	450	309	0.04%	0.005%
46	8.952	1285	1290	1301	rBV	66750	108408	13.50%	1.735%
47	9.073	1306	1310	1312	rVV3	464	560	0.07%	0.009%
48	9.110	1315	1316	1320	rVB3	577	606	0.08%	0.010%
49	9.165	1322	1325	1327	rBV3	289	313	0.04%	0.005%
50	9.269	1340	1342	1344	rBV2	461	422	0.05%	0.007%
51	9.390	1357	1362	1381	rBV	148331	295054	36.75%	4.721%
52	9.671	1406	1408	1410	rBV	302	272	0.03%	0.004%
53	9.708	1410	1414	1415	rVV2	1221	1348	0.17%	0.022%
54	9.744	1419	1420	1423	rVB	541	405	0.05%	0.006%
55	9.775	1423	1425	1426	rBV	397	293	0.04%	0.005%
56	9.829	1431	1434	1436	rBV	444	344	0.04%	0.006%
57	10.055	1465	1471	1484	rBV	426440	625015	77.85%	10.001%
58	10.305	1510	1512	1516	rBV	282	384	0.05%	0.006%
59	10.372	1521	1523	1525	rBV2	375	372	0.05%	0.006%
60	10.451	1534	1536	1538	rVB	461	407	0.05%	0.007%
61	10.482	1540	1541	1545	rBV2	376	378	0.05%	0.006%
62	10.604	1557	1561	1563	rBV	296	500	0.06%	0.008%
63	10.823	1594	1597	1599	rBV2	279	289	0.04%	0.005%
64	11.000	1624	1626	1629	rBV	187	287	0.04%	0.005%
65	11.195	1652	1658	1669	rBV	267222	367859	45.82%	5.886%
66	11.469	1701	1703	1708	rBV3	386	499	0.06%	0.008%
67	11.536	1711	1714	1715	rBV2	241	317	0.04%	0.005%
68	11.738	1744	1747	1750	rVB2	411	429	0.05%	0.007%
69	11.847	1762	1765	1766	rBV2	247	259	0.03%	0.004%
70	11.933	1777	1779	1780	rBV	366	269	0.03%	0.004%
71	12.018	1788	1793	1804	rBV	430274	569749	70.97%	9.116%
72	12.164	1815	1817	1818	rBV	581	403	0.05%	0.006%
73	12.317	1837	1842	1856	rVV	449324	592928	73.86%	9.487%
74	12.719	1905	1908	1911	rBV2	273	327	0.04%	0.005%
75	12.798	1918	1921	1923	rBV2	288	390	0.05%	0.006%
76	12.951	1943	1946	1950	rBV2	336	569	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043846.D
 Acq On : 13 Nov 2024 20:06
 Operator : JC/MD
 Sample : P4724-24ME
 Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
 Title : VOC Analysis

77	13.048	1960	1962	1965	rVB2	345	386	0.05%	0.006%
78	13.286	1999	2001	2003	rBV	238	266	0.03%	0.004%
79	13.359	2009	2013	2014	rBV2	297	375	0.05%	0.006%
80	13.500	2033	2036	2037	rBV2	399	314	0.04%	0.005%
81	13.530	2040	2041	2044	rVB2	376	285	0.04%	0.005%
82	13.603	2052	2053	2057	rBV2	237	343	0.04%	0.005%
83	13.725	2071	2073	2074	rBV	356	314	0.04%	0.005%
84	13.743	2074	2076	2079	rVB	559	483	0.06%	0.008%
85	13.804	2084	2086	2088	rBV2	269	273	0.03%	0.004%
86	14.012	2116	2120	2121	rBV2	415	421	0.05%	0.007%
87	14.048	2125	2126	2129	rVB2	539	364	0.05%	0.006%
88	14.134	2137	2140	2143	rVB3	451	512	0.06%	0.008%
89	14.170	2143	2146	2148	rBV	403	347	0.04%	0.006%
90	14.383	2179	2181	2185	rBV3	371	629	0.08%	0.010%
91	14.761	2240	2243	2245	rVV3	285	311	0.04%	0.005%
92	14.847	2255	2257	2259	rBV	434	281	0.04%	0.004%
93	14.871	2259	2261	2262	rBV	431	250	0.03%	0.004%
94	14.908	2266	2267	2269	rBV2	378	294	0.04%	0.005%
95	15.267	2324	2326	2327	rBV	397	309	0.04%	0.005%
96	15.676	2391	2393	2395	rBV3	491	295	0.04%	0.005%
97	16.054	2453	2455	2456	rBV	443	253	0.03%	0.004%
98	16.334	2500	2501	2506	rVB3	520	494	0.06%	0.008%
99	16.542	2534	2535	2538	rBV2	440	325	0.04%	0.005%
100	16.731	2565	2566	2567	rBV	573	257	0.03%	0.004%

Sum of corrected areas: 6249804




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043846.D
Acq On : 13 Nov 2024 20:06
Operator : JC/MD
Sample : P4724-24ME
Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

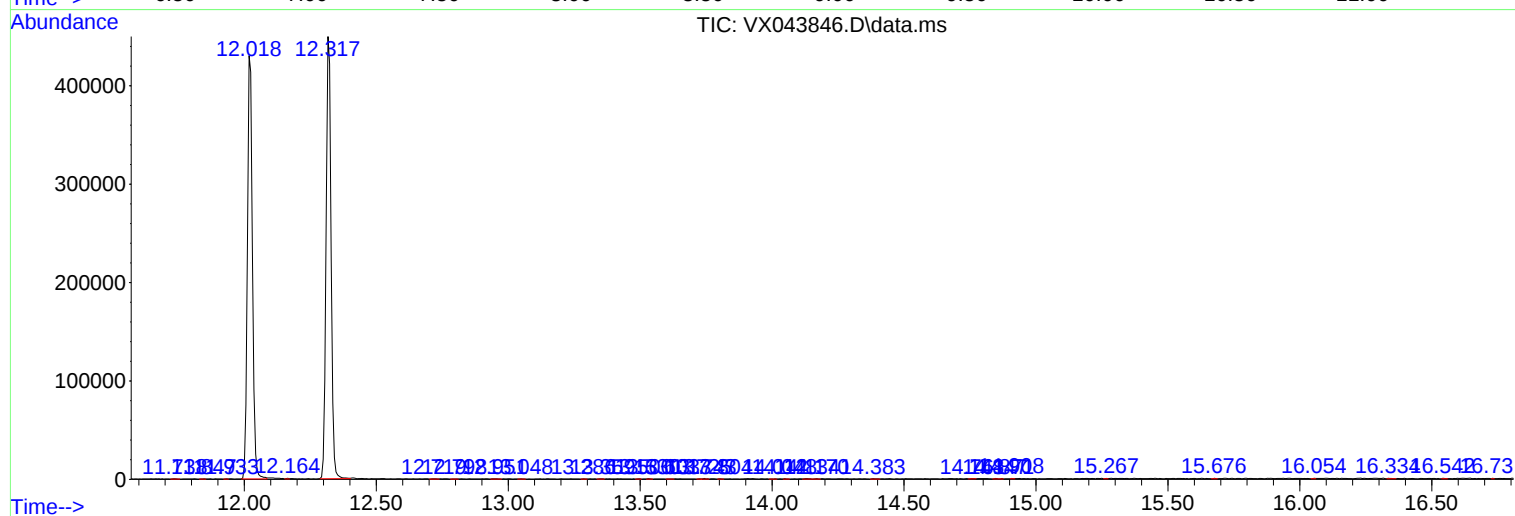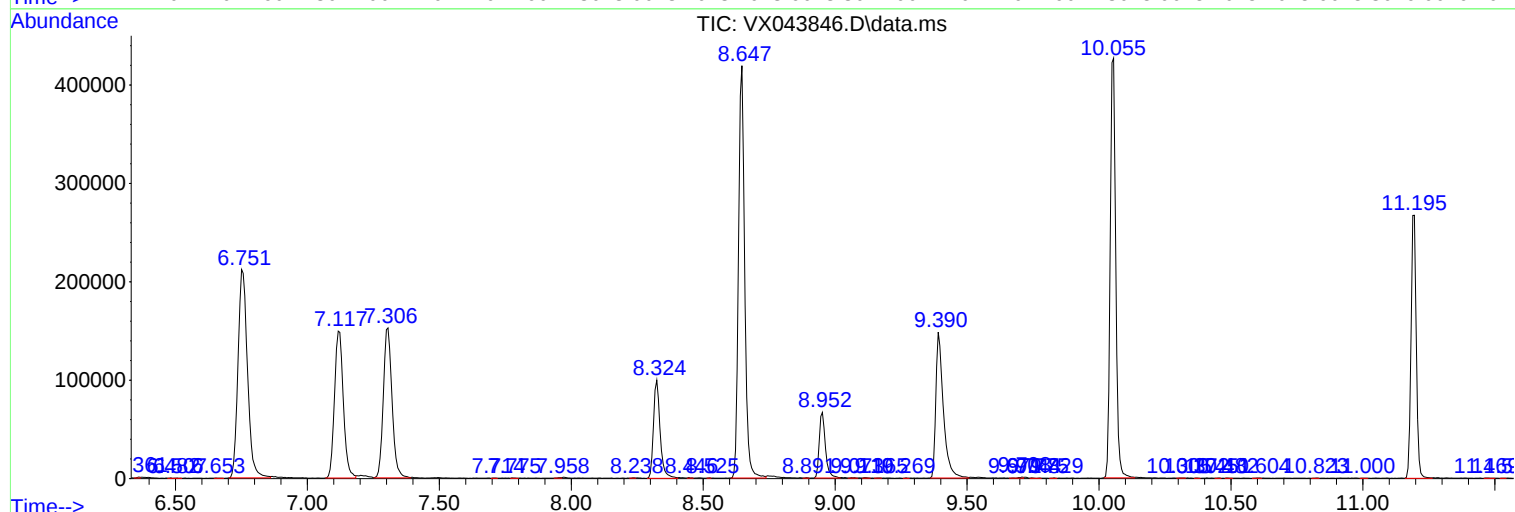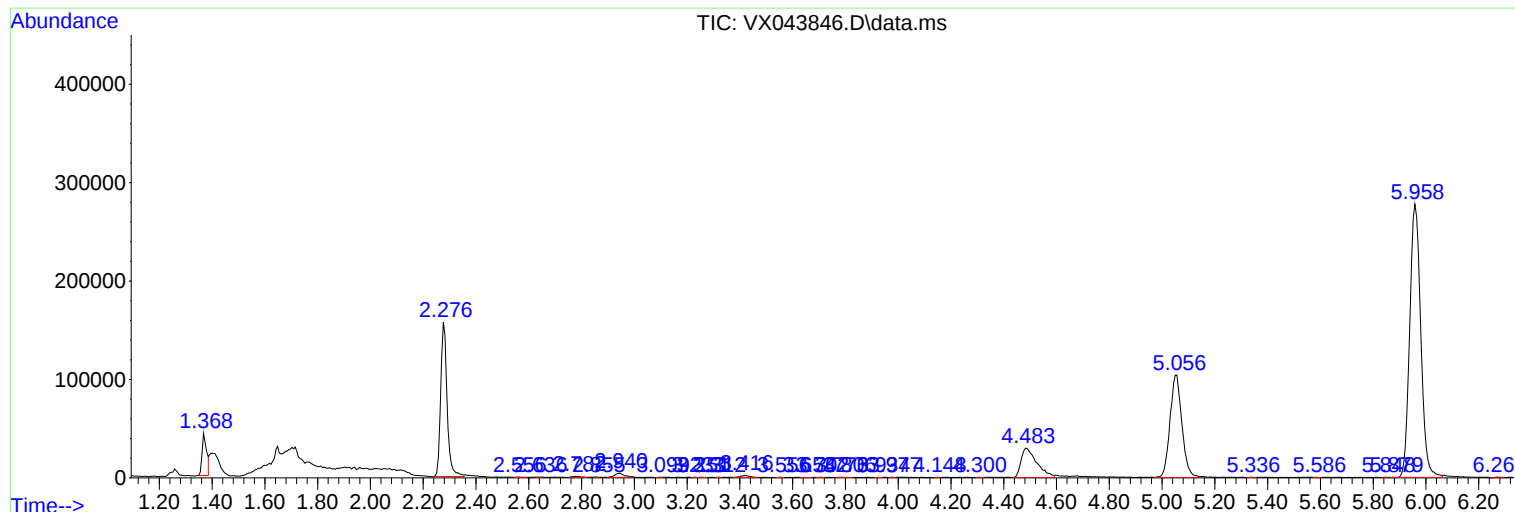

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043846.D
Acq On : 13 Nov 2024 20:06
Operator : JC/MD
Sample : P4724-24ME
Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043846.D
Acq On : 13 Nov 2024 20:06
Operator : JC/MD
Sample : P4724-24ME
Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc