

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043847.D
 Acq On : 13 Nov 2024 20:29
 Operator : JC/MD
 Sample : P4751-06ME
 Misc : 5.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M

Title : VOC Analysis

Signal : TIC: VX043847.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	34	rBV2	7655	14266	1.74%	0.226%
2	1.368	43	46	49	rBV	38527	48269	5.90%	0.764%
3	2.276	189	195	216	rBV	158700	263421	32.18%	4.171%
4	2.605	246	249	254	rBV3	401	660	0.08%	0.010%
5	2.782	271	278	281	rBV5	1224	2683	0.33%	0.042%
6	2.861	288	291	292	rBV3	504	498	0.06%	0.008%
7	2.940	296	304	317	rVB	3438	9687	1.18%	0.153%
8	3.239	349	353	354	rBV2	278	426	0.05%	0.007%
9	3.270	356	358	360	rVV	269	281	0.03%	0.004%
10	3.306	363	364	367	rVV3	267	290	0.04%	0.005%
11	3.373	373	375	377	rVV2	325	289	0.04%	0.005%
12	3.416	377	382	389	rVB4	2748	5819	0.71%	0.092%
13	3.514	397	398	400	rVV	363	259	0.03%	0.004%
14	3.538	400	402	404	rVB2	320	242	0.03%	0.004%
15	4.001	476	478	479	rBV2	357	354	0.04%	0.006%
16	4.148	501	502	504	rVV2	423	311	0.04%	0.005%
17	4.202	508	511	512	rBV2	255	299	0.04%	0.005%
18	4.257	518	520	522	rVV2	227	247	0.03%	0.004%
19	4.330	531	532	534	rBV	317	276	0.03%	0.004%
20	4.355	534	536	539	rVB	323	327	0.04%	0.005%
21	4.489	549	558	583	rBV	28443	122121	14.92%	1.934%
22	5.056	638	651	669	rBV	103755	324087	39.59%	5.132%
23	5.263	683	685	688	rBV2	444	348	0.04%	0.006%
24	5.330	694	696	698	rBV2	257	242	0.03%	0.004%
25	5.525	725	728	729	rBV	316	268	0.03%	0.004%
26	5.568	734	735	738	rVV	373	276	0.03%	0.004%
27	5.958	786	799	816	rBV2	285700	818630	100.00%	12.962%
28	6.141	828	829	833	rVB2	494	528	0.06%	0.008%
29	6.263	846	849	853	rBV3	238	331	0.04%	0.005%
30	6.367	864	866	867	rBV2	683	689	0.08%	0.011%
31	6.470	881	883	885	rBV2	434	460	0.06%	0.007%
32	6.623	905	908	909	rVB2	329	283	0.03%	0.004%
33	6.641	909	911	912	rBV2	318	267	0.03%	0.004%
34	6.751	920	929	946	rBV	219554	547395	66.87%	8.668%
35	7.117	982	989	1002	rBV	138052	310613	37.94%	4.918%
36	7.306	1012	1020	1040	rVB	154369	356456	43.54%	5.644%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043847.D
 Acq On : 13 Nov 2024 20:29
 Operator : JC/MD
 Sample : P4751-06ME
 Misc : 5.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

37	7.470	1045	1047	1049	rBV	409	491	0.06%	0.008%
38	7.568	1062	1063	1065	rBV	457	272	0.03%	0.004%
39	7.623	1070	1072	1075	rBV2	375	406	0.05%	0.006%
40	7.653	1075	1077	1080	rVB2	347	401	0.05%	0.006%
41	7.854	1109	1110	1114	rBV2	330	392	0.05%	0.006%
42	7.885	1114	1115	1119	rVB	468	354	0.04%	0.006%
43	7.927	1119	1122	1124	rBV2	245	320	0.04%	0.005%
44	7.976	1125	1130	1132	rBV4	906	1371	0.17%	0.022%
45	8.031	1137	1139	1140	rVV	457	305	0.04%	0.005%
46	8.049	1140	1142	1145	rVV	275	379	0.05%	0.006%
47	8.244	1171	1174	1175	rBV	661	548	0.07%	0.009%
48	8.324	1181	1187	1202	rBV	98993	171487	20.95%	2.715%
49	8.647	1233	1240	1254	rBV	421816	688475	84.10%	10.902%
50	8.952	1284	1290	1301	rBV	66839	110000	13.44%	1.742%
51	9.122	1314	1318	1321	rVB3	821	1022	0.12%	0.016%
52	9.159	1321	1324	1328	rBV2	427	633	0.08%	0.010%
53	9.391	1357	1362	1379	rBV	130122	289079	35.31%	4.577%
54	9.714	1411	1415	1421	rVB4	945	1691	0.21%	0.027%
55	9.756	1421	1422	1425	rVB2	318	301	0.04%	0.005%
56	9.787	1425	1427	1428	rBV	460	324	0.04%	0.005%
57	10.055	1465	1471	1484	rBV	448215	646678	79.00%	10.240%
58	10.396	1525	1527	1529	rBV2	250	291	0.04%	0.005%
59	10.567	1552	1555	1558	rBV3	259	348	0.04%	0.006%
60	11.195	1652	1658	1668	rBV	273759	367685	44.91%	5.822%
61	11.378	1687	1688	1692	rVB2	363	259	0.03%	0.004%
62	11.457	1698	1701	1702	rBV	330	255	0.03%	0.004%
63	11.475	1702	1704	1709	rBV2	499	593	0.07%	0.009%
64	11.524	1709	1712	1715	rVB2	268	281	0.03%	0.004%
65	11.628	1722	1729	1731	rVB2	344	691	0.08%	0.011%
66	11.689	1734	1739	1740	rBV	396	480	0.06%	0.008%
67	11.884	1769	1771	1772	rBV	386	248	0.03%	0.004%
68	12.018	1788	1793	1806	rBV	442274	594021	72.56%	9.406%
69	12.317	1837	1842	1851	rBV	459950	591403	72.24%	9.364%
70	12.768	1912	1916	1918	rBV2	422	498	0.06%	0.008%
71	13.030	1954	1959	1961	rVB2	487	747	0.09%	0.012%
72	13.061	1961	1964	1966	rBV	400	430	0.05%	0.007%
73	13.140	1974	1977	1980	rVB3	318	440	0.05%	0.007%
74	13.183	1980	1984	1987	rBV2	261	362	0.04%	0.006%
75	13.304	2002	2004	2006	rVV	495	359	0.04%	0.006%
76	13.408	2020	2021	2026	rVB2	353	496	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
 Data File : VX043847.D
 Acq On : 13 Nov 2024 20:29
 Operator : JC/MD
 Sample : P4751-06ME
 Misc : 5.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E3ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM110424WMA.M
 Title : VOC Analysis

77	13.487	2030	2034	2037	rBV2	365	564	0.07%	0.009%
78	13.579	2045	2049	2051	rVB2	309	413	0.05%	0.007%
79	13.609	2051	2054	2056	rBV2	278	332	0.04%	0.005%
80	13.682	2062	2066	2067	rBV	373	263	0.03%	0.004%
81	13.725	2070	2073	2074	rBV2	404	393	0.05%	0.006%
82	13.804	2084	2086	2090	rVB	424	273	0.03%	0.004%
83	13.890	2097	2100	2102	rVB	299	268	0.03%	0.004%
84	13.914	2102	2104	2109	rBV2	279	426	0.05%	0.007%
85	13.951	2109	2110	2113	rVB2	308	312	0.04%	0.005%
86	14.158	2142	2144	2147	rBV2	322	344	0.04%	0.005%
87	14.329	2169	2172	2174	rVV2	407	349	0.04%	0.006%
88	14.347	2174	2175	2178	rVB2	354	244	0.03%	0.004%
89	14.390	2178	2182	2183	rBV	401	359	0.04%	0.006%
90	14.432	2187	2189	2192	rVV2	326	399	0.05%	0.006%
91	14.536	2203	2206	2207	rBV2	465	437	0.05%	0.007%
92	14.585	2211	2214	2215	rVB2	349	366	0.04%	0.006%
93	15.024	2285	2286	2288	rBV	437	264	0.03%	0.004%
94	15.146	2303	2306	2307	rBV	311	261	0.03%	0.004%
95	16.084	2459	2460	2463	rVB2	607	398	0.05%	0.006%
96	16.200	2477	2479	2480	rBV2	466	338	0.04%	0.005%
97	16.237	2484	2485	2487	rVB	454	247	0.03%	0.004%
98	16.517	2529	2531	2534	rBV2	420	390	0.05%	0.006%
99	16.609	2545	2546	2548	rBV	527	387	0.05%	0.006%
100	16.682	2554	2558	2560	rBV4	435	644	0.08%	0.010%

Sum of corrected areas: 6315385




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043847.D
Acq On : 13 Nov 2024 20:29
Operator : JC/MD
Sample : P4751-06ME
Misc : 5.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

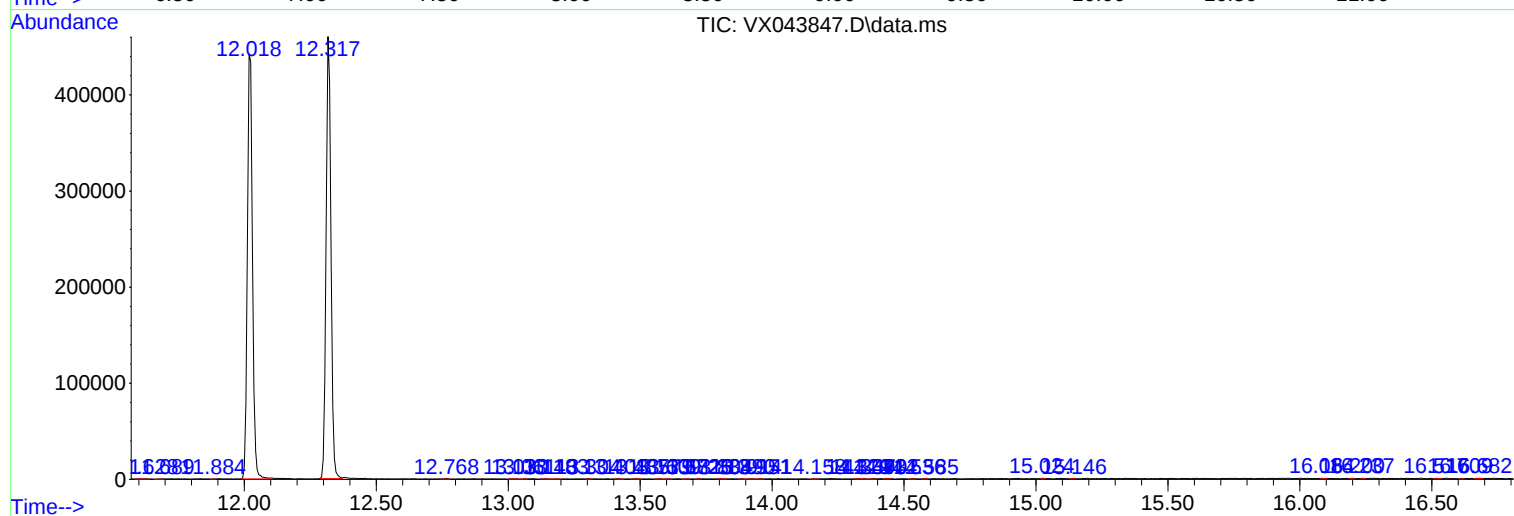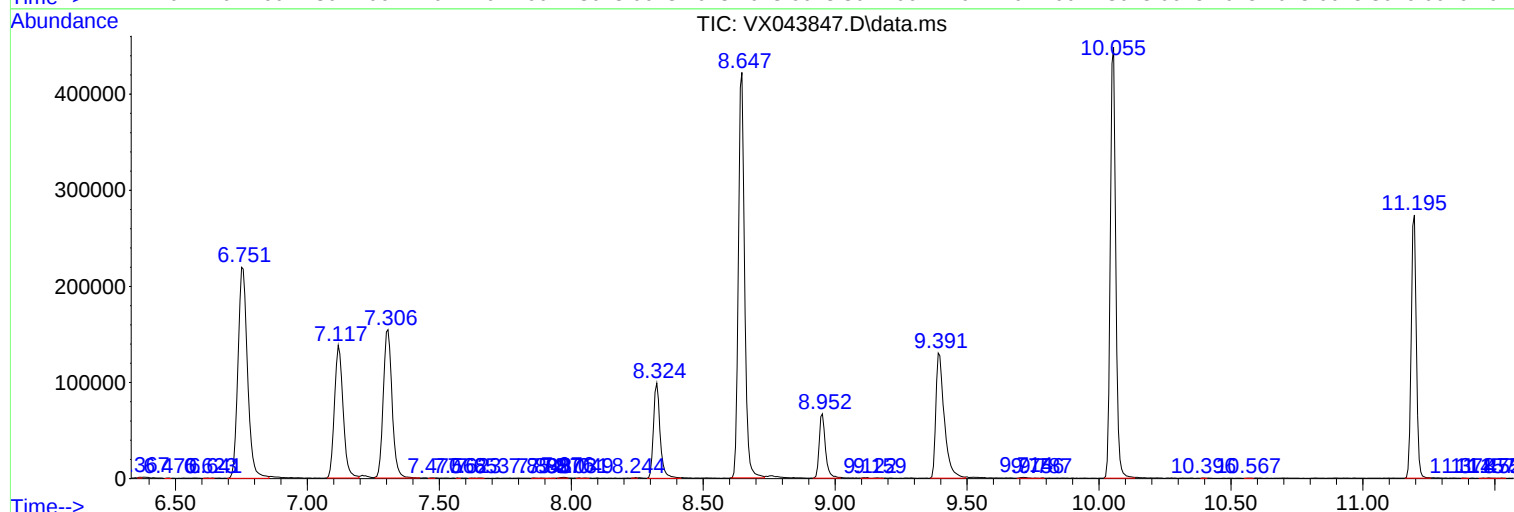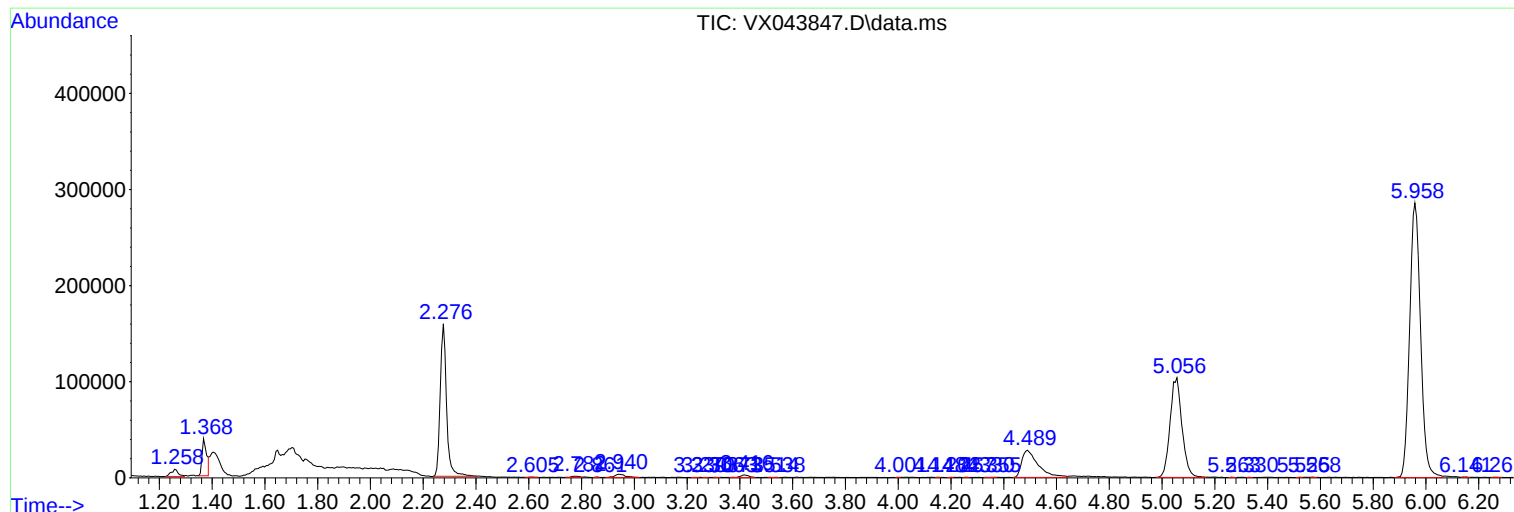

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043847.D
Acq On : 13 Nov 2024 20:29
Operator : JC/MD
Sample : P4751-06ME
Misc : 5.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111324\
Data File : VX043847.D
Acq On : 13 Nov 2024 20:29
Operator : JC/MD
Sample : P4751-06ME
Misc : 5.14g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E3ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML110424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc