

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111325\
 Data File : VX048591.D
 Acq On : 13 Nov 2025 13:41
 Operator : JC/MD
 Sample : PB170518TB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 PB170518TB

Quant Time: Nov 14 03:57:14 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
 Quant Title : SW846 8260
 QLast Update : Sat Nov 08 05:08:11 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.538	168	118773	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.745	114	235440	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.037	117	256905	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.006	152	130936	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.940	65	99602	60.182	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 120.360%#	
35) Dibromofluoromethane	5.373	113	84193	47.247	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 94.500%	
50) Toluene-d8	8.635	98	302330	54.399	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 108.800%	
62) 4-Bromofluorobenzene	11.061	95	124344	60.036	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 120.080%	


Target Compounds				Qvalue		
5) Bromomethane	1.636	94	488	0.535	ug/l #	46
10) Methyl Iodide	2.459	142	982	0.501	ug/l #	85
11) Tert butyl alcohol	2.940	59	1993	6.355	ug/l #	81
13) Acrolein	2.239	56	141	3.107	ug/l #	15
15) Acrylonitrile	3.087	53	428	0.468	ug/l #	57
16) Acetone	2.373	43	46024	58.749	ug/l	91
17) Carbon Disulfide	2.520	76	1712	0.440	ug/l #	90
18) Methyl Acetate	2.703	43	4060	1.886	ug/l	97
20) Methylene Chloride	2.794	84	13041	8.097	ug/l #	86
25) 2-Butanone	4.550	43	10940	9.440	ug/l	92
29) Tetrahydrofuran	5.007	42	425	0.514	ug/l #	63
38) Carbon Tetrachloride	5.544	117	12413	4.570	ug/l #	16
43) Isopropyl Acetate	6.324	43	12772	2.705	ug/l	97
48) Methyl methacrylate	7.781	41	62716	29.881	ug/l #	42
51) 4-Methyl-2-Pentanone	8.531	43	54363	20.227	ug/l #	50
54) cis-1,3-Dichloropropene	8.531	75	22669	8.586	ug/l #	68
58) 2-Chloroethyl Vinyl ether	8.250	63	291	0.209	ug/l #	46
59) 2-Hexanone	9.421	43	4259	2.130	ug/l	97
76) 1,2,3-Trichloropropane	11.061	75	66125	20.962	ug/l #	30
78) n-propylbenzene	11.287	91	2238	0.200	ug/l	94
81) trans-1,4-Dichloro-2-b...	11.061	75	66125	59.959	ug/l #	12
84) 1,2,4-Trimethylbenzene	11.738	105	1584	0.203	ug/l	99
85) sec-Butylbenzene	11.872	105	2740	0.277	ug/l	100
86) p-Isopropyltoluene	11.994	119	2577	0.309	ug/l #	81
87) 1,3-Dichlorobenzene	11.951	146	1271	0.276	ug/l	95
88) 1,4-Dichlorobenzene	11.951	146	1271	0.268	ug/l	95
89) n-Butylbenzene	12.317	91	3450	0.442	ug/l	91
90) Hexachloroethane	12.524	117	479	0.302	ug/l	90
93) 1,2,4-Trichlorobenzene	13.573	180	1432	0.488	ug/l	86
94) Hexachlorobutadiene	13.707	225	1049	0.855	ug/l	89
95) Naphthalene	13.762	128	2842	0.301	ug/l #	93
96) 1,2,3-Trichlorobenzene	13.945	180	1482	0.543	ug/l	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111325\
Data File : VX048591.D
Acq On : 13 Nov 2025 13:41
Operator : JC/MD
Sample : PB170518TB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
PB170518TB

Quant Time: Nov 14 03:57:14 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X110725W.M
Quant Title : SW846 8260
QLast Update : Sat Nov 08 05:08:11 2025
Response via : Initial Calibration




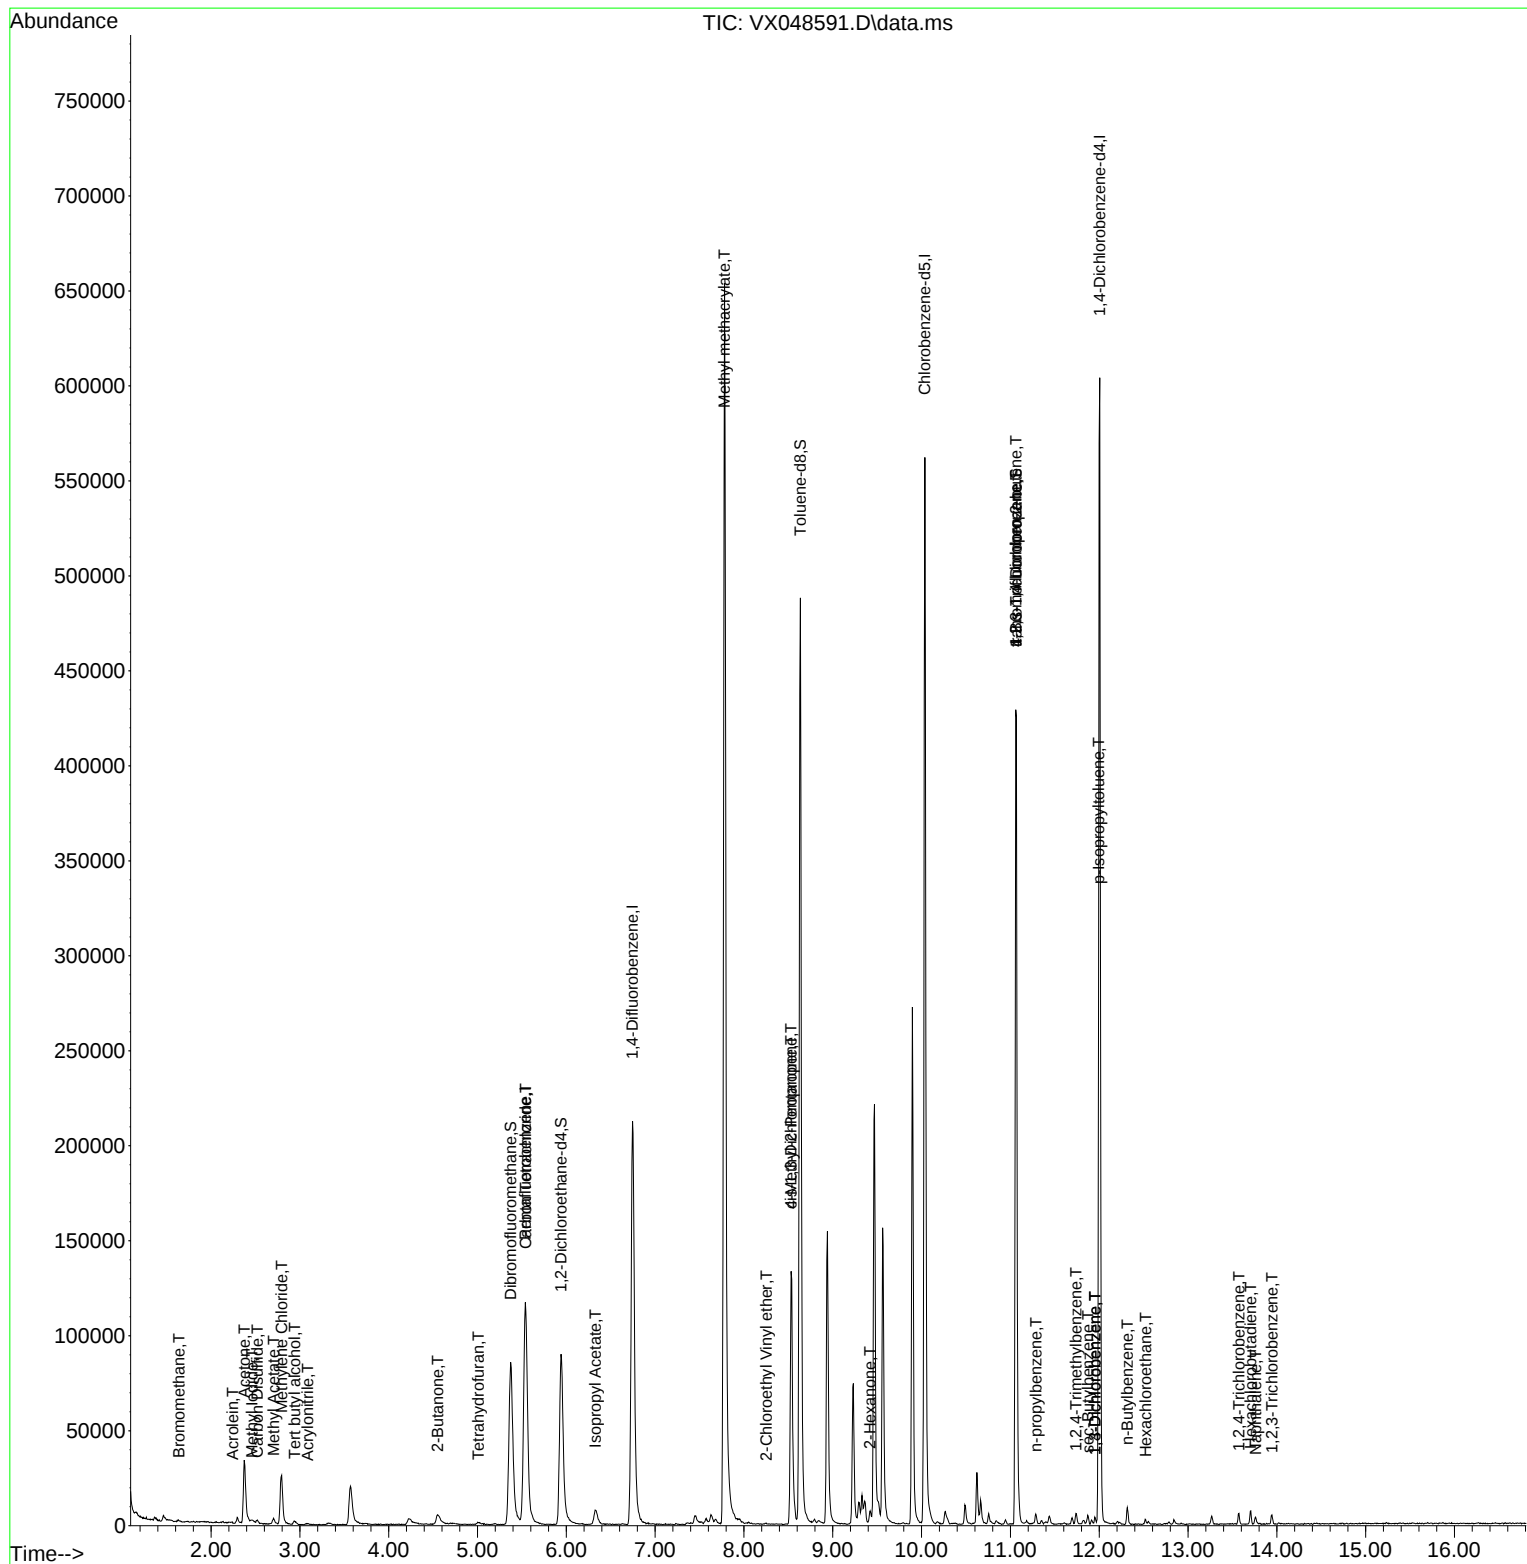




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.538 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion:168 Resp: 118773
Ion Ratio Lower Upper
168 100
99 62.0 45.2 67.8

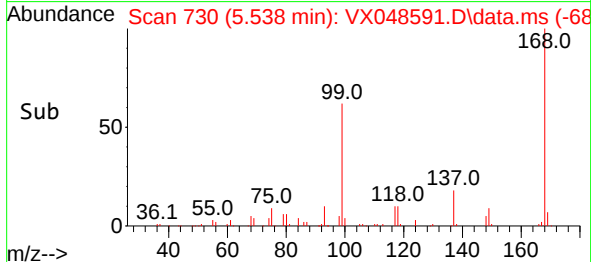

#5
Bromomethane
Concen: 0.535 ug/l
RT: 1.636 min Scan# 90
Delta R.T. 0.024 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 94 Resp: 488
Ion Ratio Lower Upper
94 100
96 39.2 72.3 108.5#


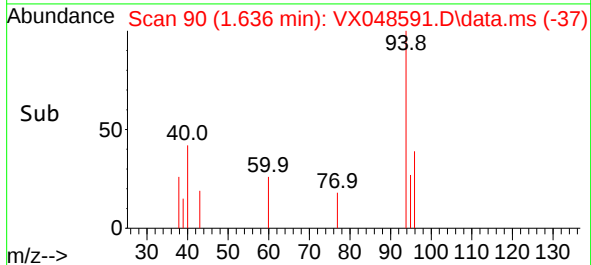




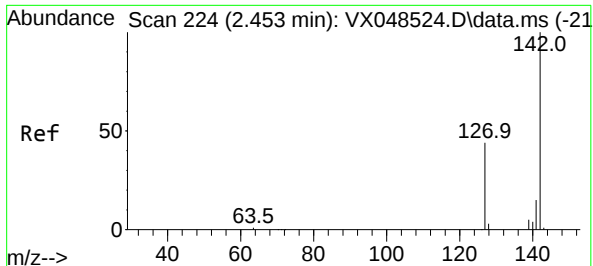

#10
Methyl Iodide
Concen: 0.501 ug/l
RT: 2.459 min Scan# 21
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion:142 Resp: 982
Ion Ratio Lower Upper
142 100
127 50.5 35.8 53.6
141 0.0 11.4 17.0#

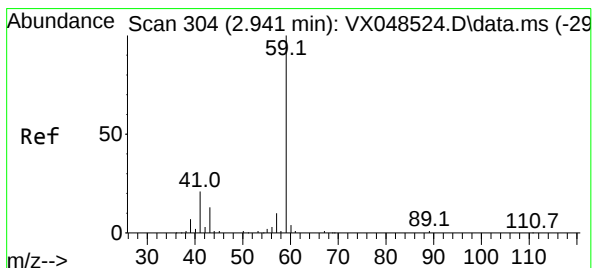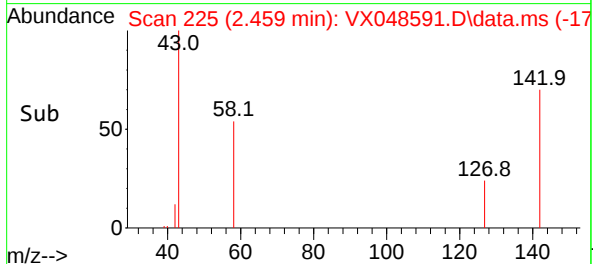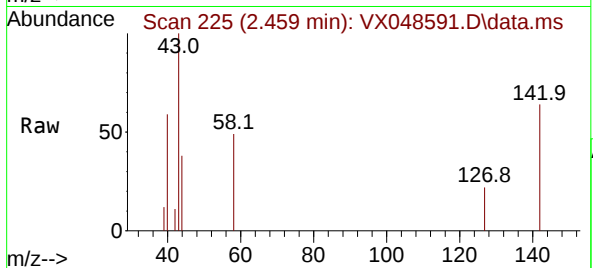

#11
Tert butyl alcohol
Concen: 6.355 ug/l
RT: 2.940 min Scan# 304
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 59 Resp: 1993
Ion Ratio Lower Upper
59 100
57 3.7 8.6 13.0#


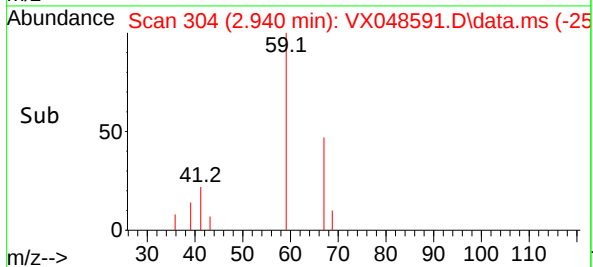
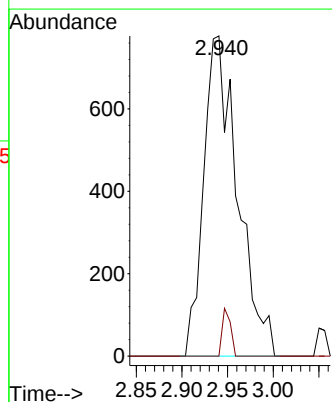
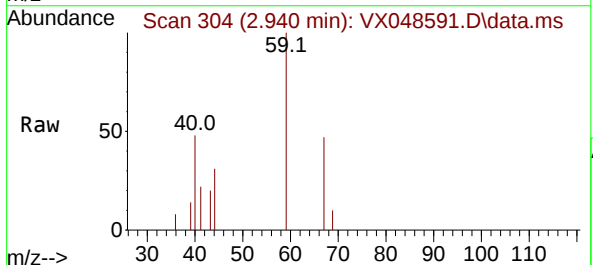




#13
Acrolein
Concen: 3.107 ug/l
RT: 2.239 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 56 Resp: 141
Ion Ratio Lower Upper
56 100
55 0.0 54.9 82.3#

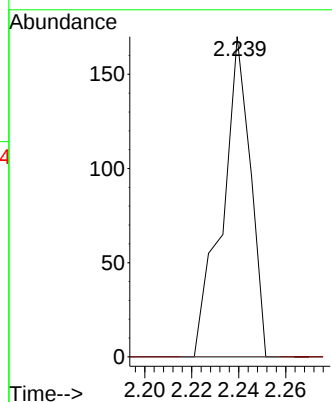

#15
Acrylonitrile
Concen: 0.468 ug/l
RT: 3.087 min Scan# 328
Delta R.T. 0.030 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 53 Resp: 428
Ion Ratio Lower Upper
53 100
52 50.0 65.3 97.9#
51 0.0 27.8 41.6#









#16
Acetone
Concen: 58.749 ug/l
RT: 2.373 min Scan# 211
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 43 Resp: 46024
Ion Ratio Lower Upper
43 100
58 27.4 25.8 38.6

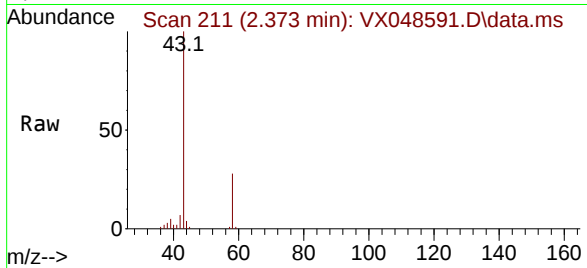

#17
Carbon Disulfide
Concen: 0.440 ug/l
RT: 2.520 min Scan# 235
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 76 Resp: 1712
Ion Ratio Lower Upper
76 100
78 5.5 7.1 10.7#

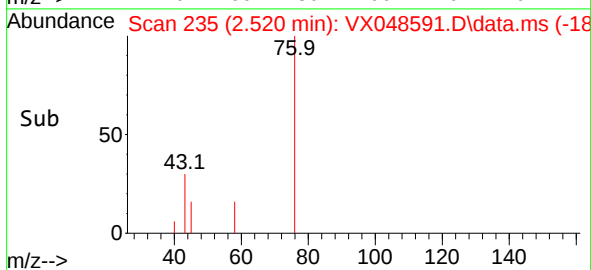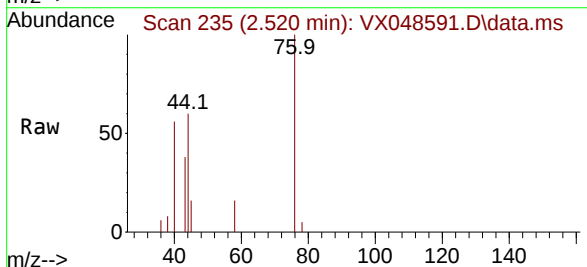



#18

Methyl Acetate

Concen: 1.886 ug/l

RT: 2.703 min Scan# 2

Delta R.T. 0.006 min

Lab File: VX048591.D

Acq: 13 Nov 2025 13:41

Instrument :

MSVOA_X

ClientSampleId :





PB170518TB

Tgt Ion: 43 Resp: 4060

Ion Ratio Lower Upper

43 100

74 22.5 19.1 28.7

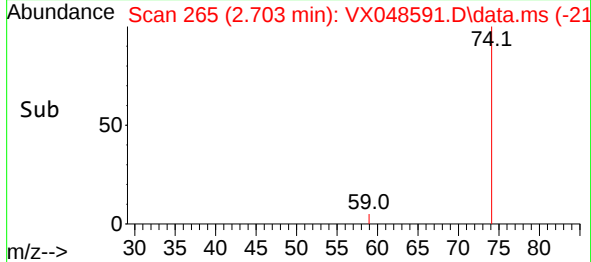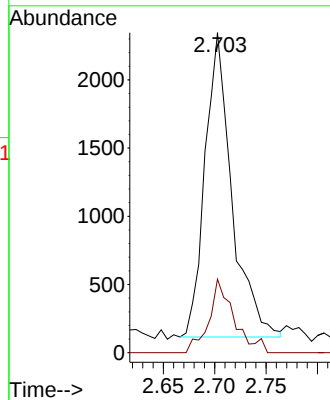

#20

Methylene Chloride

Concen: 8.097 ug/l

RT: 2.794 min Scan# 280

Delta R.T. 0.006 min

Lab File: VX048591.D

Acq: 13 Nov 2025 13:41

Tgt Ion: 84 Resp: 13041




Ion Ratio Lower Upper


84 100

49 130.2 91.2 136.8

51 43.3 28.3 42.5#

86 71.9 49.4 74.2


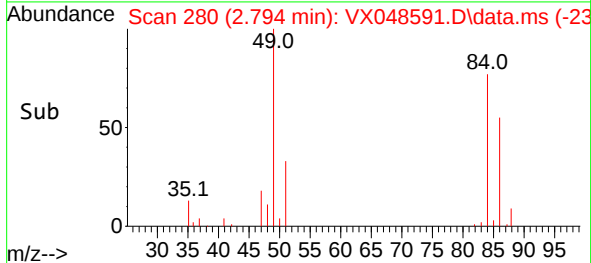
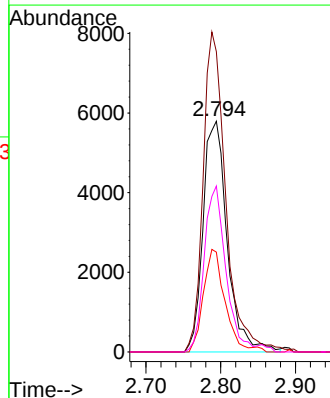





#25
2-Butanone
Concen: 9.440 ug/l
RT: 4.550 min Scan# 568
Delta R.T. 0.012 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 43 Resp: 10940
Ion Ratio Lower Upper
43 100
72 22.5 21.5 32.3



#29
Tetrahydrofuran
Concen: 0.514 ug/l
RT: 5.007 min Scan# 643
Delta R.T. 0.018 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 42 Resp: 425
Ion Ratio Lower Upper
42 100
72 90.8 36.3 54.5#
71 44.5 34.1 51.1









#33
 1,2-Dichloroethane-d4
 Concen: 60.182 ug/l
 RT: 5.940 min Scan# 797
 Delta R.T. -0.006 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41




Instrument :
 MSVOA_X
 ClientSampleId :
 PB170518TB


Tgt Ion: 65 Resp: 99602
 Ion Ratio Lower Upper
 65 100
 67 50.3 0.0 106.2

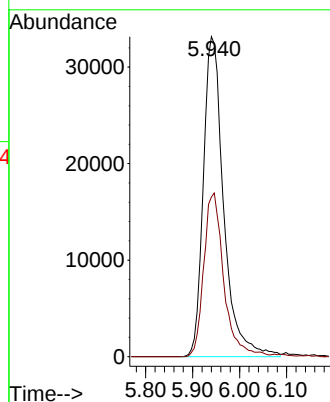

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 6.745 min Scan# 928
 Delta R.T. -0.000 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41

Tgt Ion: 114 Resp: 235440
 Ion Ratio Lower Upper
 114 100
 63 22.0 0.0 41.2
 88 16.5 0.0 32.2



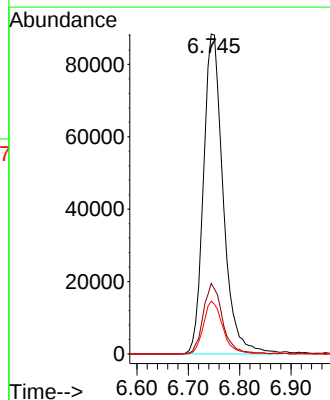
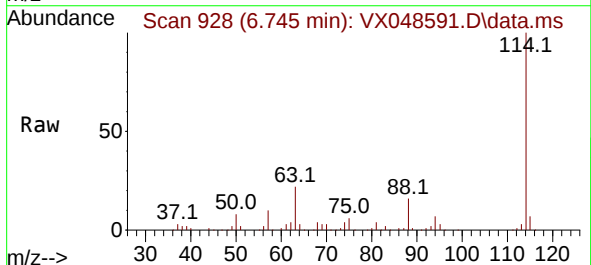




#35
Dibromofluoromethane
Concen: 47.247 ug/l
RT: 5.373 min Scan# 703
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion:113 Resp: 84193
Ion Ratio Lower Upper
113 100
111 100.0 81.9 122.9
192 19.5 15.8 23.6

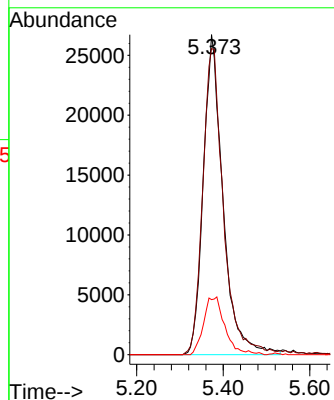

#38
Carbon Tetrachloride
Concen: 4.570 ug/l
RT: 5.544 min Scan# 731
Delta R.T. -0.122 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion:117 Resp: 12413
Ion Ratio Lower Upper
117 100
119 4.2 74.5 111.7#
121 0.0 24.8 37.2#



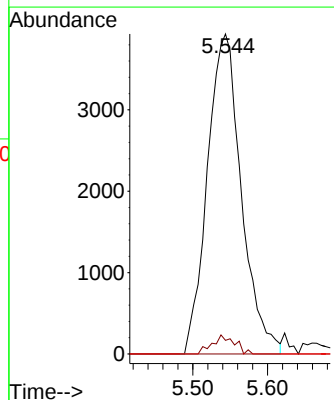





#43
Isopropyl Acetate
Concen: 2.705 ug/l
RT: 6.324 min Scan# 81
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion:	43	Resp:	12772
Ion	Ratio	Lower	Upper
43	100		
61	19.1	16.2	24.4
87	11.8	10.9	16.3

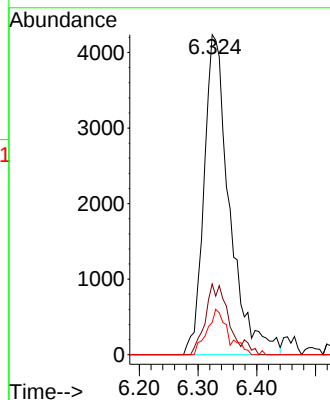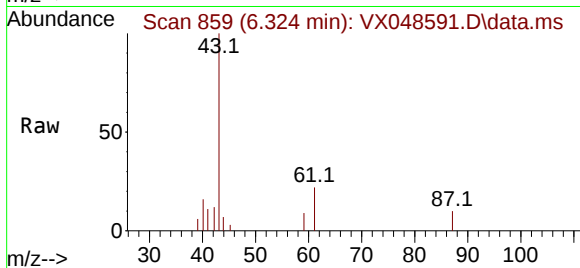

#48
Methyl methacrylate
Concen: 29.881 ug/l
RT: 7.781 min Scan# 1098
Delta R.T. 0.103 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion:	41	Resp:	62716
Ion	Ratio	Lower	Upper
41	100		
69	0.0	67.9	101.9#
39	54.2	42.2	63.2



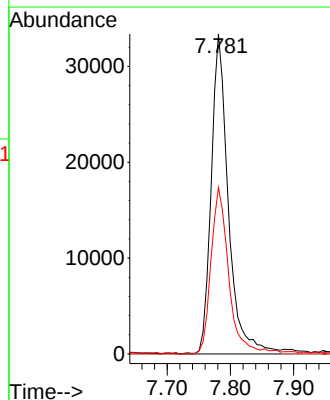
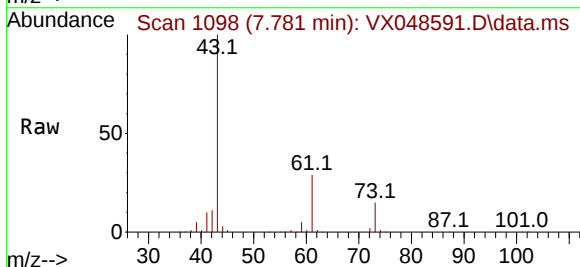




#50
Toluene-d8
Concen: 54.399 ug/l
RT: 8.635 min Scan# 11
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 98 Resp: 302330
Ion Ratio Lower Upper
98 100
100 65.2 53.6 80.4

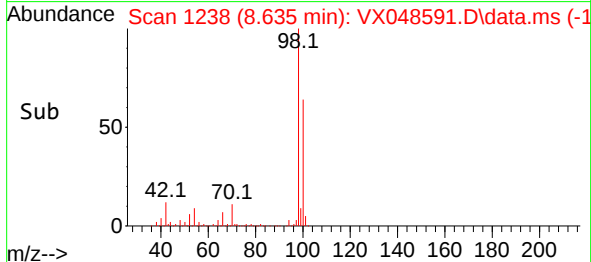

#51
4-Methyl-2-Pentanone
Concen: 20.227 ug/l
RT: 8.531 min Scan# 1221
Delta R.T. -0.025 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 43 Resp: 54363
Ion Ratio Lower Upper
43 100
58 9.1 32.3 48.5#


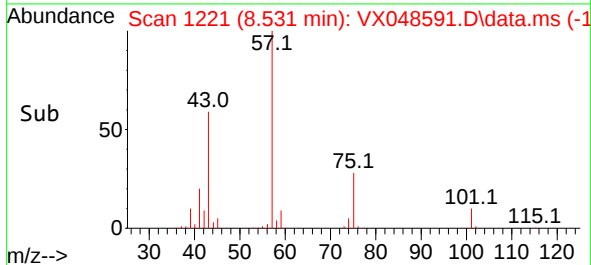




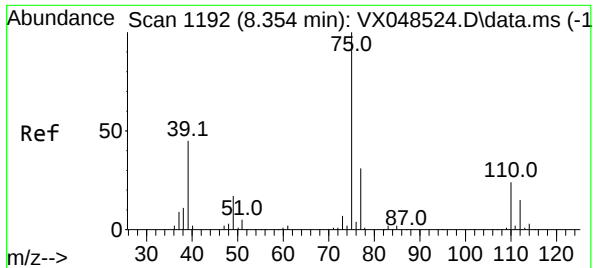

#54
 cis-1,3-Dichloropropene
 Concen: 8.586 ug/l
 RT: 8.531 min Scan# 1192
 Delta R.T. 0.177 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41




Instrument :
 MSVOA_X
 ClientSampleId :
 PB170518TB


Tgt Ion: 75 Resp: 22669
 Ion Ratio Lower Upper
 75 100
 77 0.6 24.7 37.1#
 39 34.7 36.1 54.1#

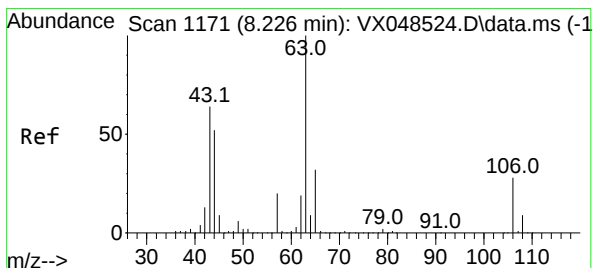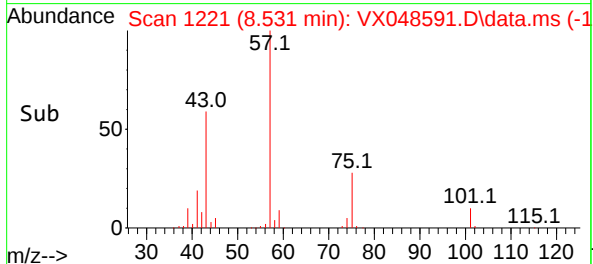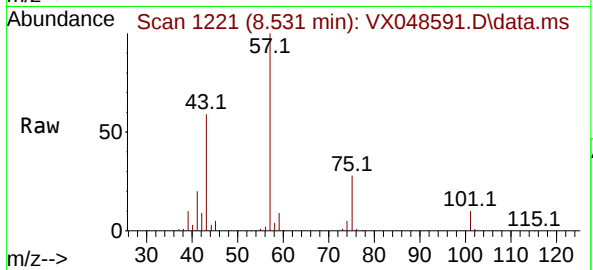

#58
 2-Chloroethyl Vinyl ether
 Concen: 0.209 ug/l
 RT: 8.250 min Scan# 1175
 Delta R.T. 0.024 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41

Tgt Ion: 63 Resp: 291
 Ion Ratio Lower Upper
 63 100
 106 0.0 23.0 34.4#


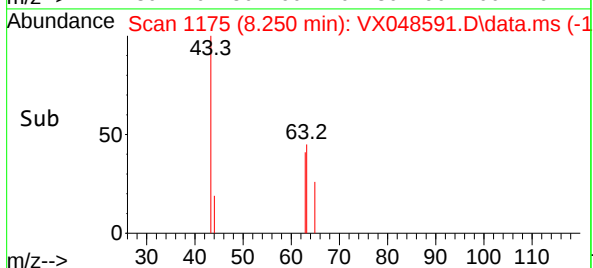

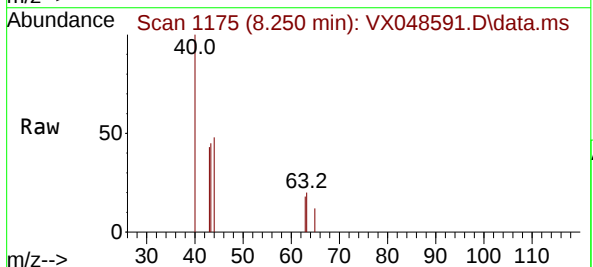


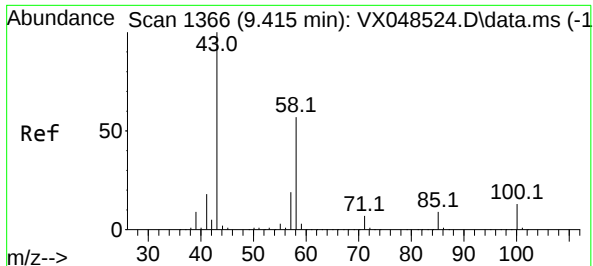

#59
2-Hexanone
Concen: 2.130 ug/l
RT: 9.421 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 43 Resp: 4259
Ion Ratio Lower Upper
43 100
58 53.7 28.1 84.2

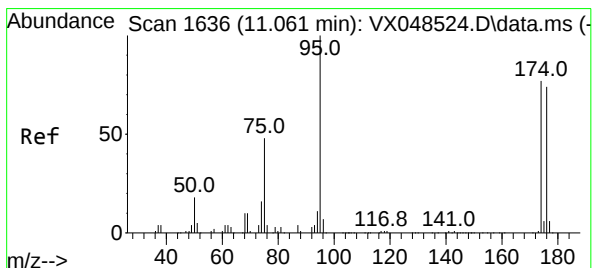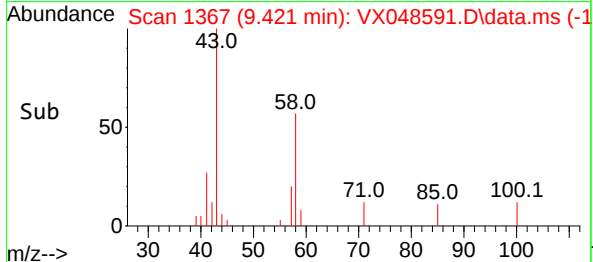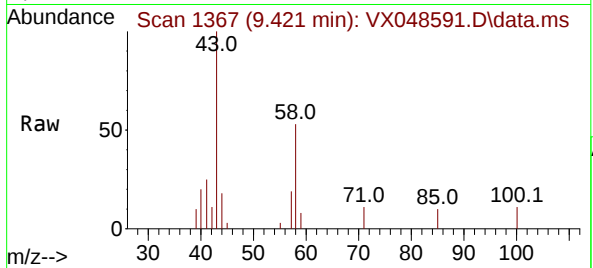

#62
4-Bromofluorobenzene
Concen: 60.036 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 95 Resp: 124344
Ion Ratio Lower Upper
95 100
174 79.8 0.0 161.8
176 77.6 0.0 153.6


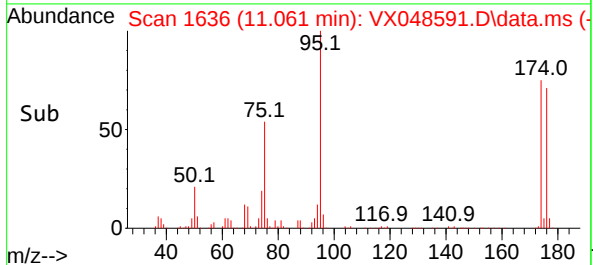

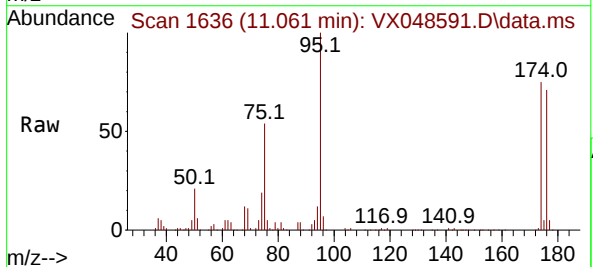




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.037 min Scan# 1468
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion:117 Resp: 256905
Ion Ratio Lower Upper
117 100
82 57.3 44.4 66.6
119 33.1 25.1 37.7

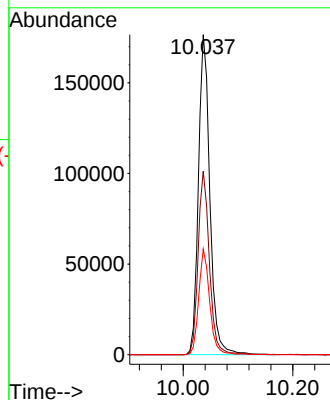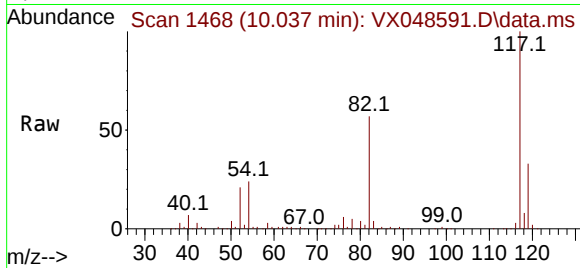

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.006 min Scan# 1791
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion:152 Resp: 130936
Ion Ratio Lower Upper
152 100
115 58.9 39.2 117.6
150 156.3 0.0 347.0



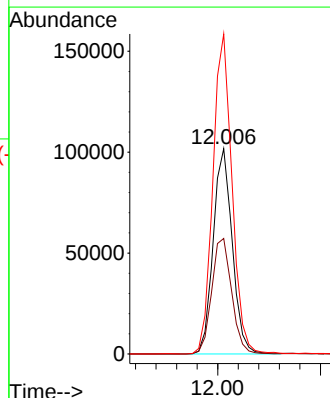
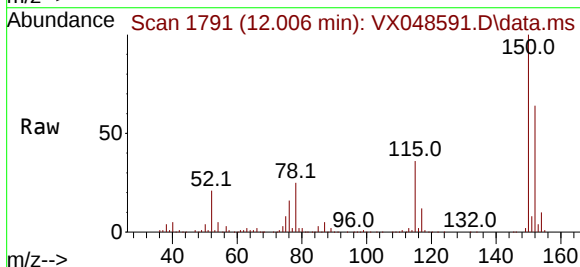




#76
1,2,3-Trichloropropane
Concen: 20.962 ug/l
RT: 11.061 min Scan# 1636
Delta R.T. -0.159 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 75 Resp: 66125
Ion Ratio Lower Upper
75 100
77 1.1 24.3 72.8#

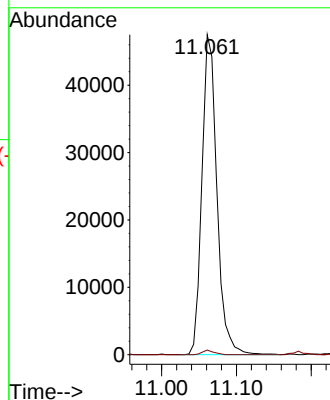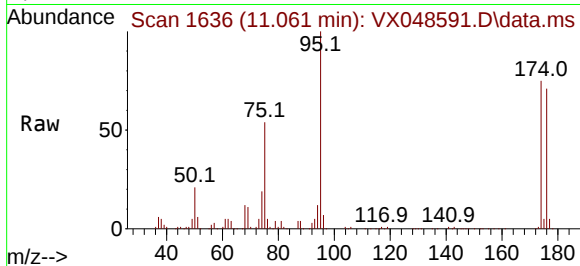

#78
n-propylbenzene
Concen: 0.200 ug/l
RT: 11.287 min Scan# 1673
Delta R.T. -0.000 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 91 Resp: 2238
Ion Ratio Lower Upper
91 100
120 26.4 11.6 34.8



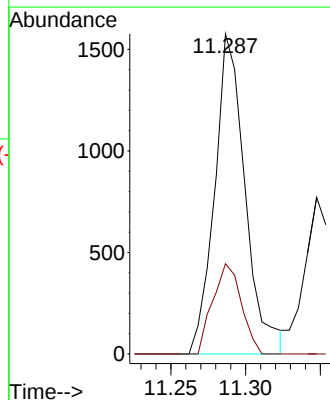
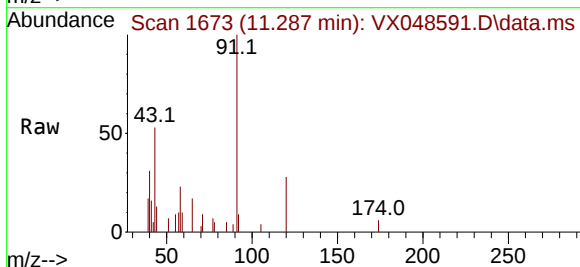




#81
trans-1,4-Dichloro-2-butene
Concen: 59.959 ug/l
RT: 11.061 min Scan# 1
Delta R.T. 0.061 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 75 Resp: 66125
Ion Ratio Lower Upper
75 100
53 0.0 72.4 108.6#
89 0.0 43.6 65.4#

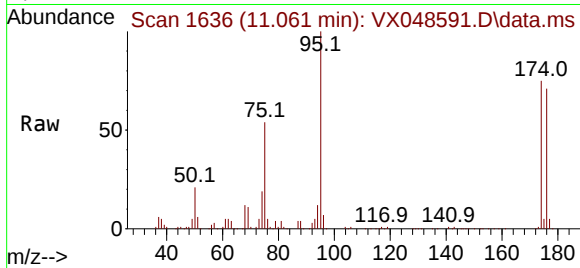

#84
1,2,4-Trimethylbenzene
Concen: 0.203 ug/l
RT: 11.738 min Scan# 1747
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 105 Resp: 1584
Ion Ratio Lower Upper
105 100
120 43.8 22.4 67.0


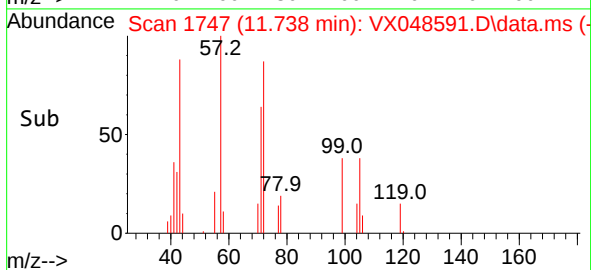

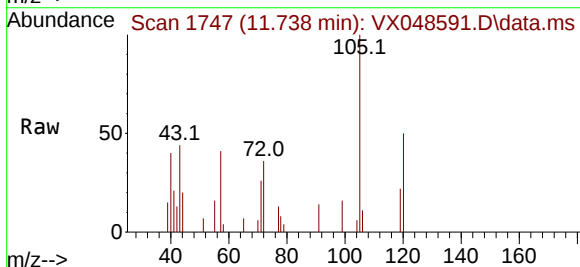




#85
 sec-Butylbenzene
 Concen: 0.277 ug/l
 RT: 11.872 min Scan# 1769
 Delta R.T. -0.000 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41




Instrument :
 MSVOA_X
 ClientSampleId :
 PB170518TB


Tgt Ion:105 Resp: 2740
 Ion Ratio Lower Upper
 105 100
 134 20.1 10.2 30.4

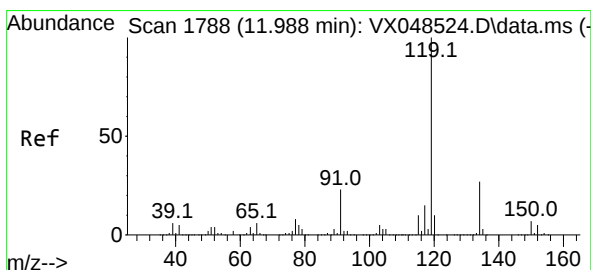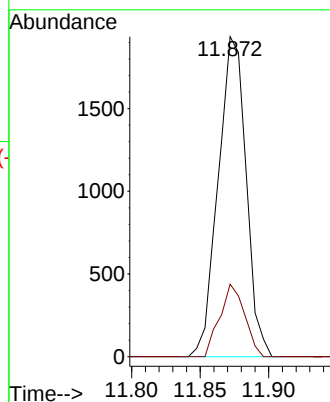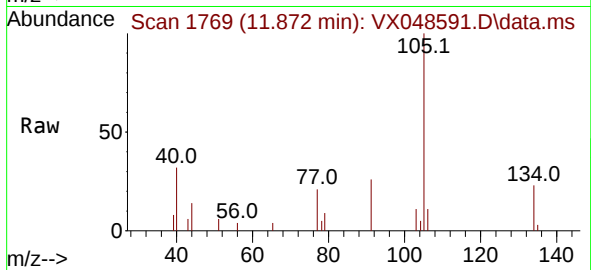

#86
 p-Isopropyltoluene
 Concen: 0.309 ug/l
 RT: 11.994 min Scan# 1789
 Delta R.T. 0.006 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41

Tgt Ion:119 Resp: 2577
 Ion Ratio Lower Upper
 119 100
 134 28.6 13.2 39.5
 91 39.5 11.3 33.9#

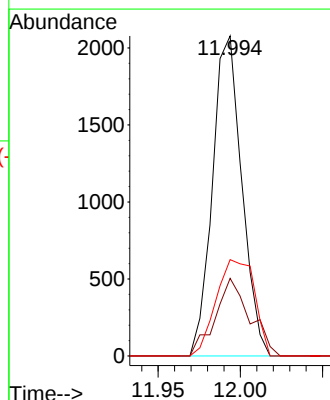



#87

1,3-Dichlorobenzene

Concen: 0.276 ug/l

RT: 11.951 min Scan# 1782

Delta R.T. -0.000 min

Lab File: VX048591.D

Acq: 13 Nov 2025 13:41

Instrument :

MSVOA_X

ClientSampleId :

PB170518TB





Tgt Ion:146 Resp: 1271

Ion Ratio Lower Upper

146 100

111 45.5 19.8 59.4

148 64.4 31.6 95.0

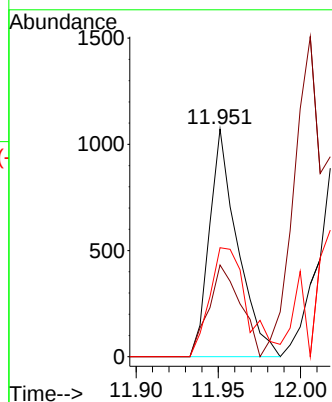

#88

1,4-Dichlorobenzene

Concen: 0.268 ug/l

RT: 11.951 min Scan# 1782

Delta R.T. -0.073 min

Lab File: VX048591.D

Acq: 13 Nov 2025 13:41




Tgt Ion:146 Resp: 1271


Ion Ratio Lower Upper

146 100

111 45.5 19.2 57.6

148 64.4 31.9 95.9


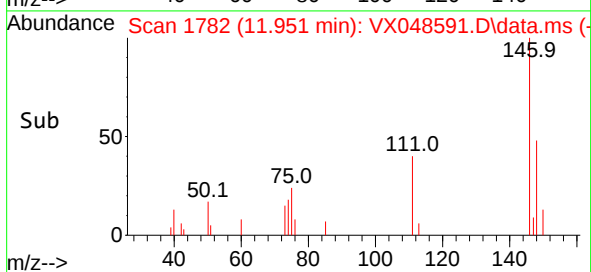
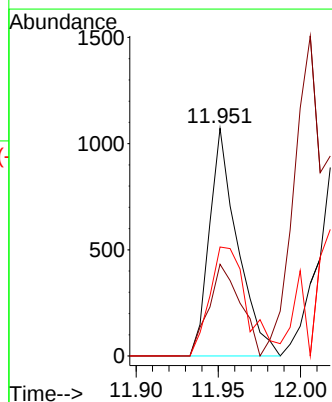





#89
n-Butylbenzene
Concen: 0.442 ug/l
RT: 12.317 min Scan# 1841
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41




Instrument :
MSVOA_X
ClientSampleId :
PB170518TB


Tgt Ion: 91 Resp: 3450
Ion Ratio Lower Upper
91 100
92 46.6 27.2 81.5
134 23.1 13.0 39.0

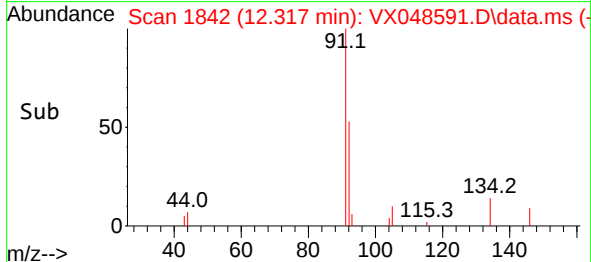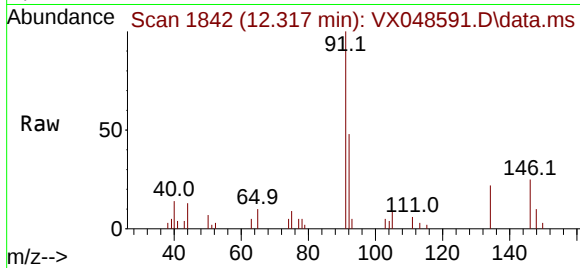

#90
Hexachloroethane
Concen: 0.302 ug/l
RT: 12.524 min Scan# 1876
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion: 117 Resp: 479
Ion Ratio Lower Upper
117 100
201 63.3 35.9 107.8




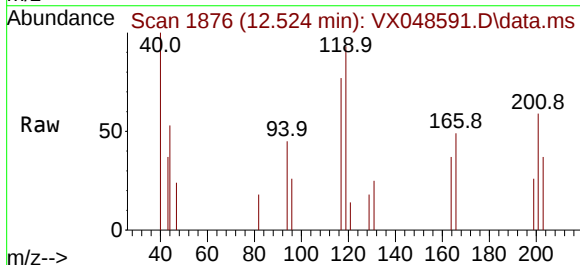




#93
 1,2,4-Trichlorobenzene
 Concen: 0.488 ug/l
 RT: 13.573 min Scan# 2047
 Delta R.T. 0.006 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41




Instrument :
 MSVOA_X
 ClientSampleId :
 PB170518TB


Tgt Ion:180 Resp: 1432
 Ion Ratio Lower Upper
 180 100
 182 113.0 47.5 142.6
 145 31.6 15.9 47.7

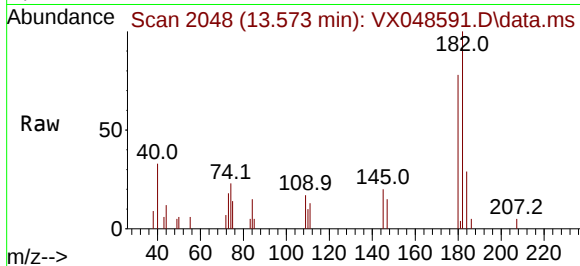

#94
 Hexachlorobutadiene
 Concen: 0.855 ug/l
 RT: 13.707 min Scan# 2070
 Delta R.T. -0.000 min
 Lab File: VX048591.D
 Acq: 13 Nov 2025 13:41

Tgt Ion:225 Resp: 1049
 Ion Ratio Lower Upper
 225 100
 223 62.9 30.6 92.0
 227 50.1 32.5 97.4


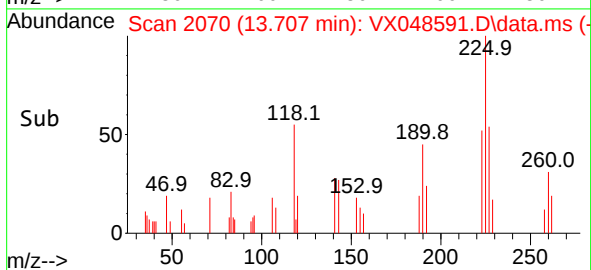

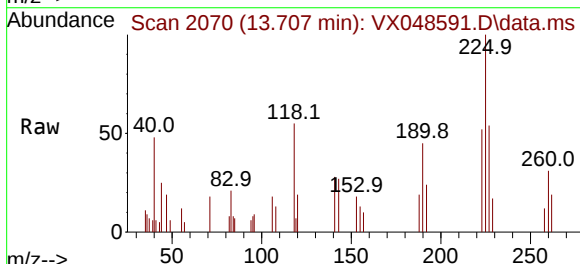




#95
Naphthalene
Concen: 0.301 ug/l
RT: 13.762 min Scan# 2078
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Instrument :
MSVOA_X
ClientSampleId :
PB170518TB

Tgt Ion:128 Resp: 2842
Ion Ratio Lower Upper
128 100
127 15.0 10.1 15.1
129 8.2 8.7 13.1#

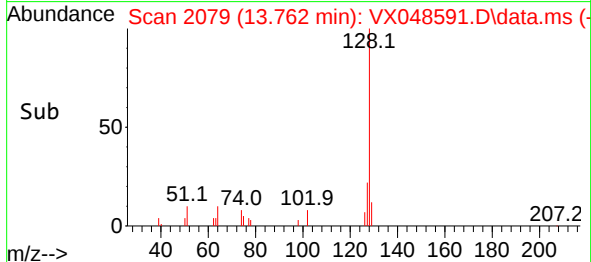

#96
1,2,3-Trichlorobenzene
Concen: 0.543 ug/l
RT: 13.945 min Scan# 2109
Delta R.T. 0.006 min
Lab File: VX048591.D
Acq: 13 Nov 2025 13:41

Tgt Ion:180 Resp: 1482
Ion Ratio Lower Upper
180 100
182 86.5 47.3 142.0
145 30.1 16.7 50.0

