

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111418\
 Data File : VX005985.D
 Acq On : 14 Nov 2018 20:08
 Operator : JC/MD
 Sample : J5921-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-UST-MIDDLEDL

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.934	286	292	303	rVB	4718	9871	1.74%	0.153%
2	4.397	522	532	541	rBV2	9935	29080	5.12%	0.451%
3	5.501	701	713	721	rBV2	70393	206189	36.31%	3.197%
4	5.580	721	726	731	rVV2	17352	45496	8.01%	0.706%
5	5.665	731	740	754	rVB2	128327	351401	61.88%	5.449%
6	6.061	795	805	815	rBV3	77445	208709	36.75%	3.236%
7	6.141	815	818	827	rVB3	6157	13644	2.40%	0.212%
8	6.299	831	844	851	rBV8	1796	6584	1.16%	0.102%
9	6.452	860	869	877	rVB3	4379	10924	1.92%	0.169%
10	6.860	926	936	948	rBV	177578	422634	74.43%	6.554%
11	7.458	1025	1034	1046	rVB2	17736	40626	7.15%	0.630%
12	8.214	1151	1158	1163	rBV	6647	11215	1.98%	0.174%
13	8.573	1210	1217	1224	rVB	6631	11297	1.99%	0.175%
14	8.713	1234	1240	1256	rVB	356480	567843	100.00%	8.806%
15	9.024	1286	1291	1298	rVB4	4605	10251	1.81%	0.159%
16	9.110	1300	1305	1310	rVV3	3592	5723	1.01%	0.089%
17	9.219	1319	1323	1329	rBV	4210	6243	1.10%	0.097%
18	10.116	1464	1470	1479	rBV	337273	481181	84.74%	7.462%
19	10.268	1490	1495	1500	rBV5	3388	5788	1.02%	0.090%
20	10.359	1500	1510	1517	rVB	72814	96177	16.94%	1.491%
21	10.475	1522	1529	1540	rVB5	5873	10913	1.92%	0.169%
22	10.926	1597	1603	1611	rBV6	2470	6739	1.19%	0.105%
23	11.140	1632	1638	1649	rBV	296604	389339	68.56%	6.038%
24	11.457	1685	1690	1694	rBV	16191	20565	3.62%	0.319%
25	11.670	1720	1725	1733	rBV	13284	20404	3.59%	0.316%
26	11.762	1733	1740	1743	rBV3	9299	13587	2.39%	0.211%
27	11.804	1743	1747	1753	rVB	398517	485771	85.55%	7.533%
28	12.079	1786	1792	1798	rBV	405933	491526	86.56%	7.622%
29	12.140	1798	1802	1807	rVB	46280	59203	10.43%	0.918%
30	12.298	1823	1828	1836	rVV	293235	353389	62.23%	5.480%
31	12.371	1836	1840	1846	rVB2	8179	12779	2.25%	0.198%
32	12.463	1847	1855	1859	rBV3	14499	20959	3.69%	0.325%
33	12.518	1859	1864	1869	rVB	19671	23689	4.17%	0.367%
34	12.585	1869	1875	1877	rBV	70198	86085	15.16%	1.335%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111418\
 Data File : VX005985.D
 Acq On : 14 Nov 2018 20:08
 Operator : JC/MD
 Sample : J5921-08DL 20X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 SP-UST-MIDDLEDL

Integration Parameters: RTEINT.P

Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260

35	12.609	1877	1879	1884	rVB	46781	51238	9.02%	0.795%
36	12.670	1884	1889	1892	rBV	87005	108447	19.10%	1.682%
37	12.701	1892	1894	1898	rVV	36223	39605	6.97%	0.614%
38	12.755	1898	1903	1910	rVB	175065	233924	41.20%	3.627%
39	12.902	1922	1927	1933	rVB2	13473	19325	3.40%	0.300%
40	12.975	1933	1939	1943	rBV	87800	112610	19.83%	1.746%
41	13.018	1943	1946	1951	rVV	137549	160342	28.24%	2.486%
42	13.091	1951	1958	1962	rVV3	9556	19790	3.49%	0.307%
43	13.146	1965	1967	1971	rVV2	5574	6374	1.12%	0.099%
44	13.194	1971	1975	1977	rVV2	12342	16139	2.84%	0.250%
45	13.225	1977	1980	1990	rVV	60694	81389	14.33%	1.262%
46	13.310	1990	1994	1996	rVV2	12071	17932	3.16%	0.278%
47	13.347	1996	2000	2006	rVV2	271110	376572	66.32%	5.840%
48	13.402	2006	2009	2012	rVV2	12881	19845	3.49%	0.308%
49	13.481	2016	2022	2029	rVB	53287	68609	12.08%	1.064%
50	13.560	2030	2035	2038	rBV2	11012	15496	2.73%	0.240%
51	13.603	2038	2042	2045	rVV	37800	55276	9.73%	0.857%
52	13.639	2045	2048	2054	rVV3	38697	71303	12.56%	1.106%
53	13.719	2054	2061	2068	rVB2	43370	89046	15.68%	1.381%
54	13.834	2073	2080	2088	rVB	94534	123792	21.80%	1.920%
55	13.914	2088	2093	2100	rBV4	3985	7234	1.27%	0.112%
56	13.987	2100	2105	2108	rBV2	8818	12223	2.15%	0.190%
57	14.030	2108	2112	2116	rVB	13976	16521	2.91%	0.256%
58	14.133	2124	2129	2133	rBV	26043	32169	5.67%	0.499%
59	14.273	2146	2152	2157	rBV	20962	35506	6.25%	0.551%
60	14.377	2165	2169	2174	rBV	7840	12021	2.12%	0.186%
61	14.432	2174	2178	2183	rVB2	15111	20016	3.52%	0.310%
62	14.542	2191	2196	2201	rBV2	5139	7313	1.29%	0.113%
63	14.658	2208	2215	2218	rBV	12785	16562	2.92%	0.257%
64	14.694	2218	2221	2227	rVB	19797	24212	4.26%	0.375%
65	14.840	2240	2245	2254	rVB2	27868	42018	7.40%	0.652%


Sum of corrected areas: 6448673

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_X\DATA\VX111418\
Data File : VX005985.D
Acq On : 14 Nov 2018 20:08
Operator : JC/MD
Sample : J5921-08DL 20X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
SP-UST-MIDDLEDL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

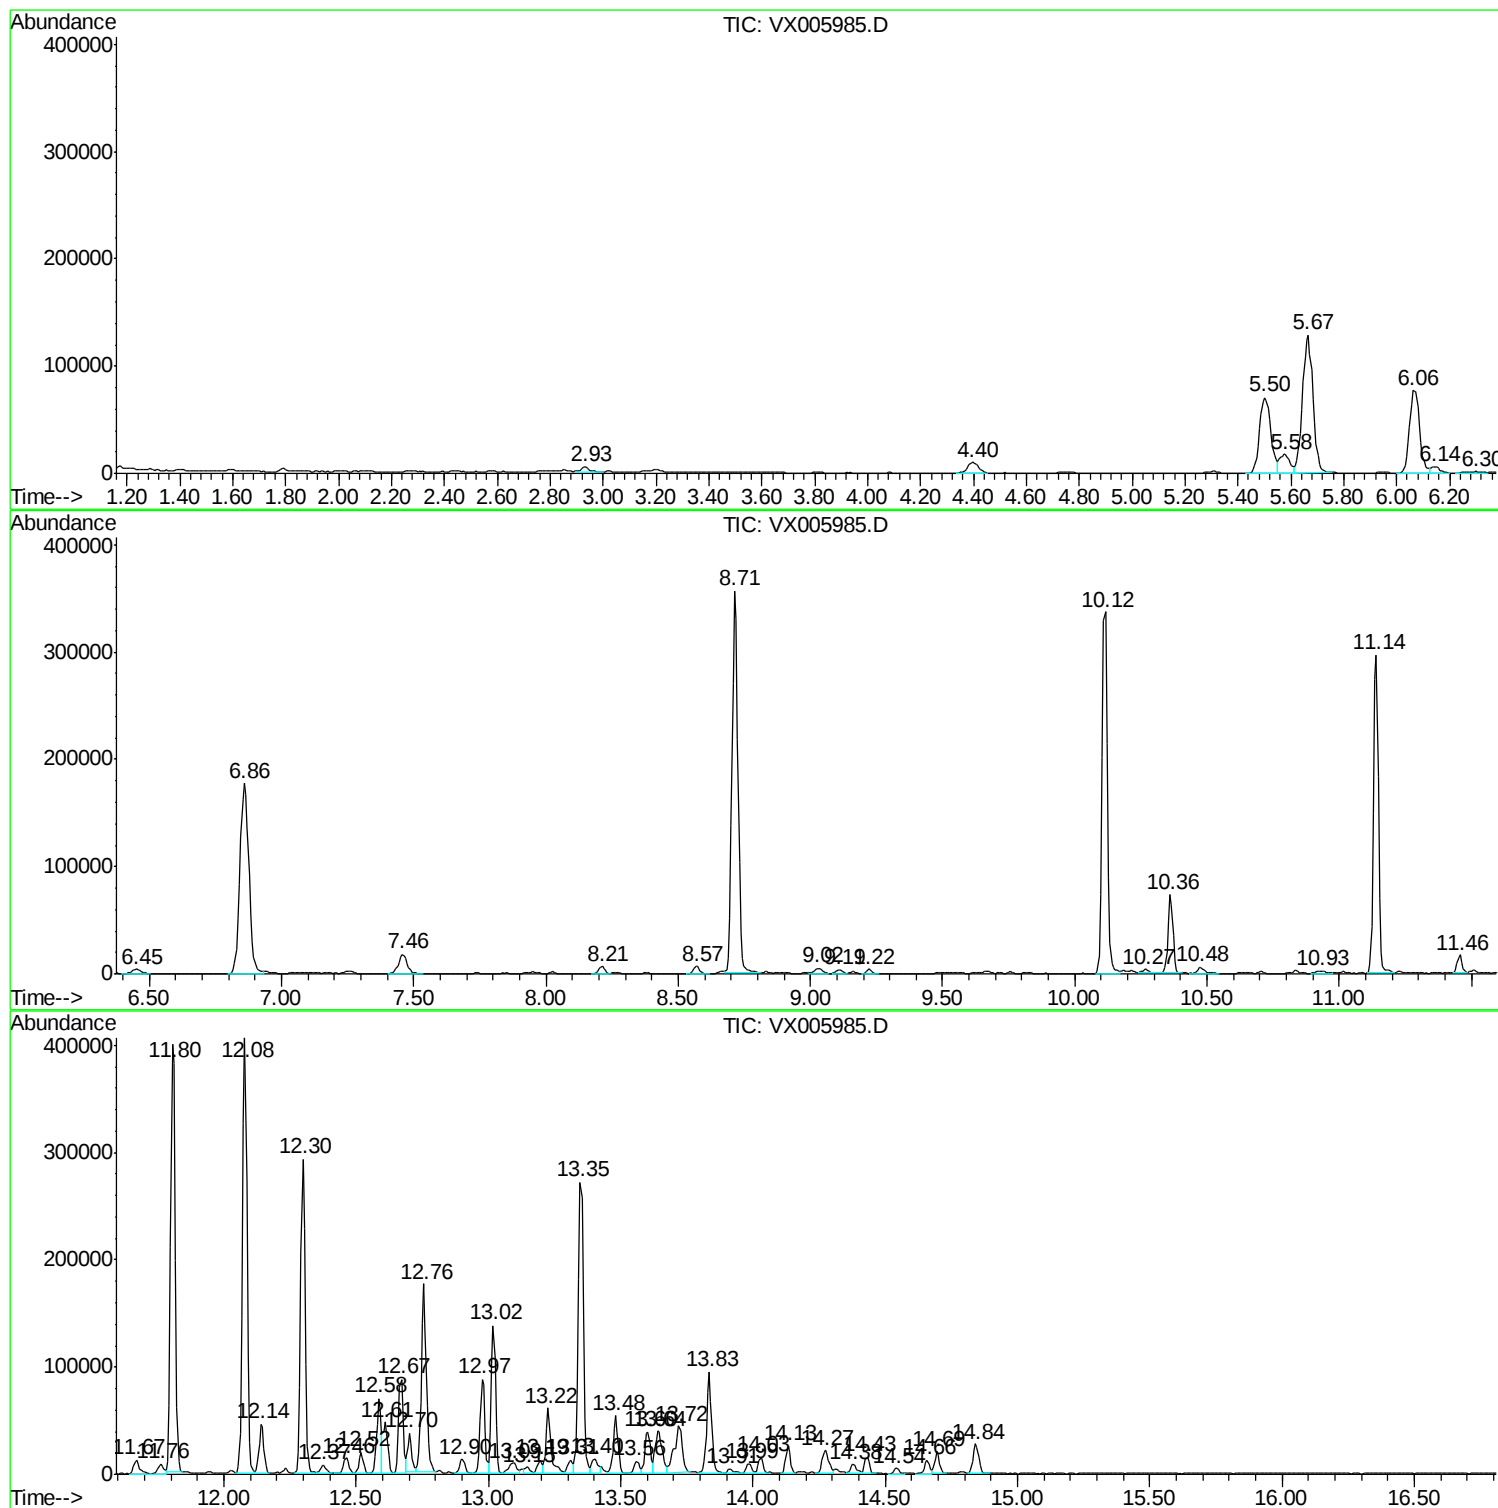

Instrument :
MSVOA_X
ClientSampleId :
SP-UST-MIDDLEDL

```
TTCCLibbaary ::CC\DATA\BBSSENNSSIT11LL
TTCCLibbaary ::CC\DATA\BBSSENNSSIT11LL
```
