


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111418\
Data File : VX005966.D
Acq On : 14 Nov 2018 09:56
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Title : SW846 8260
Last Update : Wed Nov 07 14:40:53 2018

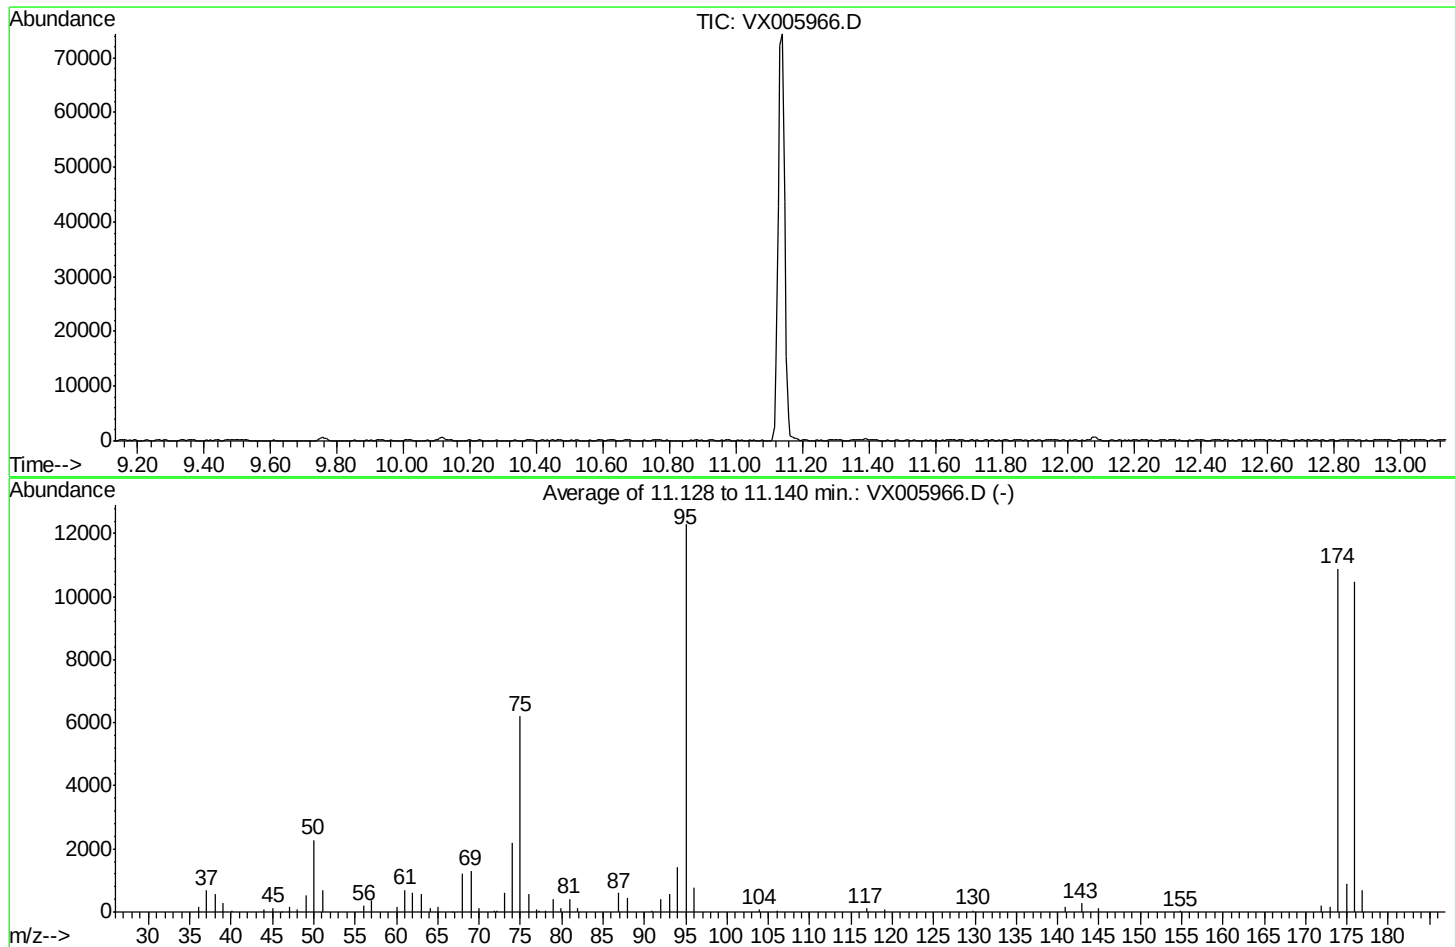

AutoFind: Scans 1636, 1637, 1638; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	2283	PASS
75	95	30	60	50.4	6195	PASS
95	95	100	100	100.0	12293	PASS
96	95	5	9	6.4	786	PASS
173	174	0.00	2	1.6	170	PASS
174	95	50	100	88.6	10897	PASS
175	174	5	9	8.2	897	PASS
176	174	95	101	96.3	10491	PASS
177	176	5	9	6.7	698	PASS