


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111418\
 Data File : VX005989.D
 Acq On : 14 Nov 2018 22:21
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
 Title : SW846 8260
 Last Update : Wed Nov 07 14:40:53 2018

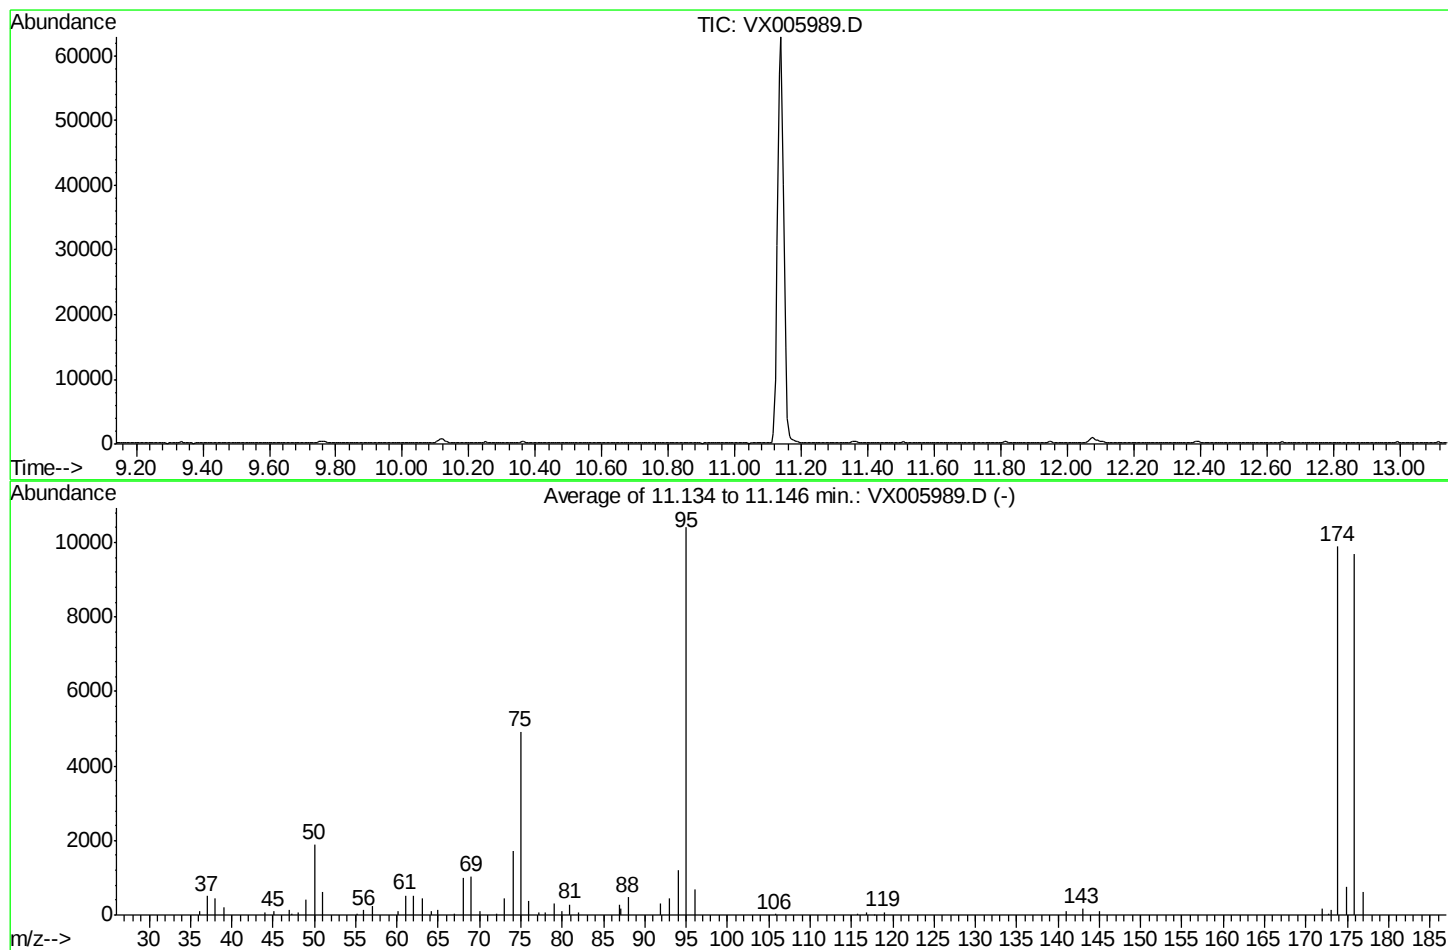

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	1887	PASS
75	95	30	60	47.2	4915	PASS
95	95	100	100	100.0	10409	PASS
96	95	5	9	6.7	698	PASS
173	174	0.00	2	1.3	125	PASS
174	95	50	100	95.0	9890	PASS
175	174	5	9	7.5	742	PASS
176	174	95	101	98.0	9695	PASS
177	176	5	9	6.3	606	PASS