

Data Path : Z:\VOASRV\HPCHEM1\MSVOA X\DATA\VX111419\
Data File : VX013421.D
Acq On : 14 Nov 2019 14:49
Operator : JC/SP
Sample : K5828-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
REP111319

Integration Parameters: RTEINT3.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA X\METHOD\624X111119W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.594	274	280	290	rVB	197518	347066	1.17%	0.713%
2	3.161	360	373	387	rBV2	621144	1821251	6.13%	3.743%
3	4.587	594	607	626	rBV	10838742	29722904	100.00%	61.085%
4	5.008	663	676	689	rBV	254953	751028	2.53%	1.543%
5	6.051	838	847	856	rBV	270830	681855	2.29%	1.401%
6	6.849	970	978	991	rBV	593773	1380634	4.65%	2.837%
7	7.209	1028	1037	1047	rBV	3650725	7689429	25.87%	15.803%
8	8.709	1277	1283	1294	rBV	1243282	1920066	6.46%	3.946%
9	9.330	1379	1385	1397	rBV	1114673	1609749	5.42%	3.308%
10	10.111	1507	1513	1520	rBV	1135435	1571559	5.29%	3.230%
11	11.135	1676	1681	1690	rVB	900127	1163037	3.91%	2.390%




Sum of corrected areas: 48658578

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX111419\
Data File : VX013421.D
Acq On : 14 Nov 2019 14:49
Operator : JC/SP
Sample : K5828-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
REP111319

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X111119W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

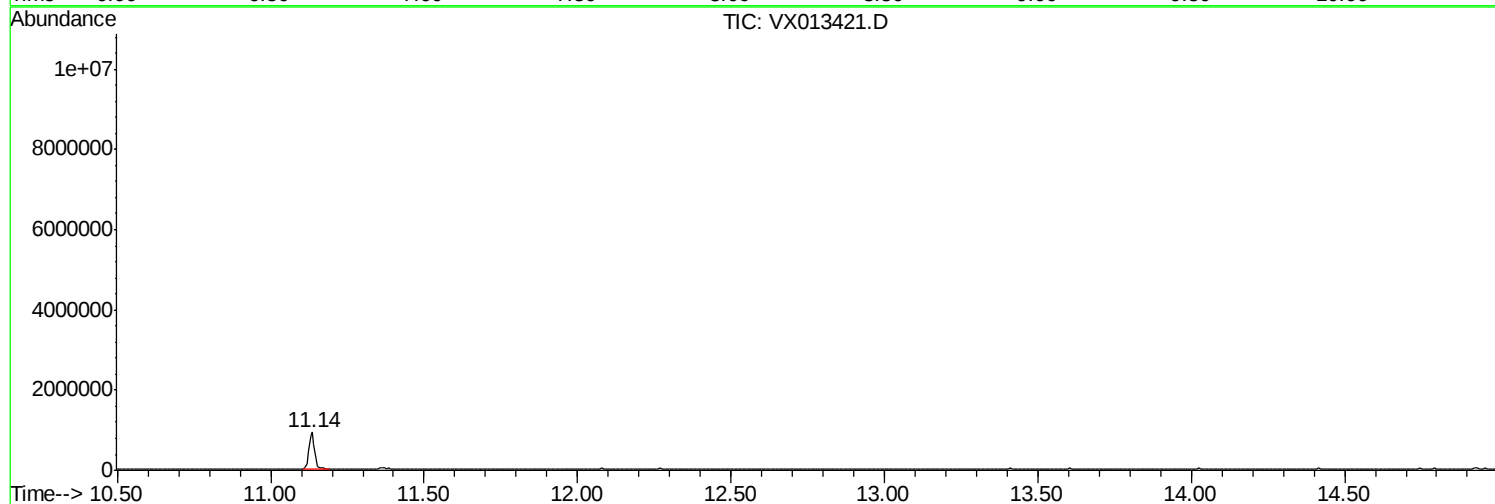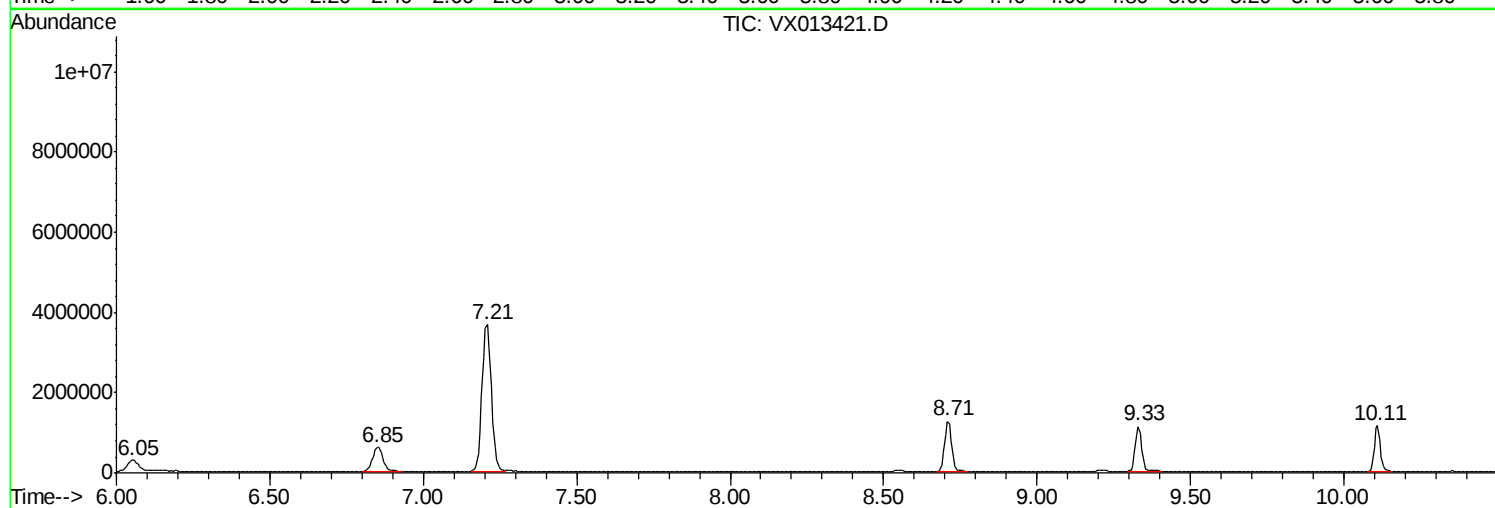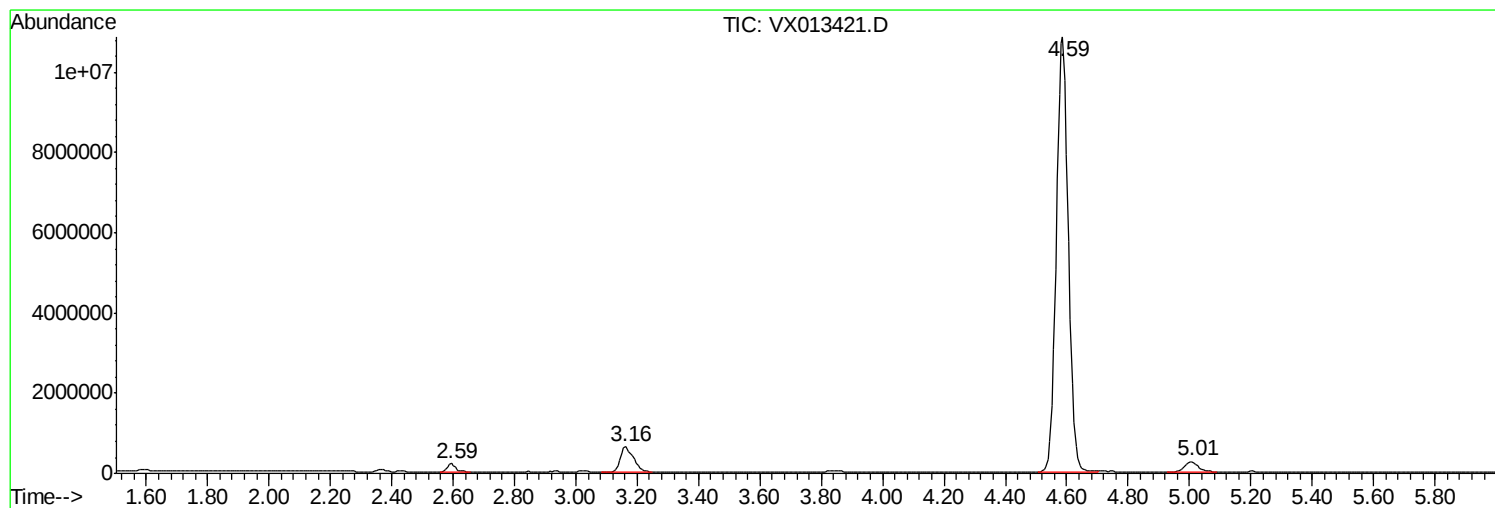

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA X\DATA\VX111419\
Data File : VX013421.D
Acq On : 14 Nov 2019 14:49
Operator : JC/SP
Sample : K5828-03
Misc : 5.0mL/MSVOA X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
REP111319










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA X\METHOD\624X111119W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.59	13.86 ug/l	347066	Bromochloromethane	5.01

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	86
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	78
4		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56
5		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	56

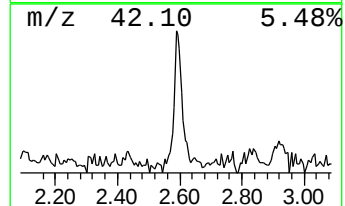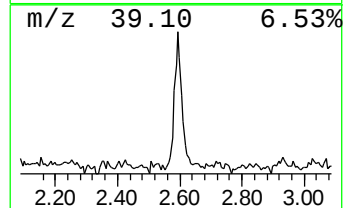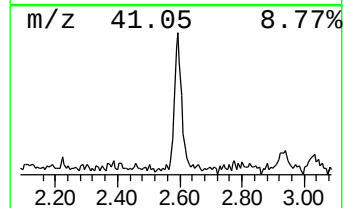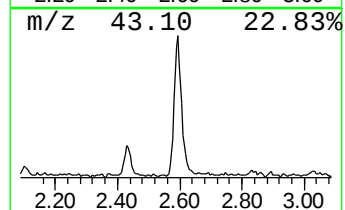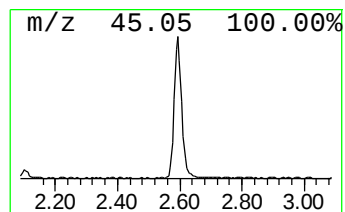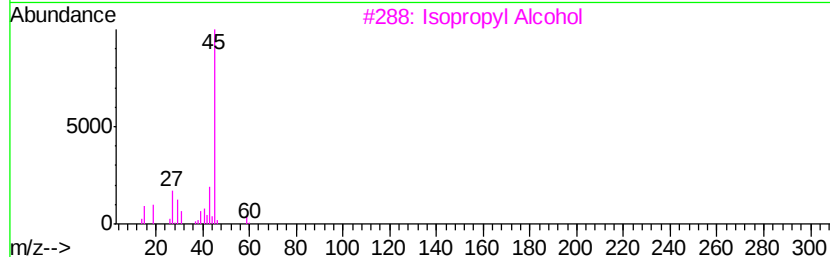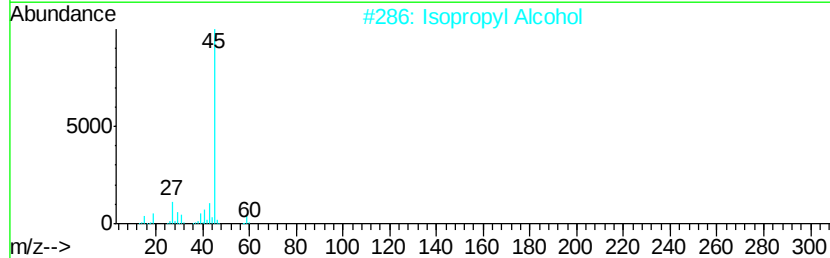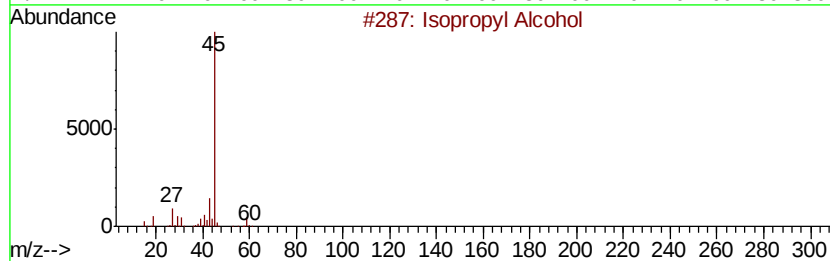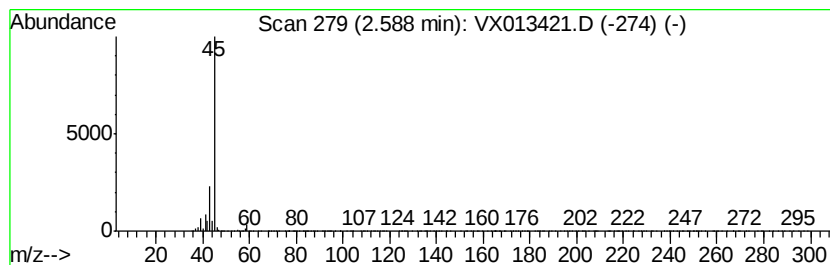

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111419\
Data File : VX013421.D
Acq On : 14 Nov 2019 14:49
Operator : JC/SP
Sample : K5828-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
REP111319

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\624X111119W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.59	13.9	ug/l	347066	1	5.01	751028	30.0