

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111422\
 Data File : VX032790.D
 Acq On : 14 Nov 2022 13:31
 Operator : JC/MD
 Sample : N5558-07 25X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 20BR-20221109

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	58	rVB	58492	65070	6.65%	1.624%
2	4.489	547	558	579	rBV	357990	978879	100.00%	24.431%
3	5.385	693	705	721	rBV2	64003	185755	18.98%	4.636%
4	5.550	721	732	747	rVB	101394	286597	29.28%	7.153%
5	5.958	788	799	813	rBV	66312	176766	18.06%	4.412%
6	6.763	921	931	944	rBV	156761	366818	37.47%	9.155%
7	7.129	982	991	1006	rBV	105439	232118	23.71%	5.793%
8	8.647	1234	1240	1254	rBV	329905	512542	52.36%	12.792%
9	10.055	1465	1471	1483	rBV	313047	429352	43.86%	10.716%
10	11.079	1634	1639	1651	rBV	309938	377713	38.59%	9.427%
11	12.024	1788	1794	1805	rBV	301832	395180	40.37%	9.863%




Sum of corrected areas: 4006790

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111422\
Data File : VX032790.D
Acq On : 14 Nov 2022 13:31
Operator : JC/MD
Sample : N5558-07 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

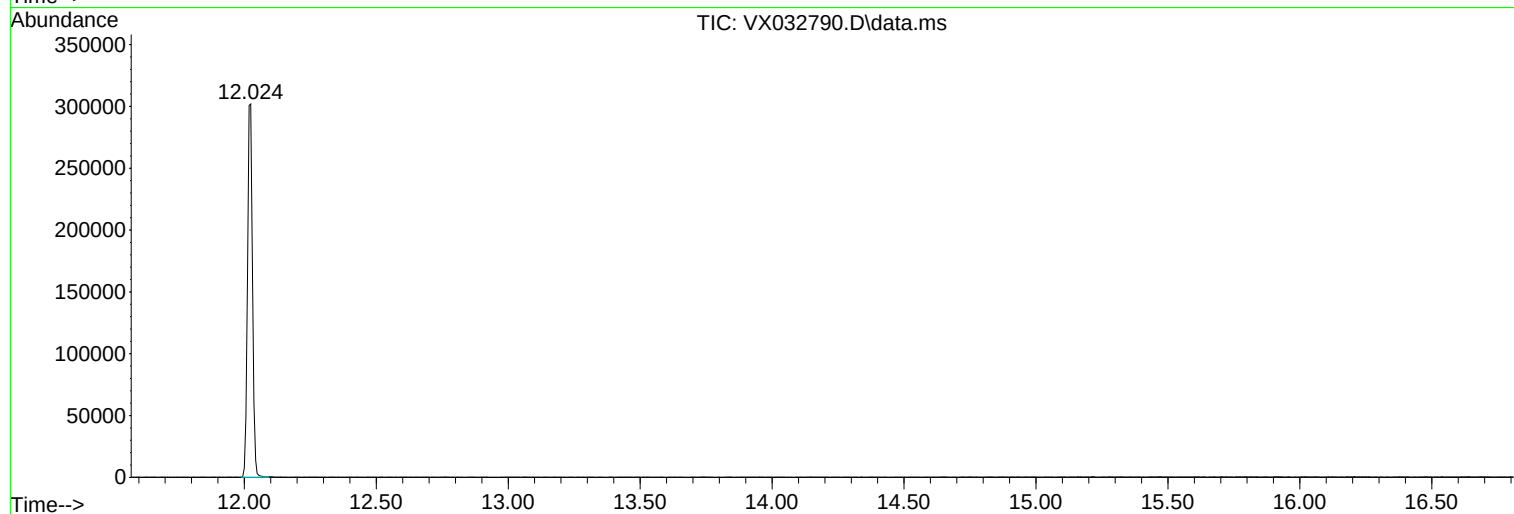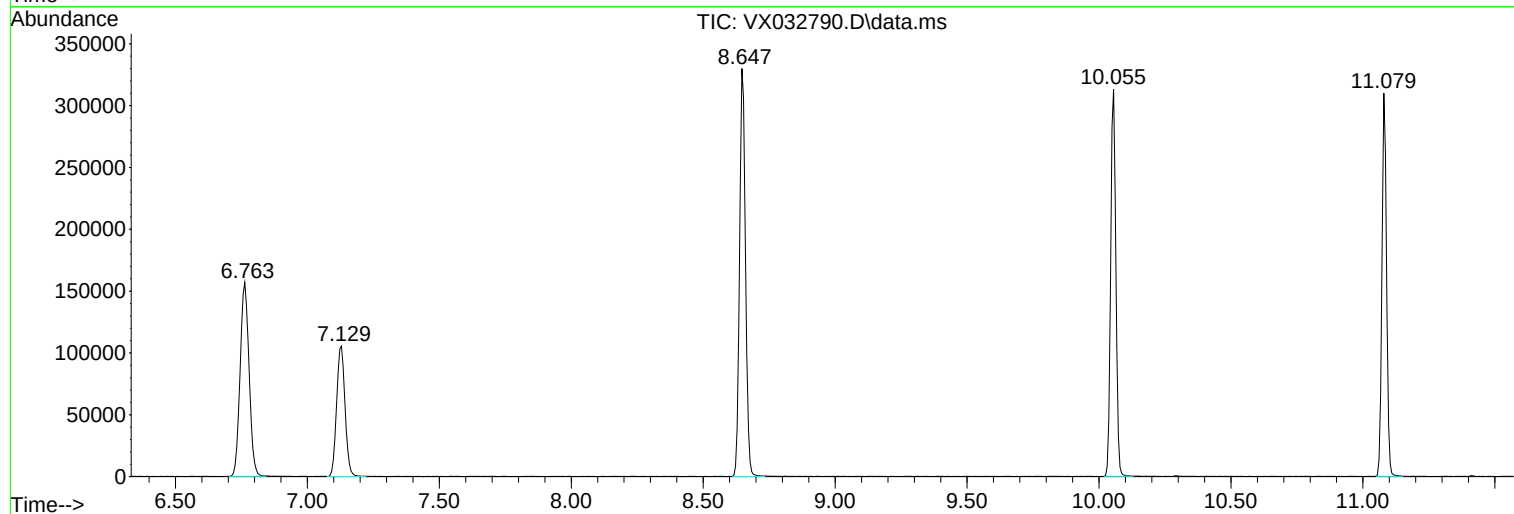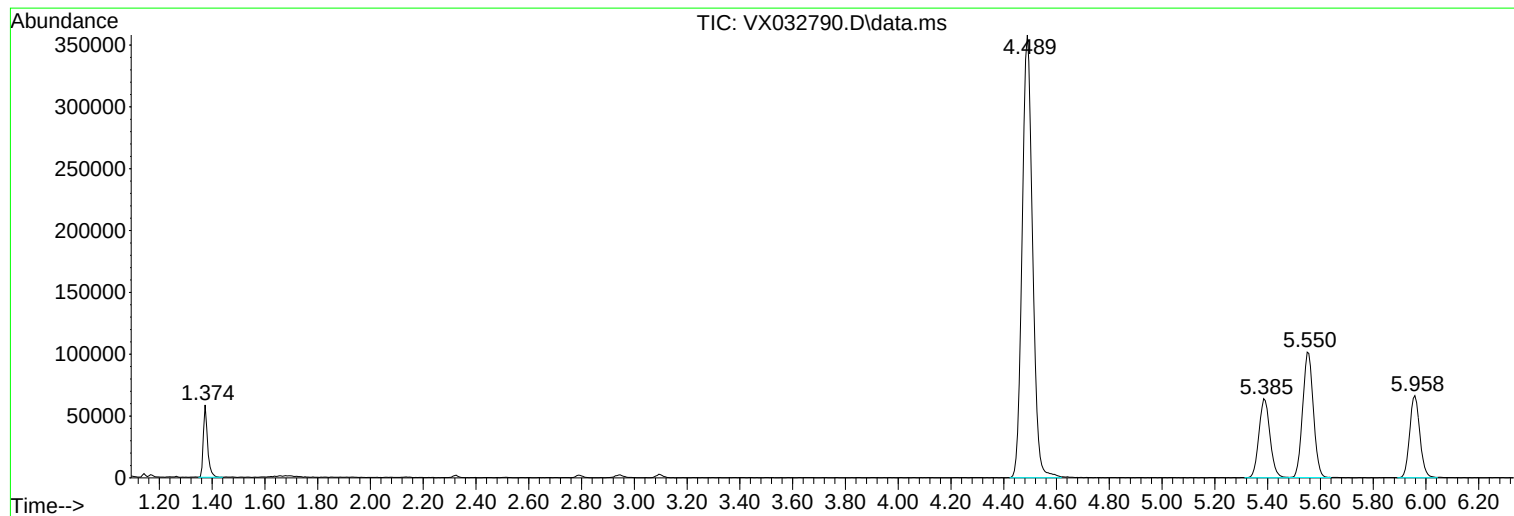

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111422\
Data File : VX032790.D
Acq On : 14 Nov 2022 13:31
Operator : JC/MD
Sample : N5558-07 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111422\
Data File : VX032790.D
Acq On : 14 Nov 2022 13:31
Operator : JC/MD
Sample : N5558-07 25X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------