
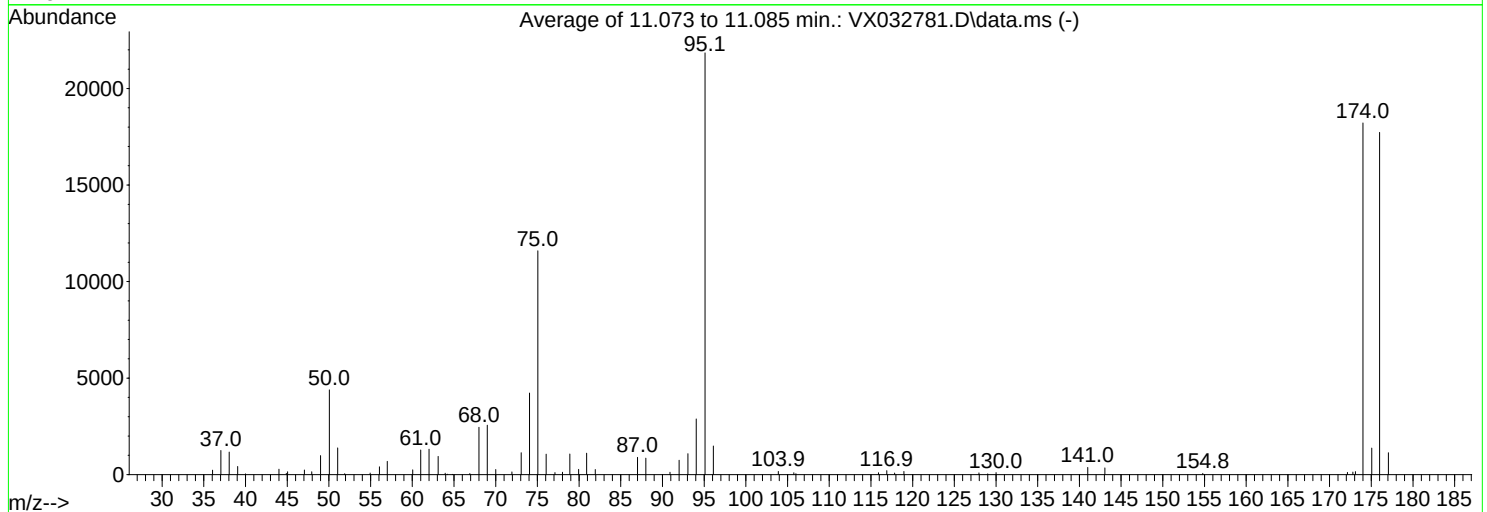


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111422\
 Data File : VX032781.D
 Acq On : 14 Nov 2022 09:11
 Operator : JC/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260
 Last Update : Thu Oct 27 08:28:06 2022

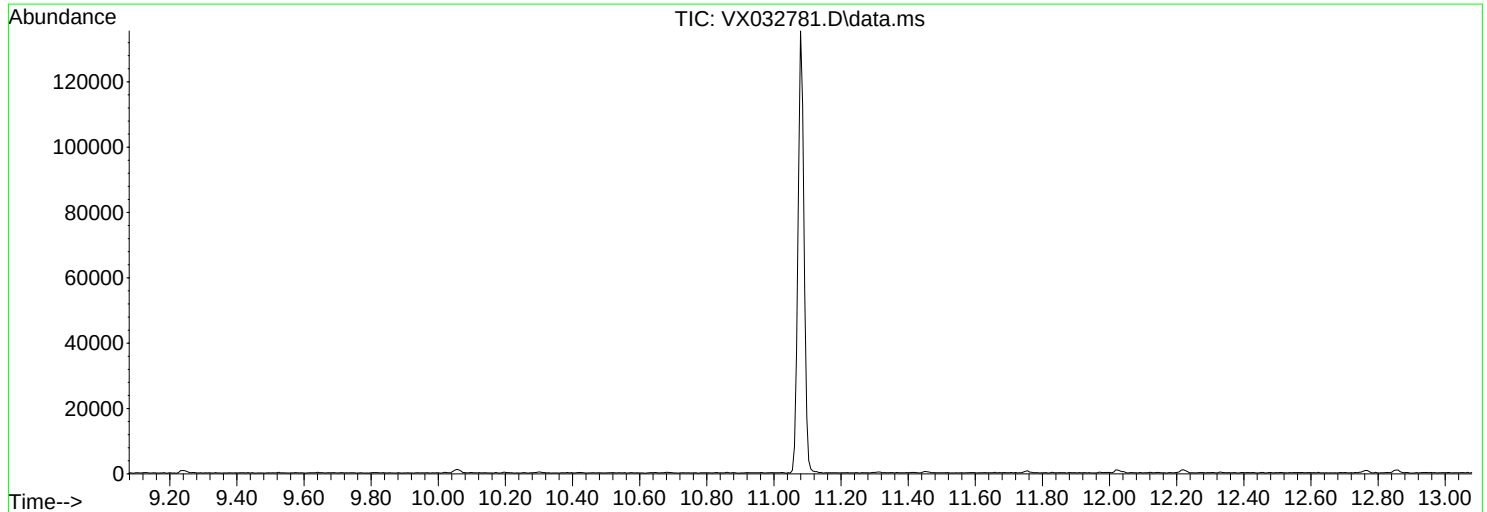

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.1	4391	PASS
75	95	30	60	53.1	11593	PASS
95	95	100	100	100.0	21848	PASS
96	95	5	9	6.8	1485	PASS
173	174	0.00	2	0.9	159	PASS
174	95	50	100	83.4	18217	PASS
175	174	5	9	7.5	1373	PASS
176	174	95	101	97.3	17730	PASS
177	176	5	9	6.4	1135	PASS