
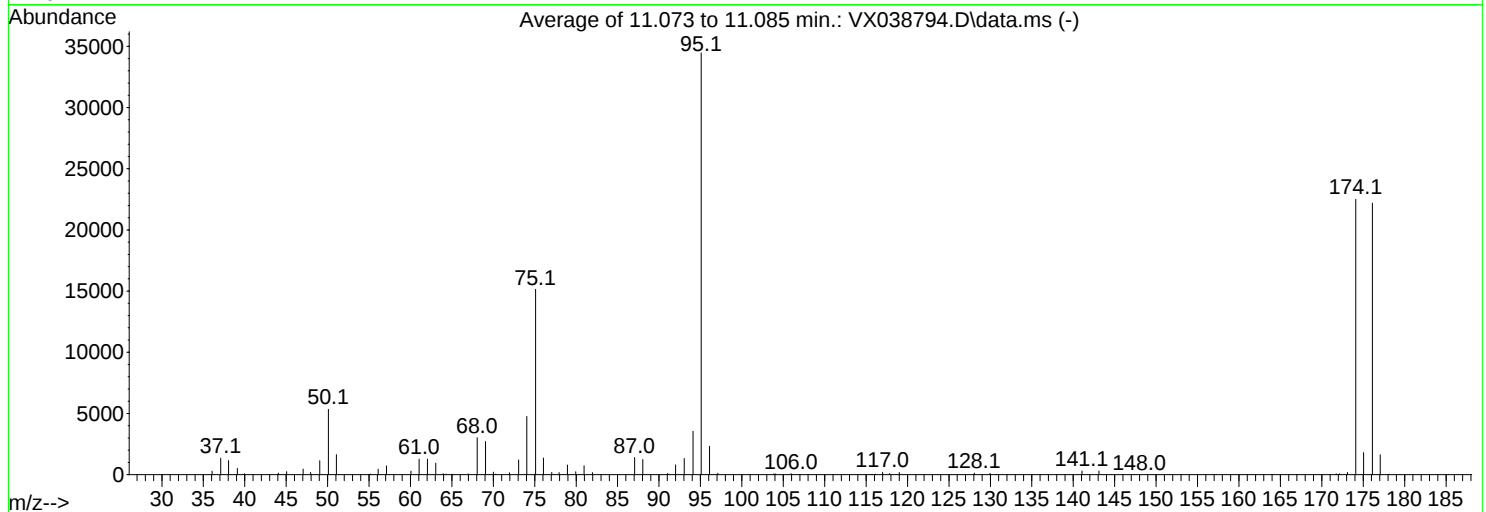


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111423\
Data File : VX038794.D
Acq On : 14 Nov 2023 08:18
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111423W.M
Title : SW846 8260
Last Update : Tue Nov 14 09:15:55 2023

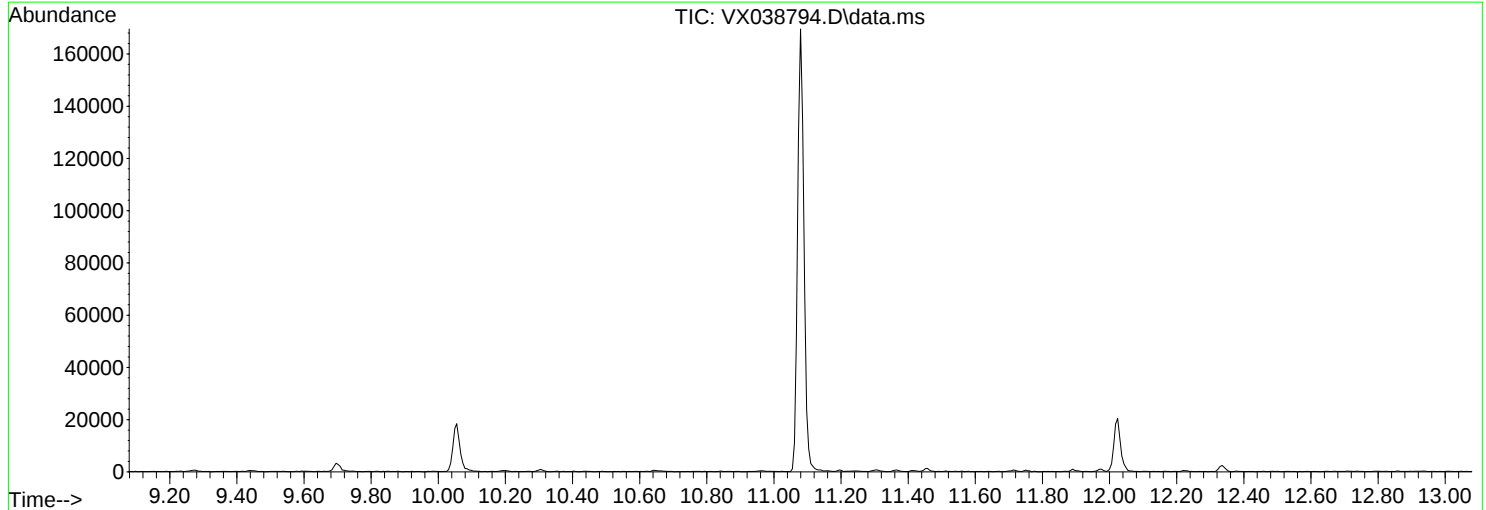

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.5	5337	PASS
75	95	30	60	43.9	15139	PASS
95	95	100	100	100.0	34472	PASS
96	95	5	9	6.7	2311	PASS
173	174	0.00	2	0.8	181	PASS
174	95	50	100	65.3	22507	PASS
175	174	5	9	8.0	1808	PASS
176	174	95	101	98.6	22192	PASS
177	176	5	9	7.3	1617	PASS