
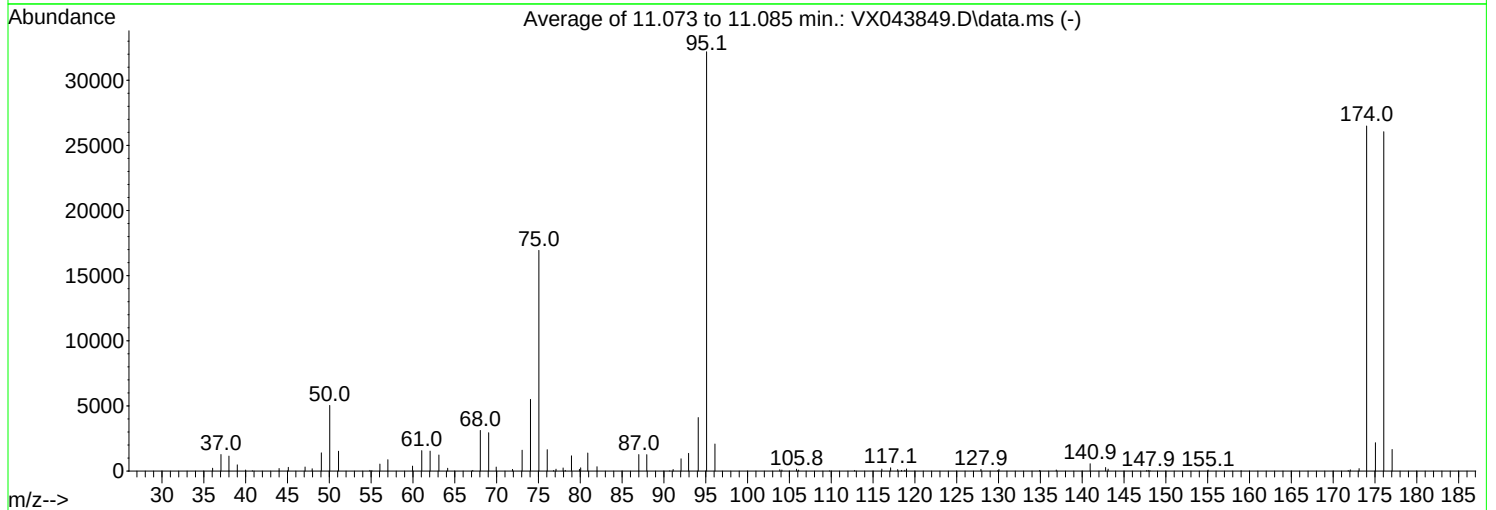


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111424\
Data File : VX043849.D
Acq On : 14 Nov 2024 12:32
Operator : JC/MD
Sample : BFB699
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB699

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Title : VOC Analysis
Last Update : Fri Nov 15 03:21:47 2024

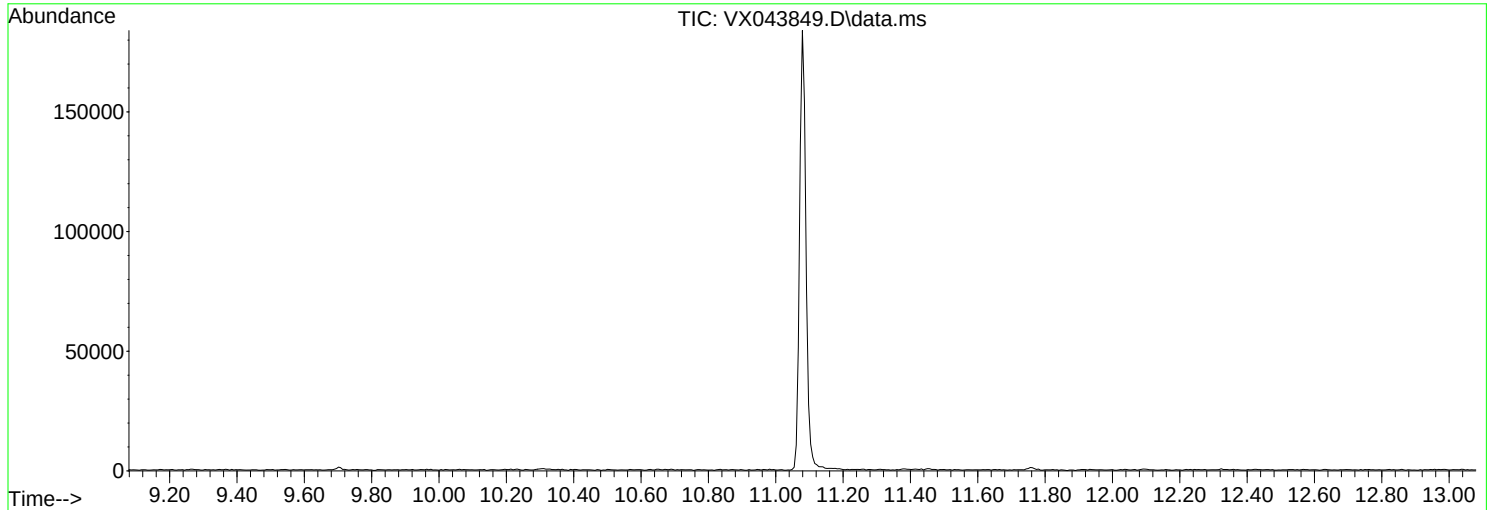

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	5040	PASS
75	95	30	80	52.6	16941	PASS
95	95	100	100	100.0	32189	PASS
96	95	5	9	6.5	2081	PASS
173	174	0.00	2	0.7	193	PASS
174	95	50	120	82.3	26488	PASS
175	174	5	9	8.2	2178	PASS
176	174	95	101	98.3	26048	PASS
177	176	5	9	6.4	1659	PASS

m/z	Abundance
38.90	52.0
40.00	168.0
44.00	119.0

Instrument :
MSVOA_X
ClientSampleId :
BFB699

m/z	Abundance
36.10	195.0
37.00	1261.0
38.00	1151.0
39.00	447.0
40.10	221.0
44.00	226.0
45.10	212.0
47.10	271.0
48.00	217.0
49.10	1506.0
50.10	4553.0
51.10	1452.0
56.00	498.0
57.00	765.0
60.00	287.0
61.10	1313.0
62.10	1524.0
63.10	1183.0
64.10	281.0
67.10	71.0
68.10	3246.0
69.00	3063.0
70.00	215.0
73.10	1348.0
74.10	4928.0
75.00	16696.0
76.00	1512.0
77.10	228.0
78.10	296.0
78.90	996.0
79.90	395.0
81.00	1315.0
82.00	280.0
87.00	1159.0
87.90	1112.0
90.70	62.0
91.20	77.0
92.10	963.0
93.00	1177.0
94.10	3886.0
95.10	29816.0
96.20	1681.0
103.80	144.0
105.80	214.0
112.80	63.0
115.90	77.0
117.00	196.0
118.00	51.0
118.80	196.0
127.90	140.0
129.90	92.0
134.90	53.0
136.90	65.0
140.90	442.0
142.80	378.0
147.70	130.0
154.90	53.0
174.00	20280.0
175.00	1533.0
176.10	18720.0
177.00	1130.0

Instrument :
MSVOA_X
ClientSampleId :
BFB699

m/z	Abundance
36.10	252.0
37.10	1360.0
38.00	1425.0
39.10	675.0
40.00	231.0
40.80	78.0
44.00	333.0
45.10	388.0
47.10	435.0
48.00	166.0
49.00	1380.0
50.00	6025.0
51.10	1986.0
54.80	102.0
56.10	594.0
57.00	1002.0
60.00	434.0
61.00	2058.0
62.00	1744.0
63.10	1385.0
64.20	249.0
67.20	85.0
68.00	3673.0
69.10	3171.0
69.90	413.0
71.90	201.0
73.10	2086.0
74.00	6266.0
75.10	19536.0
76.10	1958.0
77.10	164.0
77.90	235.0
79.00	1459.0
80.10	379.0
80.80	1620.0
82.00	416.0
87.00	1742.0
88.00	1559.0
91.10	158.0
92.00	902.0
92.90	1629.0
94.10	4702.0
95.10	37256.0
96.10	2894.0
104.10	243.0
105.90	239.0
112.80	92.0
116.00	245.0
117.10	246.0
117.90	146.0
119.00	323.0
127.90	148.0
130.10	216.0
134.90	81.0
136.90	72.0
141.00	750.0
142.80	447.0
147.90	164.0
155.00	53.0
171.80	126.0
172.20	98.0
173.10	350.0
174.00	30288.0
175.10	2583.0
176.00	30304.0
177.00	1943.0

Instrument :
MSVOA_X
ClientSampleId :
BFB699

m/z	Abundance
36.00	212.0
37.10	1196.0
38.00	868.0
39.00	468.0
40.00	293.0
44.00	397.0
45.10	262.0
47.10	229.0
47.80	167.0
49.10	1321.0
50.10	4543.0
51.10	1134.0
54.90	64.0
55.10	64.0
56.00	524.0
57.00	853.0
59.90	429.0
61.00	1332.0
62.10	1336.0
63.10	1142.0
64.10	122.0
68.10	2442.0
69.10	2601.0
69.90	299.0
71.90	193.0
73.00	1377.0
74.10	5328.0
75.10	14592.0
76.00	1457.0
76.80	113.0
77.20	53.0
77.80	187.0
78.20	156.0
79.00	1061.0
80.00	372.0
80.90	1222.0
82.00	316.0
87.00	896.0
88.00	1119.0
91.00	135.0
92.10	966.0
93.00	1267.0
94.10	3742.0
95.10	29496.0
96.00	1667.0
103.90	174.0
106.10	233.0
109.80	62.0
116.10	142.0
117.20	311.0
118.00	145.0
118.40	153.0
119.00	176.0
127.90	130.0
130.00	168.0
136.90	122.0
141.00	504.0
143.10	452.0
148.10	86.0
155.10	125.0
159.00	53.0
172.00	193.0
173.10	229.0
174.00	28896.0
175.00	2418.0
176.10	29120.0
177.10	1904.0

Instrument :
MSVOA_X
ClientSampleId :
BFB699