


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_X\DATA\VX111518\
Data File : VX006016.D
Acq On : 15 Nov 2018 11:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\82X110718W.M
Title : SW846 8260
Last Update : Wed Nov 07 14:40:53 2018

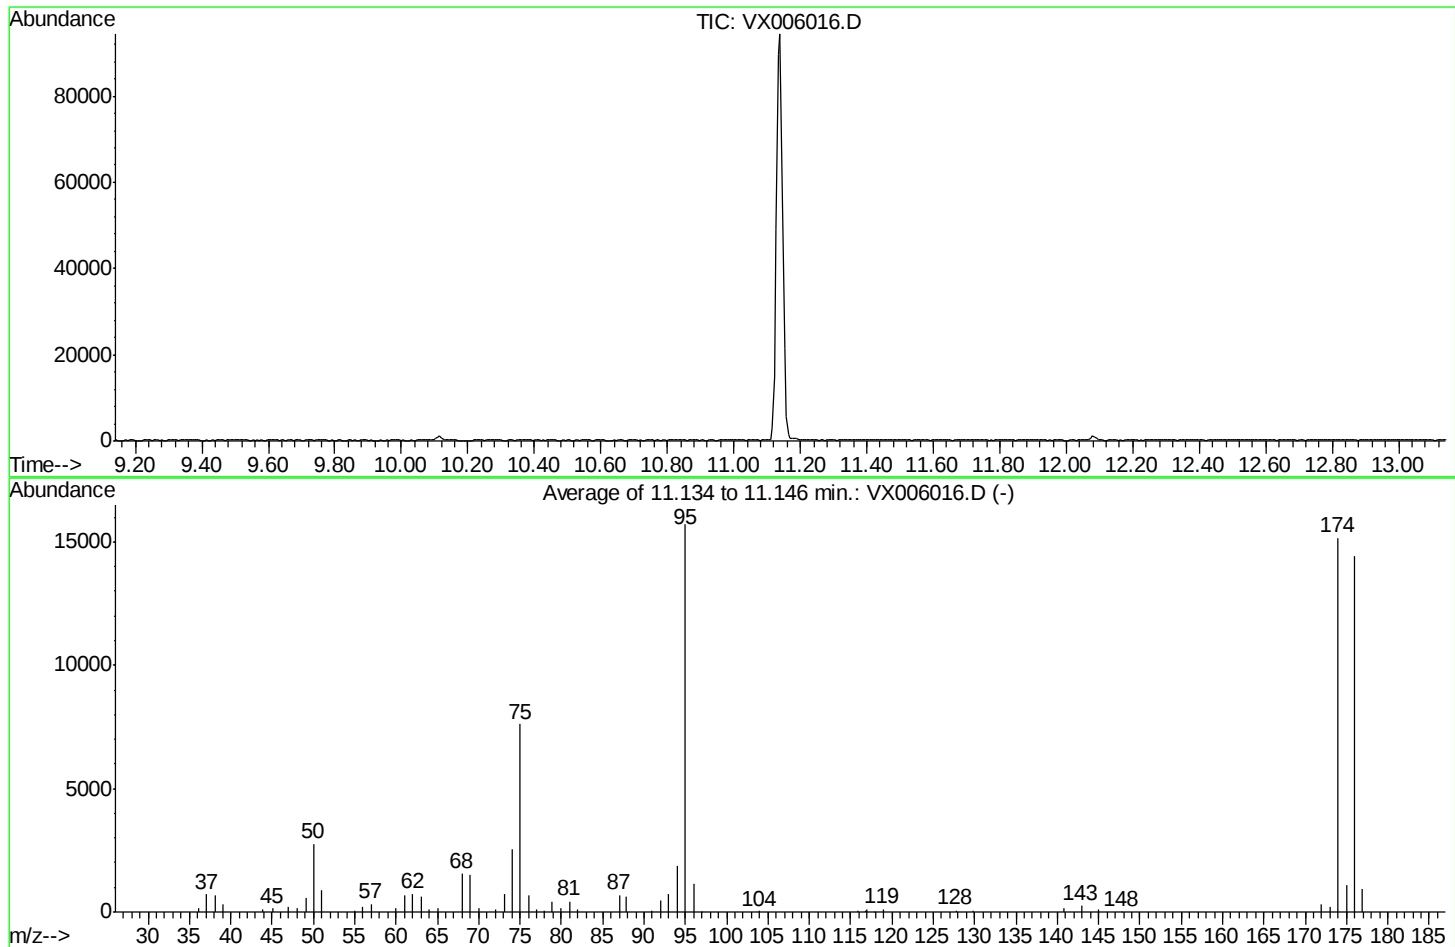

AutoFind: Scans 1637, 1638, 1639; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	2766	PASS
75	95	30	60	48.4	7602	PASS
95	95	100	100	100.0	15710	PASS
96	95	5	9	7.2	1124	PASS
173	174	0.00	2	1.4	219	PASS
174	95	50	100	96.5	15153	PASS
175	174	5	9	7.4	1116	PASS
176	174	95	101	95.2	14430	PASS
177	176	5	9	6.6	946	PASS