


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX111519\  
 Data File : VX013433.D  
 Acq On : 15 Nov 2019 08:56  
 Operator : JC/SP  
 Sample : BFB  
 Misc : 5.0mL/MSVOA X/WATER  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_X  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_X\METHOD\82X103119W.M  
 Title : SW846 8260  
 Last Update : Sat Nov 02 07:06:38 2019

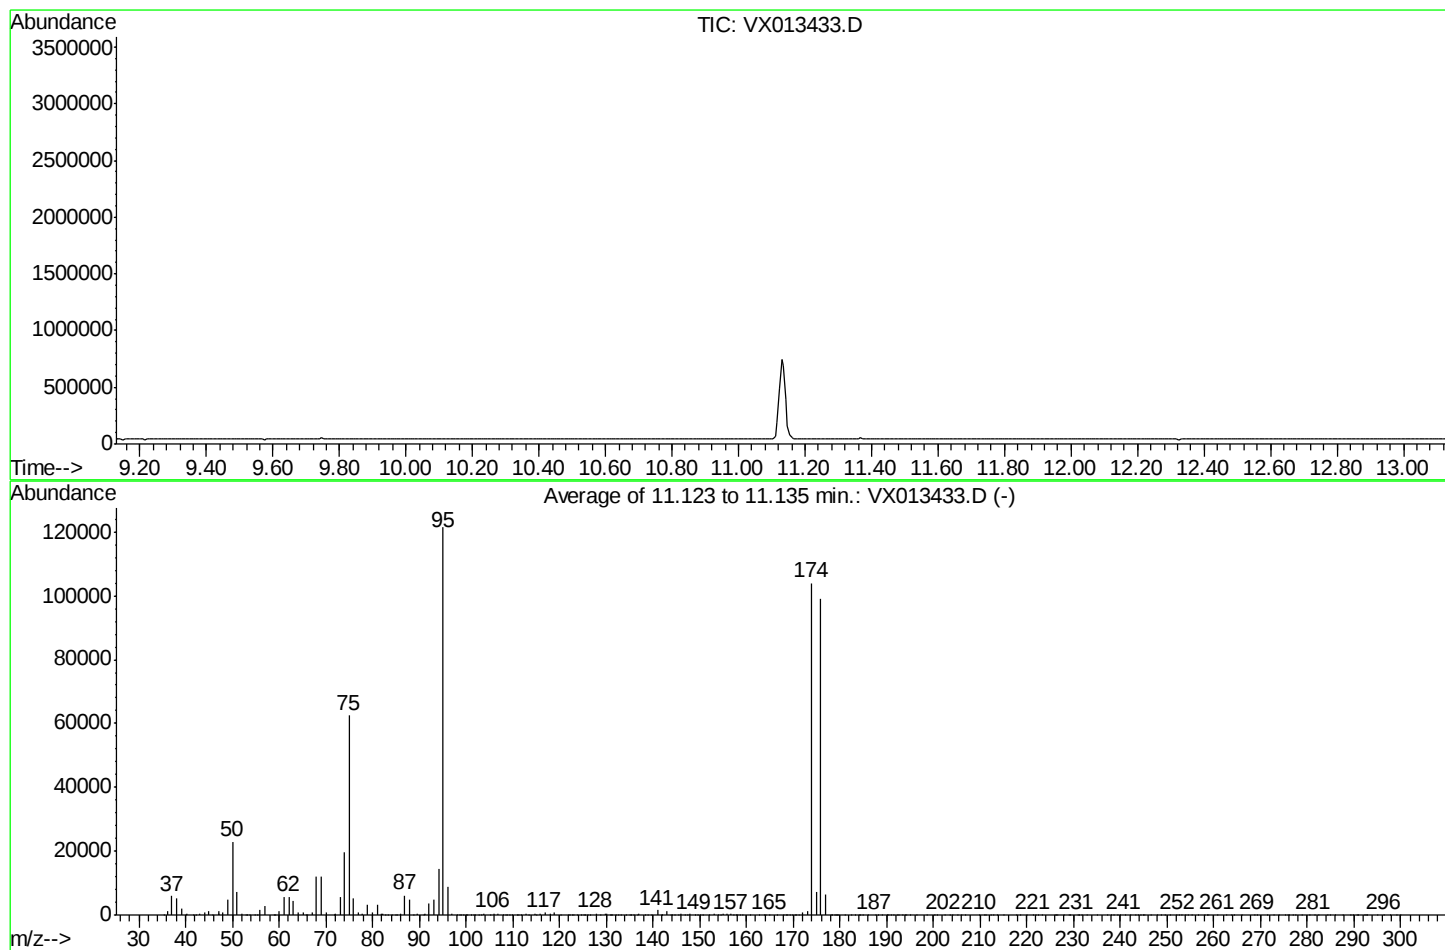

AutoFind: Scans 1679, 1680, 1681; Background Corrected with Scan 1672

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 19.0      | 23056   | PASS             |
| 75          | 95           | 30           | 60           | 51.4      | 62437   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 121445  | PASS             |
| 96          | 95           | 5            | 9            | 7.2       | 8732    | PASS             |
| 173         | 174          | 0.00         | 2            | 1.1       | 1137    | PASS             |
| 174         | 95           | 50           | 100          | 85.7      | 104069  | PASS             |
| 175         | 174          | 5            | 9            | 7.1       | 7429    | PASS             |
| 176         | 174          | 95           | 101          | 95.3      | 99174   | PASS             |
| 177         | 176          | 5            | 9            | 6.4       | 6339    | PASS             |