

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111522\
 Data File : VX032852.D
 Acq On : 16 Nov 2022 07:43
 Operator : JC/MD
 Sample : N5640-06
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-120

Quant Time: Nov 16 08:37:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.556	168	99772	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	164297	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	148191	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	67692	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	71021	51.230	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	= 102.460%	
35) Dibromofluoromethane	5.385	113	56932	48.579	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 97.160%	
50) Toluene-d8	8.647	98	206860	50.762	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	= 101.520%	
62) 4-Bromofluorobenzene	11.079	95	76790	48.240	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 96.480%	


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111522\
Data File : VX032852.D
Acq On : 16 Nov 2022 07:43
Operator : JC/MD
Sample : N5640-06
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-120


Quant Time: Nov 16 08:37:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration

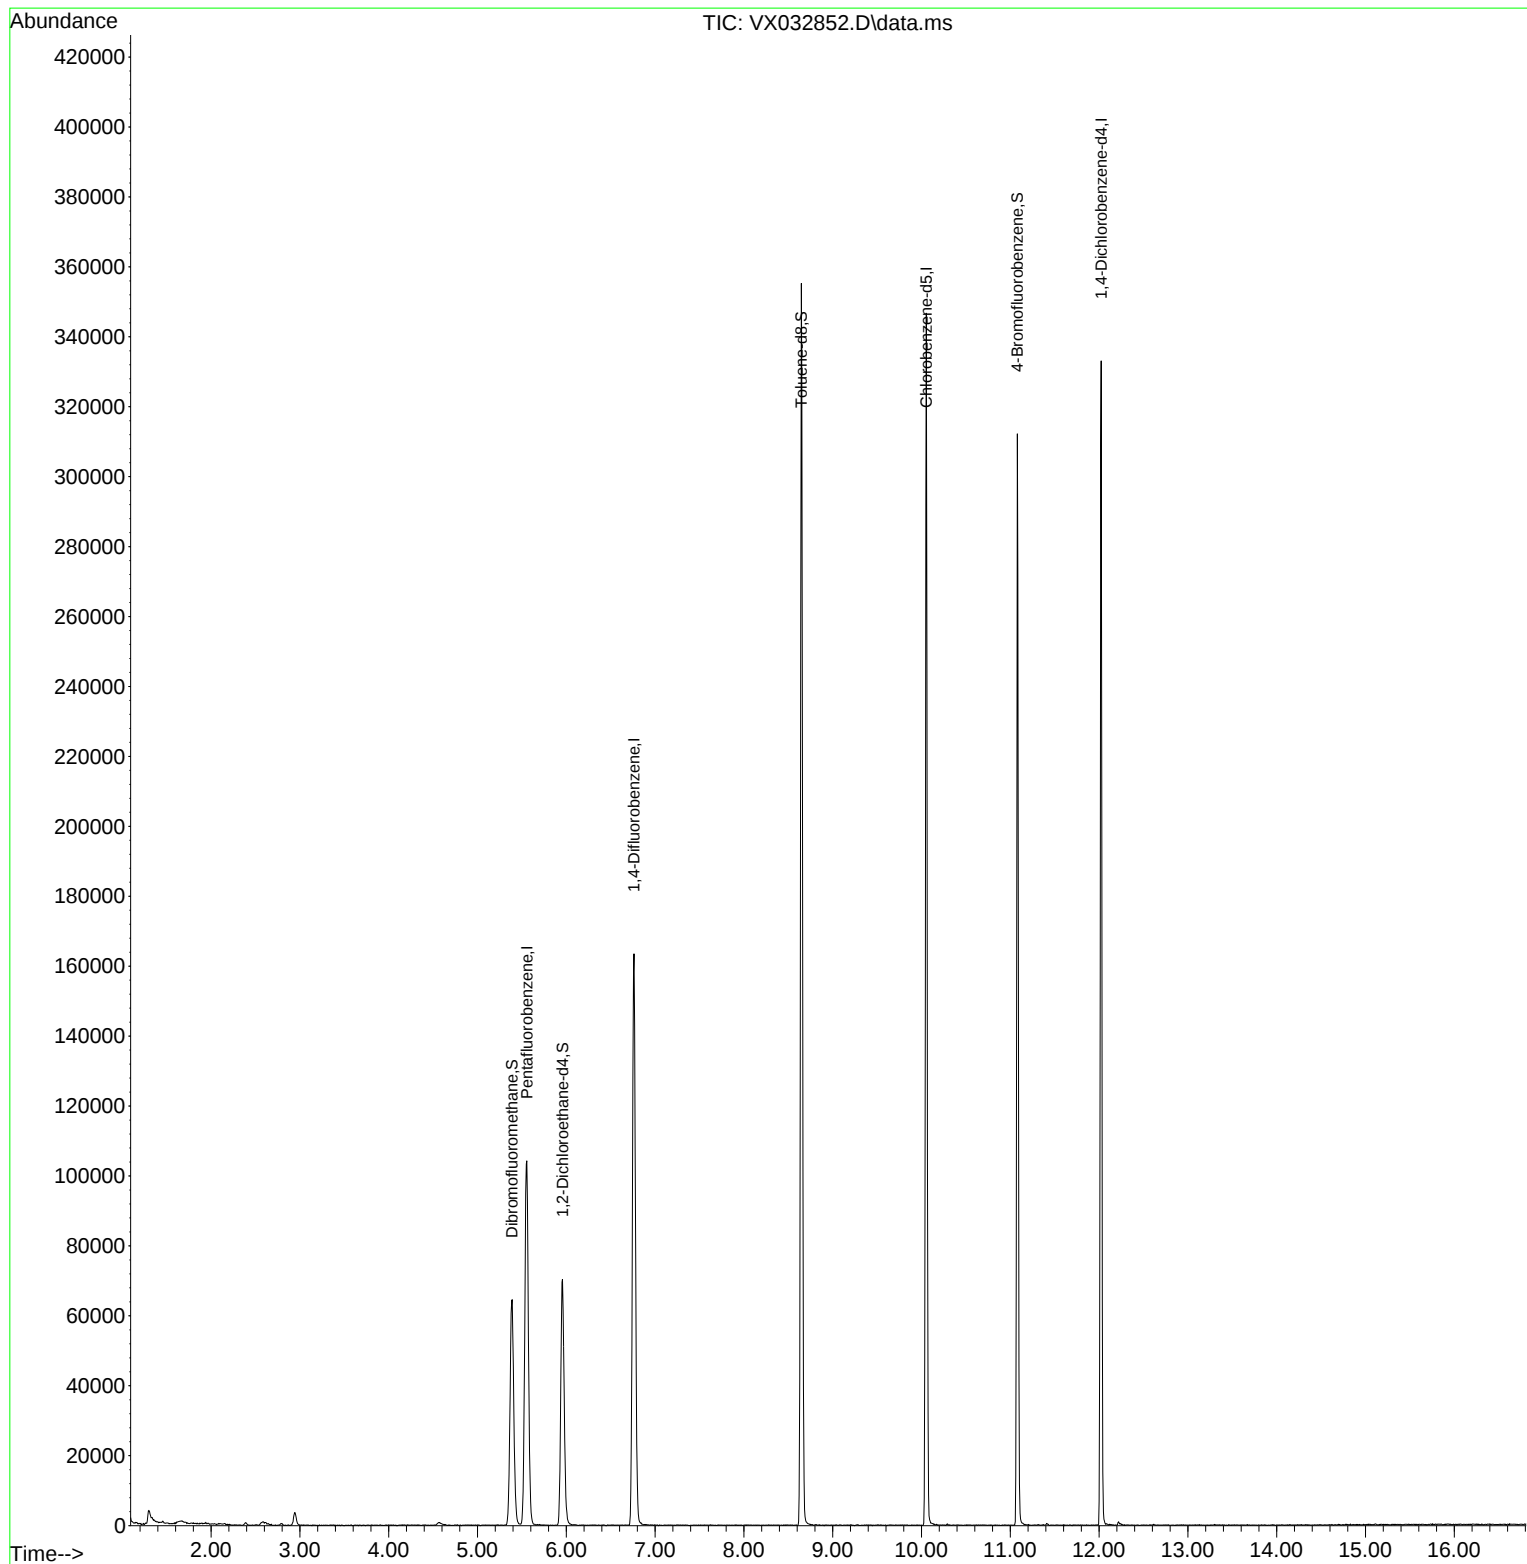



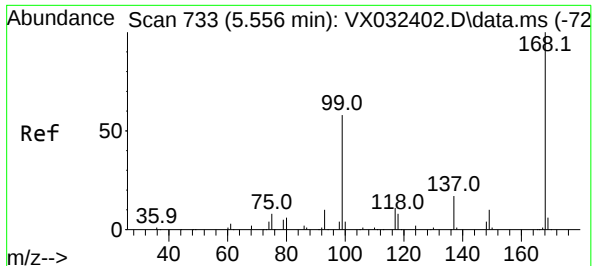


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43

Instrument :
MSVOA_X
ClientSampleId :
MW-120



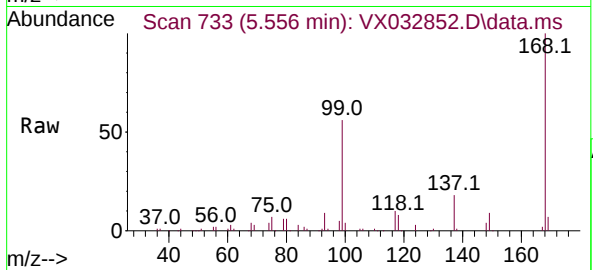



Tgt Ion:168 Resp: 99772
Ion Ratio Lower Upper
168 100
99 56.0 46.1 69.1

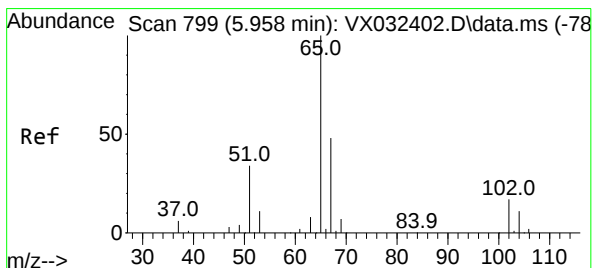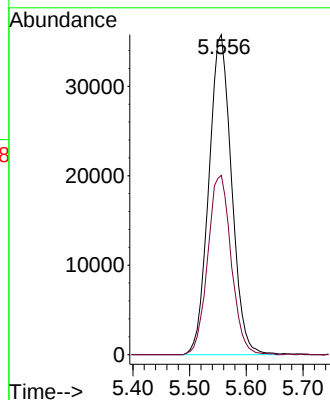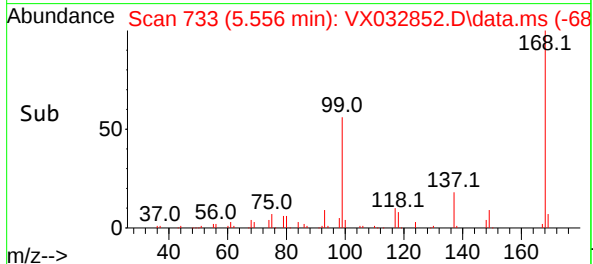

#33
1,2-Dichloroethane-d4
Concen: 51.230 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43

Tgt Ion: 65 Resp: 71021
Ion Ratio Lower Upper
65 100
67 50.5 0.0 101.8


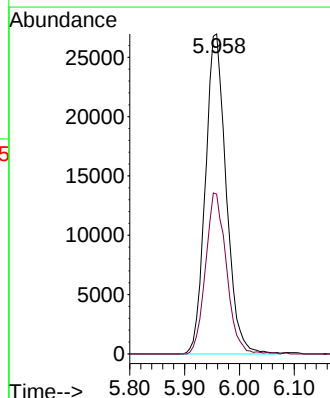
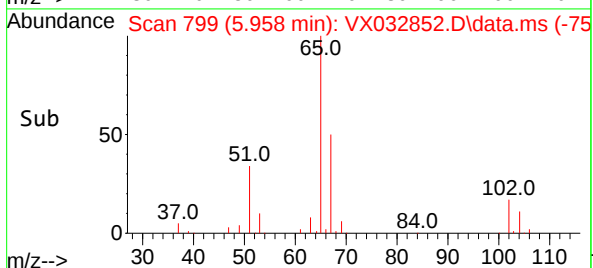
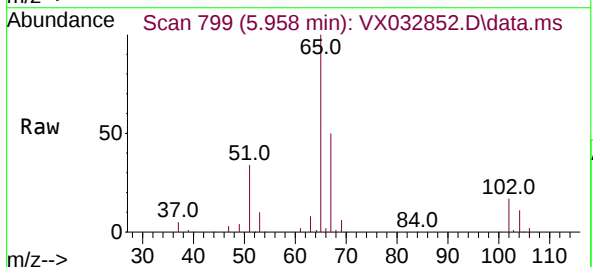


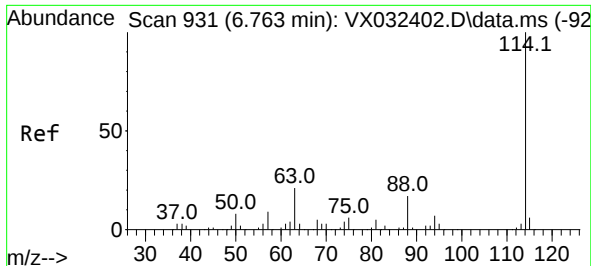

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 931
Delta R.T. 0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43




Instrument :
MSVOA_X
ClientSampleId :
MW-120


Tgt Ion:114 Resp: 164297
Ion Ratio Lower Upper
114 100
63 19.4 0.0 41.6
88 15.2 0.0 33.4

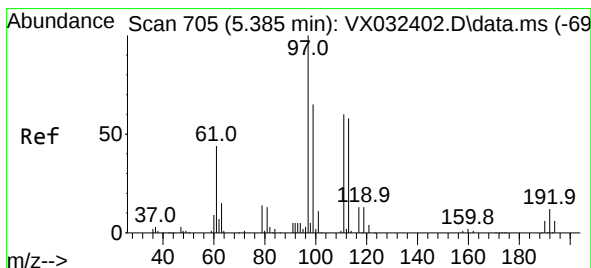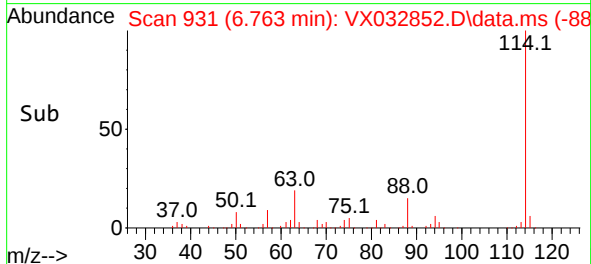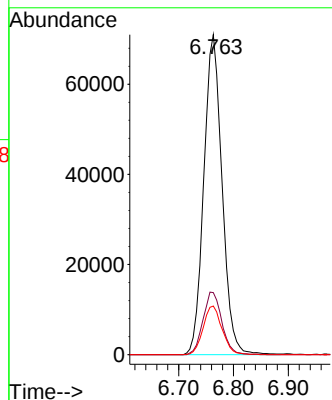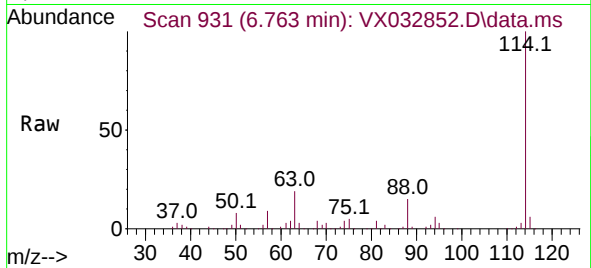

#35
Dibromofluoromethane
Concen: 48.579 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43

Tgt Ion:113 Resp: 56932
Ion Ratio Lower Upper
113 100
111 102.7 82.4 123.6
192 18.9 15.4 23.2


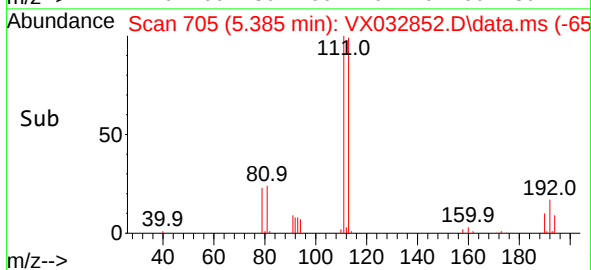
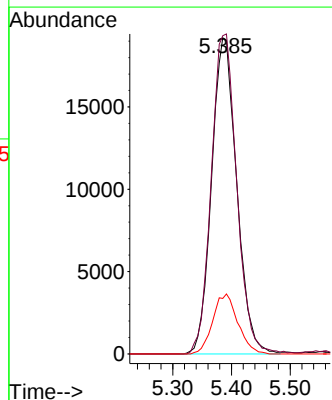
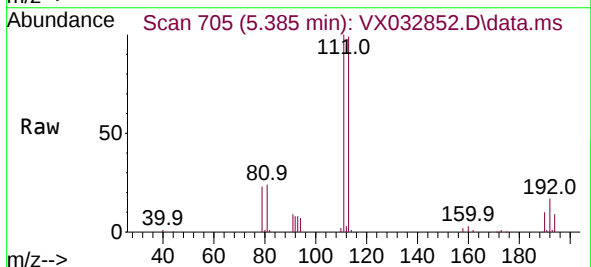


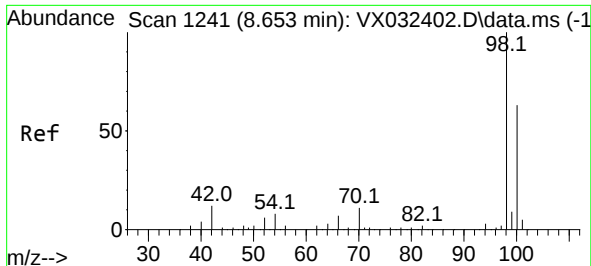

#50
Toluene-d8
Concen: 50.762 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43




Instrument :
MSVOA_X
ClientSampleId :
MW-120


Tgt Ion: 98 Resp: 206860
Ion Ratio Lower Upper
98 100
100 63.9 50.9 76.3

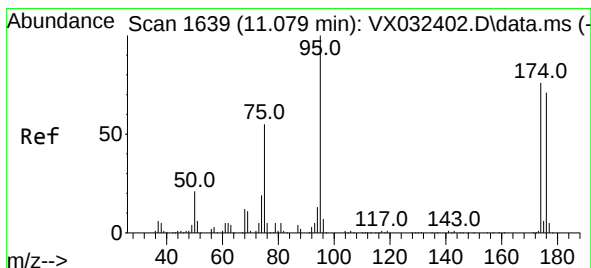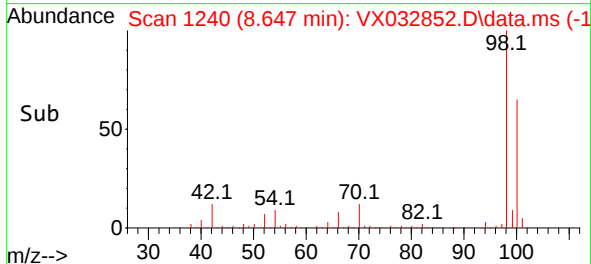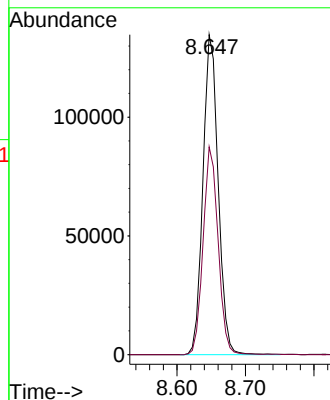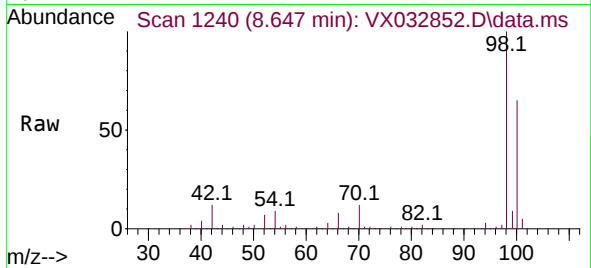

#62
4-Bromofluorobenzene
Concen: 48.240 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43

Tgt Ion: 95 Resp: 76790
Ion Ratio Lower Upper
95 100
174 84.3 0.0 164.0
176 81.6 0.0 154.4


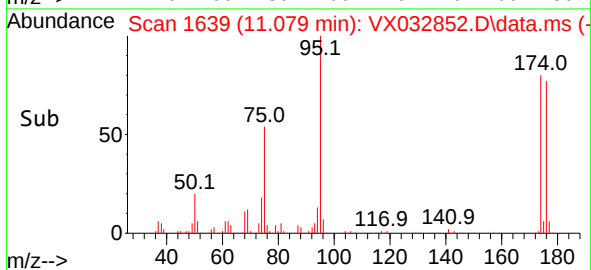
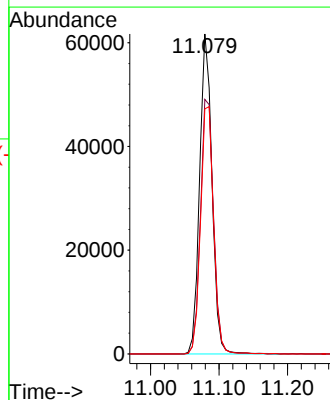
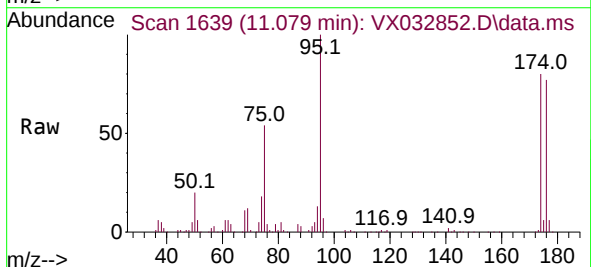


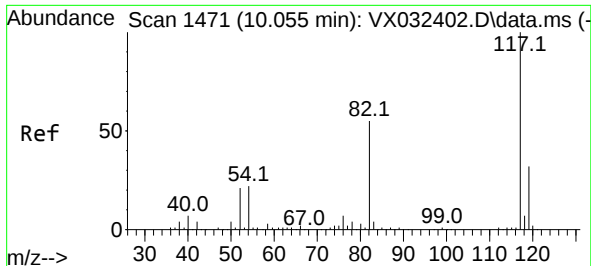

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43

Instrument :
MSVOA_X
ClientSampleId :
MW-120

Tgt Ion:117 Resp: 148191
Ion Ratio Lower Upper
117 100
82 55.1 44.3 66.5
119 31.7 25.7 38.5

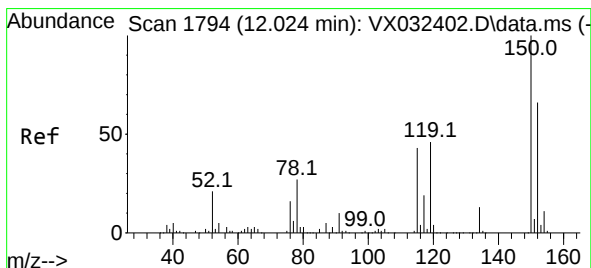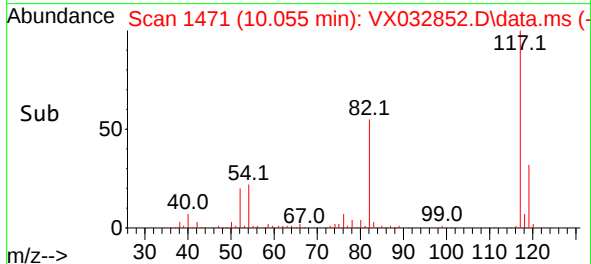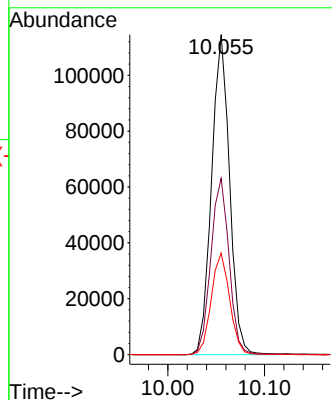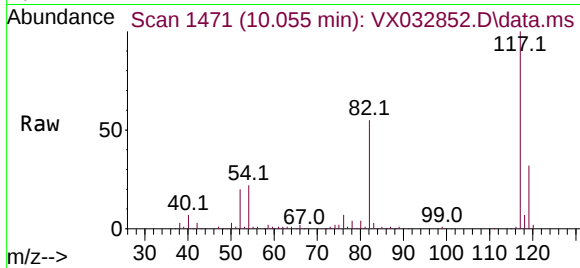

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.000 min
Lab File: VX032852.D
Acq: 16 Nov 2022 07:43

Tgt Ion:152 Resp: 67692
Ion Ratio Lower Upper
152 100
115 58.9 44.0 132.0
150 156.5 0.0 351.8

