

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111522\
Data File : VX032815.D
Acq On : 15 Nov 2022 12:21
Operator : JC/MD
Sample : N5558-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032815.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.374	43	47	56	rVB	31206	34113	6.20%	0.952%
2	4.489	546	558	580	rBV	181144	502541	91.27%	14.025%
3	5.385	694	705	721	rBV2	66257	195012	35.42%	5.442%
4	5.550	721	732	747	rVB2	108361	306479	55.66%	8.553%
5	5.958	789	799	814	rBV	70452	185627	33.71%	5.180%
6	6.763	921	931	945	rBV	167279	392741	71.33%	10.961%
7	7.129	983	991	1005	rVB	52338	115230	20.93%	3.216%
8	8.647	1234	1240	1250	rBV	351693	550584	100.00%	15.366%
9	10.055	1465	1471	1483	rBV	341288	460935	83.72%	12.864%
10	11.079	1634	1639	1651	rBV	314945	405226	73.60%	11.309%
11	12.024	1788	1794	1804	rBV	340193	434745	78.96%	12.133%




Sum of corrected areas: 3583233

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111522\
Data File : VX032815.D
Acq On : 15 Nov 2022 12:21
Operator : JC/MD
Sample : N5558-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

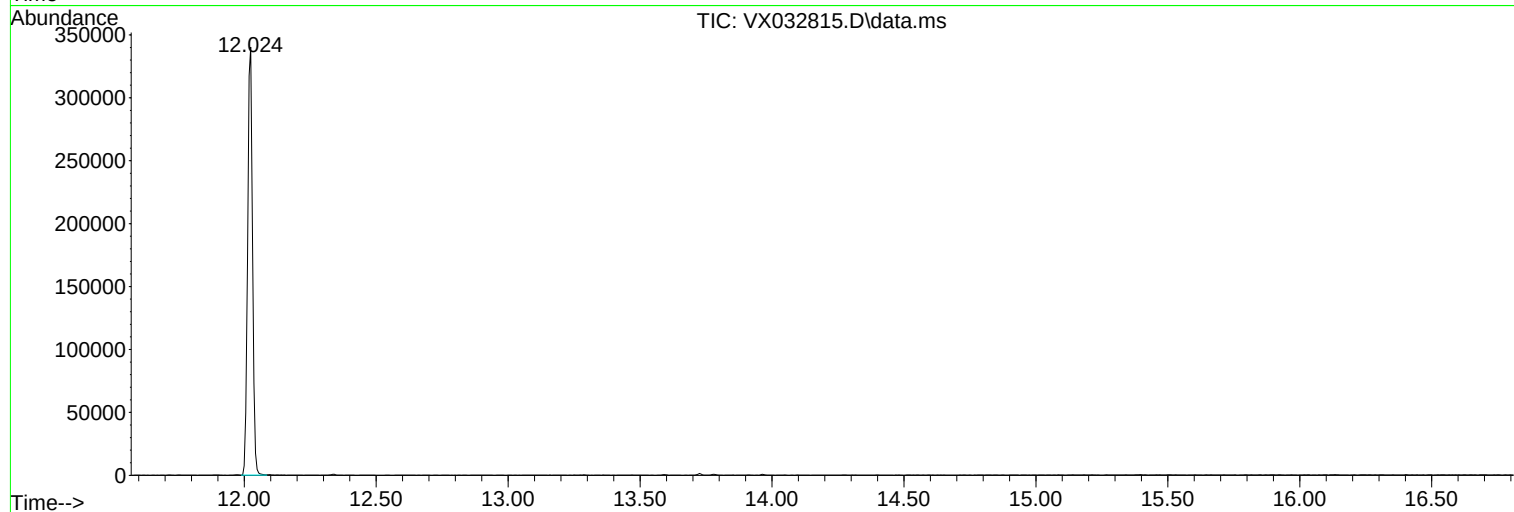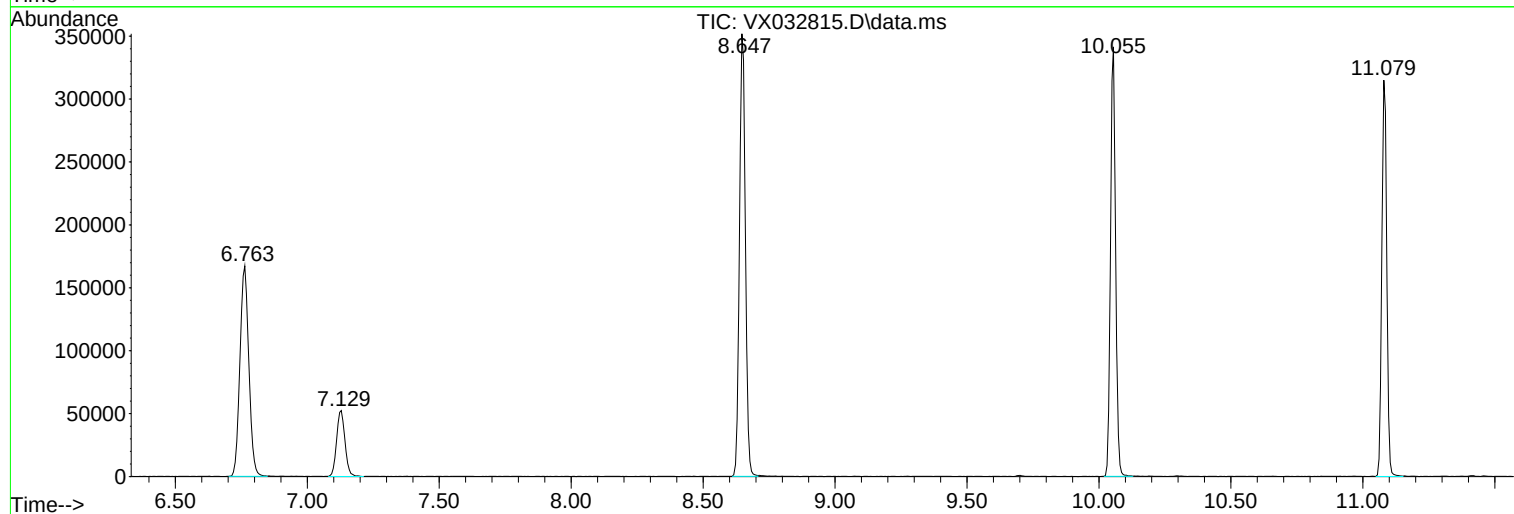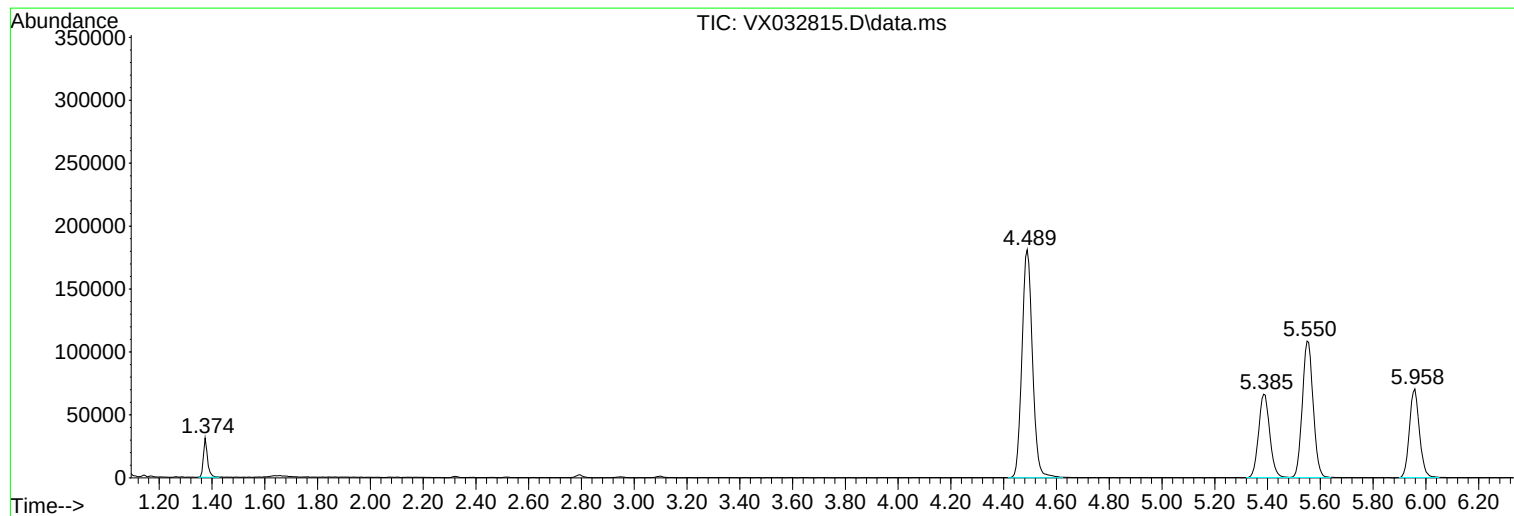

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111522\
Data File : VX032815.D
Acq On : 15 Nov 2022 12:21
Operator : JC/MD
Sample : N5558-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111522\
Data File : VX032815.D
Acq On : 15 Nov 2022 12:21
Operator : JC/MD
Sample : N5558-07 50X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
20BR-20221109DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------