

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043879.D
 Acq On : 15 Nov 2024 16:27
 Operator : JC/MD
 Sample : P4785-21
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 16 00:12:44 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 15 03:21:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	217569	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	199865	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	85071	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	59460	44.013	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.020%
7) Chloroethane-d5	1.721	69	3264	3.586	ug/L	0.07
Spiked Amount	50.000	Range	70 - 130	Recovery	=	7.180%#
11) 1,1-Dichloroethene-d2	2.294	65	30871	50.647	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.300%
21) 2-Butanone-d5	4.459	46	78247	108.918	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	108.920%
24) Chloroform-d	5.050	84	140819	48.992	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	97.980%
26) 1,2-Dichloroethane-d4	5.952	65	96533	52.591	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.180%
32) Benzene-d6	5.964	84	269281	48.426	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.860%
36) 1,2-Dichloropropane-d6	7.306	67	76728	48.449	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.900%
41) Toluene-d8	8.647	98	249593	47.470	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.940%
43) trans-1,3-Dichloroprop...	8.952	79	37271	46.698	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.400%
47) 2-Hexanone-d5	9.384	63	60555	103.802	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	103.800%
56) 1,1,2,2-Tetrachloroeth...	11.189	84	107798	49.468	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.940%
66) 1,2-Dichlorobenzene-d4	12.317	152	95614	53.876	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	107.760%
Target Compounds						
					Qvalue	
37) 1,2-Dichloropropane	7.306	63	9527	7.161	ug/L #	83
39) cis-1,3-Dichloropropene	8.318	75	2970	1.319	ug/L #	68
61) 1,2,3-Trichloropropane	12.018	75	9038	6.228	ug/L #	61


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043879.D
Acq On : 15 Nov 2024 16:27
Operator : JC/MD
Sample : P4785-21
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 16 00:12:44 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 15 03:21:47 2024
Response via : Initial Calibration




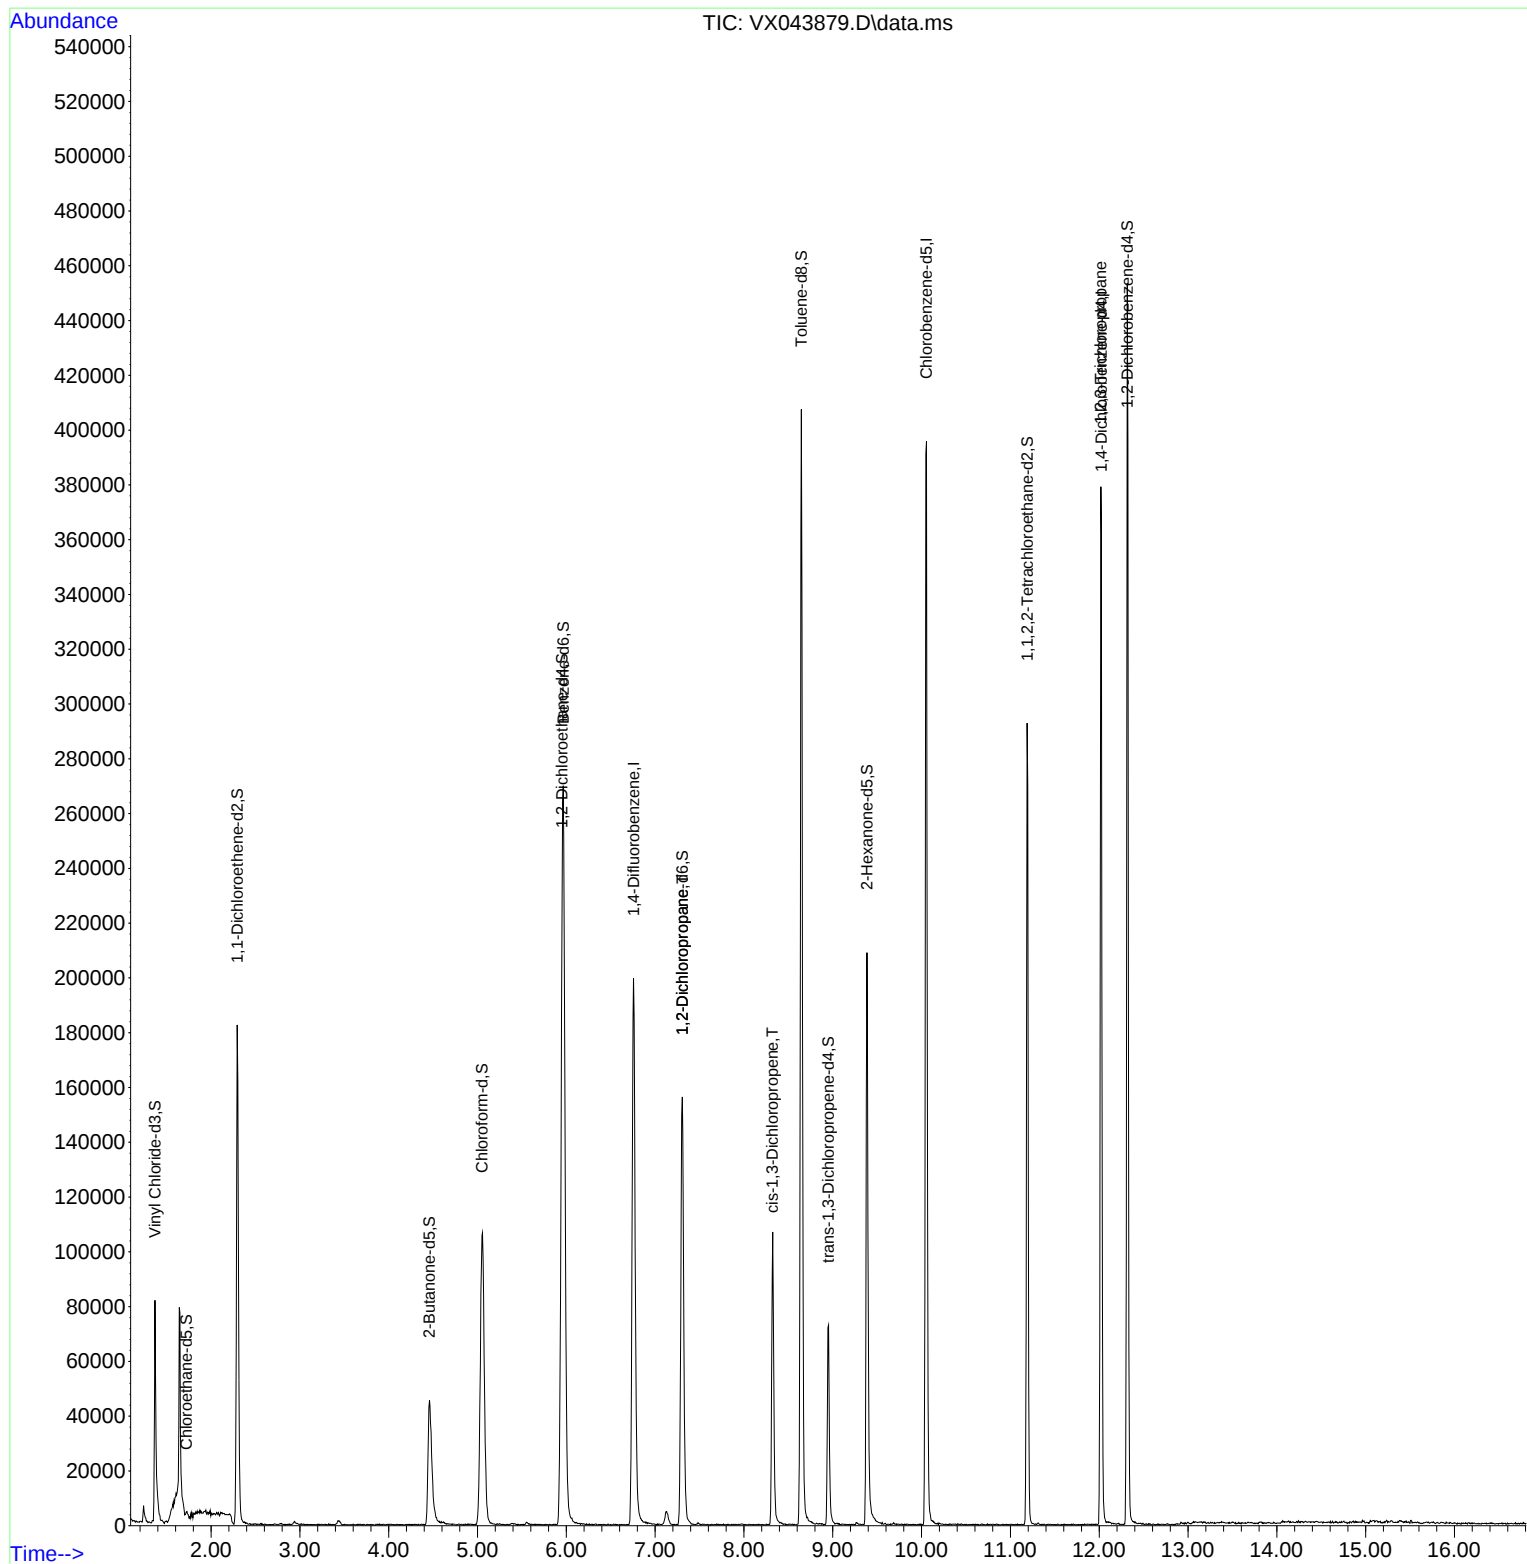


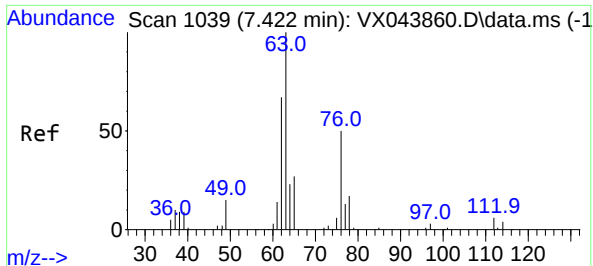

#37
1,2-Dichloropropane
Concen: 7.161 ug/L
RT: 7.306 min Scan# 1186
Delta R.T. -0.122 min
Lab File: VX043879.D
Acq: 15 Nov 2024 16:27




Instrument :
MSVOA_X
ClientSampleId :


Tgt Ion: 63 Resp: 9527
Ion Ratio Lower Upper
63 100
112 0.0 4.6 7.0#

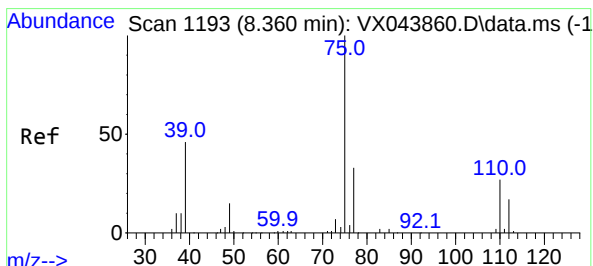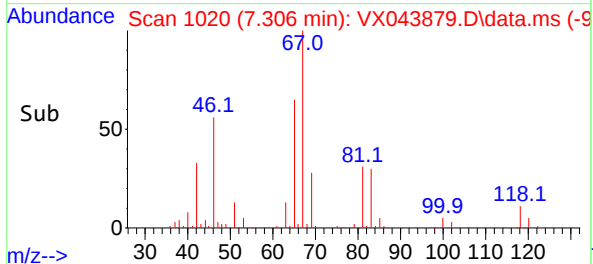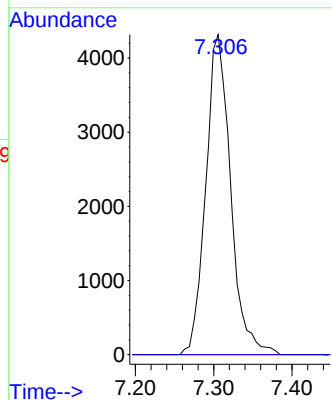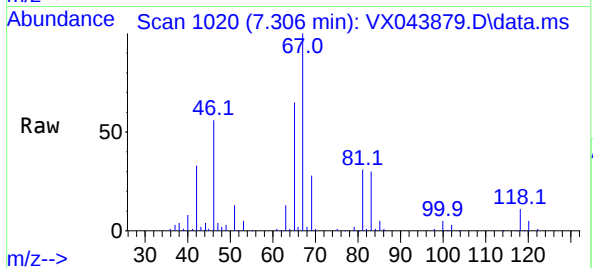

#39
cis-1,3-Dichloropropene
Concen: 1.319 ug/L
RT: 8.318 min Scan# 1186
Delta R.T. -0.043 min
Lab File: VX043879.D
Acq: 15 Nov 2024 16:27


Tgt Ion: 75 Resp: 2970
Ion Ratio Lower Upper
75 100
77 52.3 23.7 44.1#

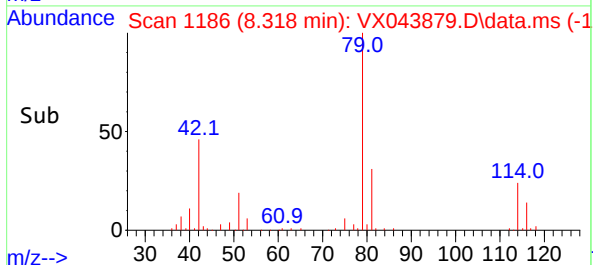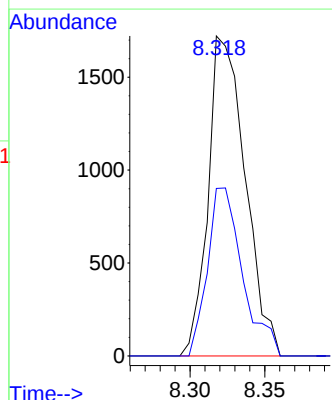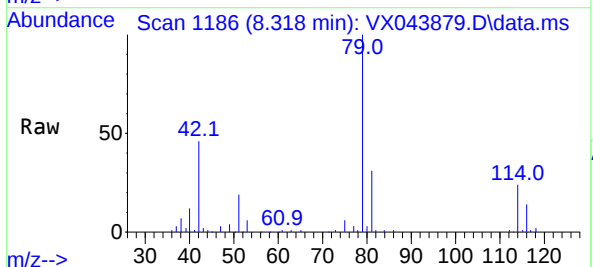

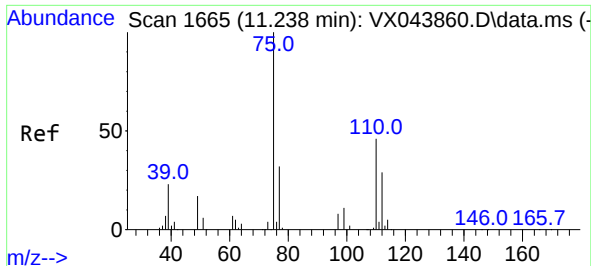

#61
1,2,3-Trichloropropane
Concen: 6.228 ug/L
RT: 12.018 min Scan# 11
Delta R.T. 0.780 min
Lab File: VX043879.D
Acq: 15 Nov 2024 16:27

Instrument :
MSVOA_X
ClientSampleId :

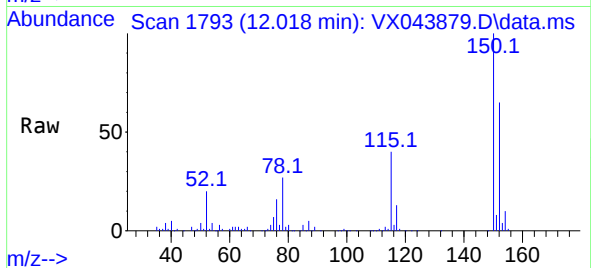

Tgt Ion: 75 Resp: 9038
Ion Ratio Lower Upper
75 100
77 33.9 25.7 38.5
110 4.2 37.0 55.6#

