

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043882.D
 Acq On : 15 Nov 2024 17:36
 Operator : JC/MD
 Sample : P4785-13
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 16 00:12:59 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 15 03:21:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	214258	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	189735	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	82411	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	57466	43.195	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.380%		
7) Chloroethane-d5	1.642	69	44367	49.492	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.980%		
11) 1,1-Dichloroethene-d2	2.294	65	30091	50.130	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	100.260%		
21) 2-Butanone-d5	4.458	46	77233	109.168	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	109.170%		
24) Chloroform-d	5.056	84	140320	49.573	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.140%		
26) 1,2-Dichloroethane-d4	5.952	65	95333	52.740	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	105.480%		
32) Benzene-d6	5.964	84	268434	50.851	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.700%		
36) 1,2-Dichloropropane-d6	7.305	67	77220	51.363	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	102.720%		
41) Toluene-d8	8.647	98	246043	49.293	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.580%		
43) trans-1,3-Dichloroprop...	8.951	79	35934	47.427	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.860%		
47) 2-Hexanone-d5	9.384	63	61595	111.222	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	111.220%		
56) 1,1,2,2-Tetrachloroeth...	11.189	84	107626	52.026	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	104.060%		
66) 1,2-Dichlorobenzene-d4	12.317	152	95755	55.697	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	111.400%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	8.324	75	3128	1.463	ug/L	93
61) 1,2,3-Trichloropropane	12.018	75	8583	6.106	ug/L #	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043882.D
Acq On : 15 Nov 2024 17:36
Operator : JC/MD
Sample : P4785-13
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 16 00:12:59 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 15 03:21:47 2024
Response via : Initial Calibration




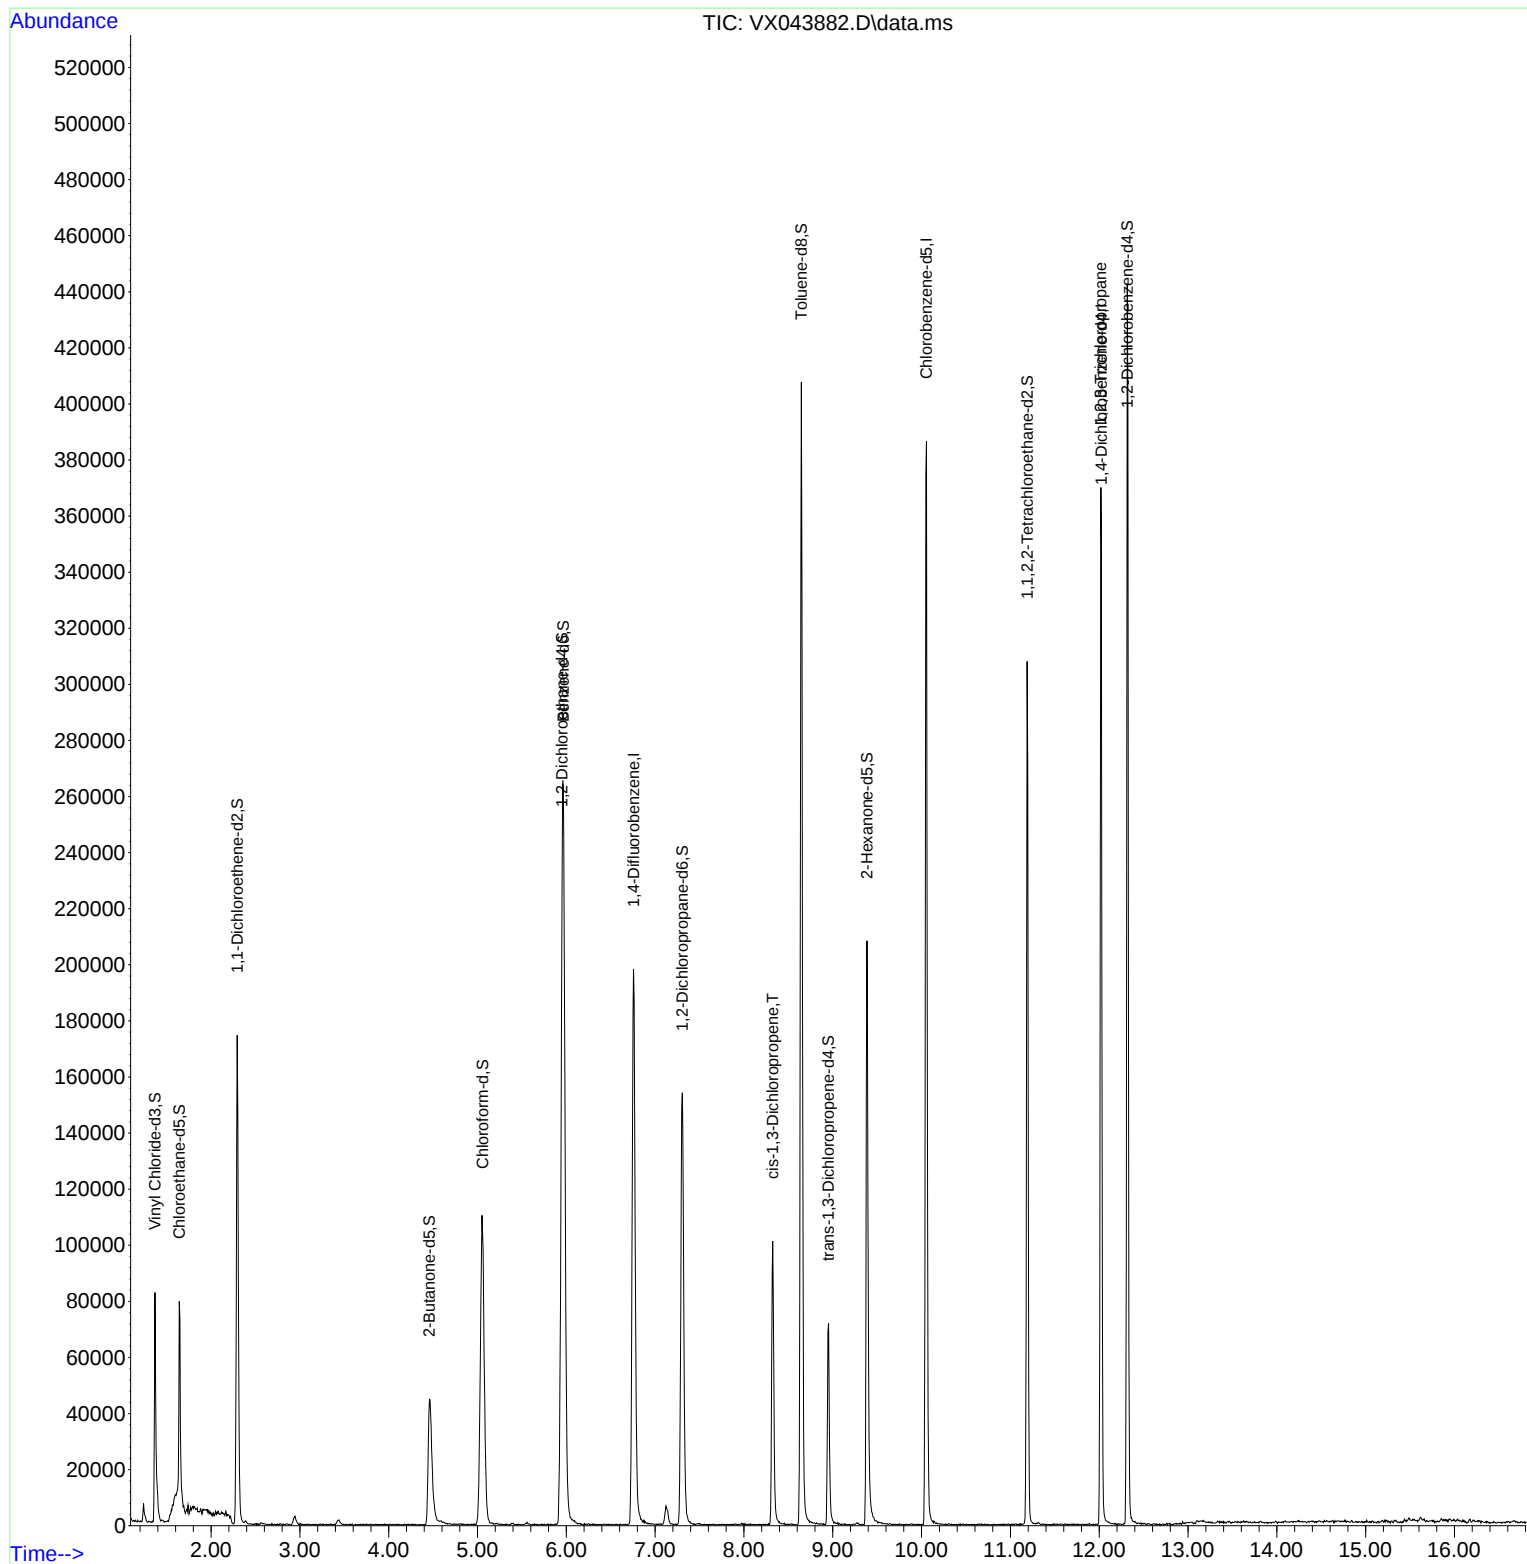


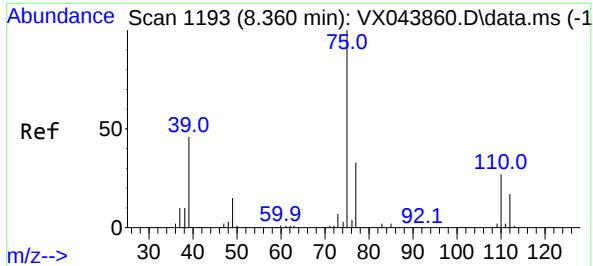

#39
cis-1,3-Dichloropropene
Concen: 1.463 ug/L
RT: 8.324 min Scan# 1193
Delta R.T. -0.037 min
Lab File: VX043882.D
Acq: 15 Nov 2024 17:36

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 3128
Ion Ratio Lower Upper
75 100
77 38.0 23.7 44.1

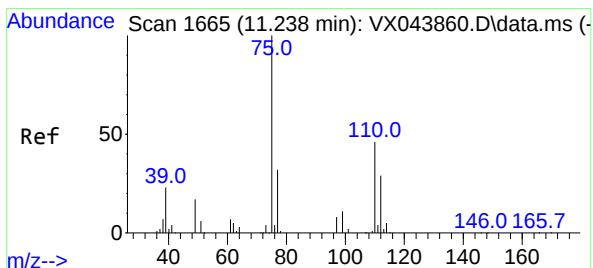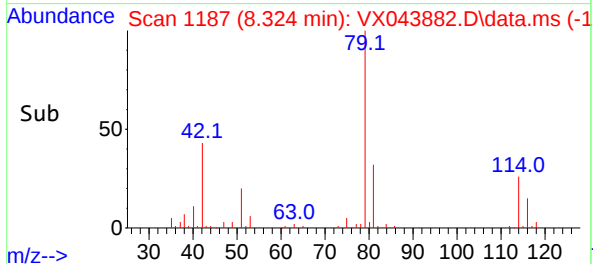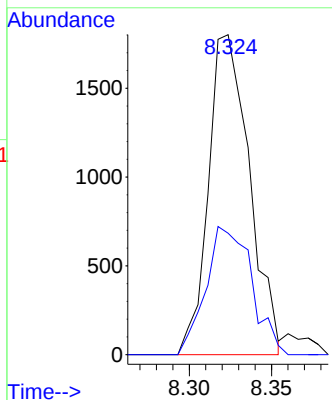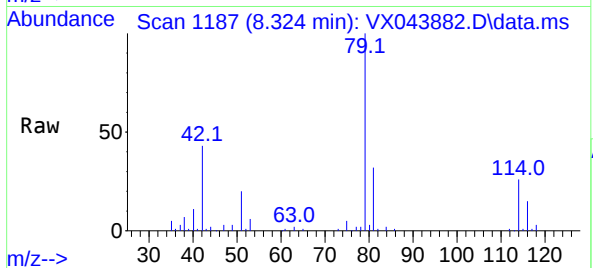

#61
1,2,3-Trichloropropane
Concen: 6.106 ug/L
RT: 12.018 min Scan# 1793
Delta R.T. 0.780 min
Lab File: VX043882.D
Acq: 15 Nov 2024 17:36

Tgt Ion: 75 Resp: 8583
Ion Ratio Lower Upper
75 100
77 36.5 25.7 38.5
110 4.2 37.0 55.6#

