

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043886.D
 Acq On : 15 Nov 2024 19:08
 Operator : JC/MD
 Sample : P4785-18
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :

Quant Time: Nov 16 00:13:34 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 15 03:21:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	221718	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	196646	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	86223	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.367	65	58355	42.387	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	84.780%	
7) Chloroethane-d5	1.648	69	52594	56.695	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	113.380%	
11) 1,1-Dichloroethene-d2	2.294	65	40349	64.958	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	129.920%#	
21) 2-Butanone-d5	4.458	46	78062	106.627	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	106.630%	
24) Chloroform-d	5.050	84	140867	48.092	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.180%	
26) 1,2-Dichloroethane-d4	5.952	65	96309	51.487	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	102.980%	
32) Benzene-d6	5.970	84	267961	48.978	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.960%	
36) 1,2-Dichloropropane-d6	7.305	67	123016	78.949	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	157.900%#	
41) Toluene-d8	8.653	98	394000	76.161	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	152.320%#	
43) trans-1,3-Dichloroprop...	8.951	79	42760	54.453	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	108.900%	
47) 2-Hexanone-d5	9.384	63	62696	109.231	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	109.230%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	111716	52.105	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	104.220%	
66) 1,2-Dichlorobenzene-d4	12.317	152	96744	53.784	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	107.560%	
Target Compounds						
					Qvalue	
44) trans-1,3-Dichloropropene	8.951	75	2247	1.093	ug/L #	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043886.D
Acq On : 15 Nov 2024 19:08
Operator : JC/MD
Sample : P4785-18
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :

Quant Time: Nov 16 00:13:34 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 15 03:21:47 2024
Response via : Initial Calibration

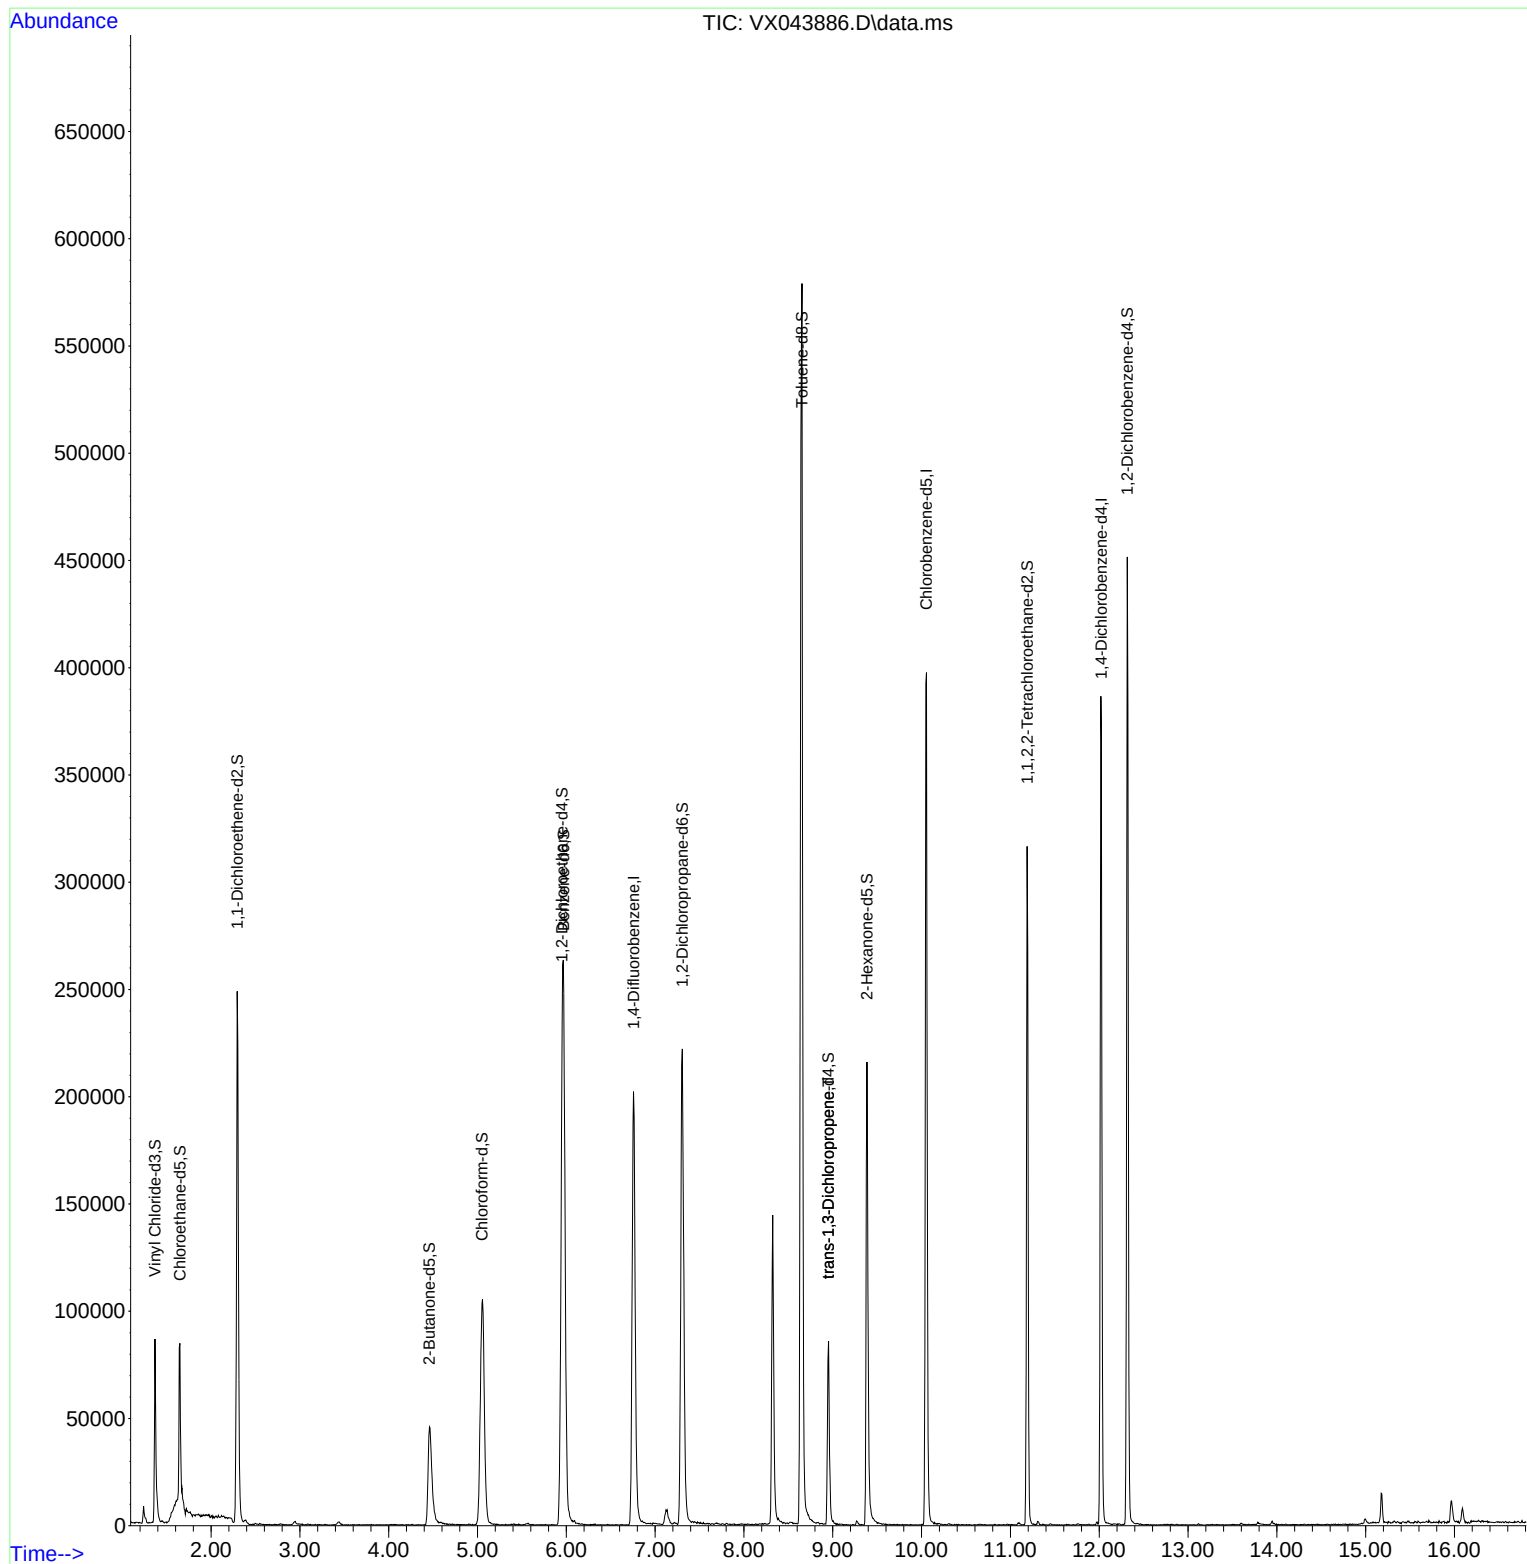

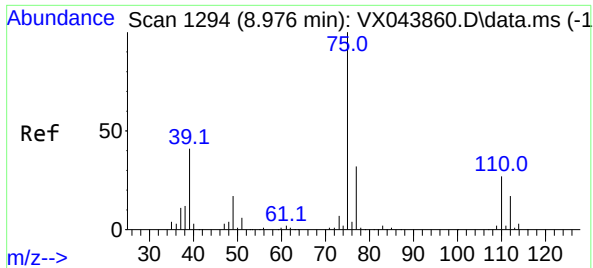

#44
trans-1,3-Dichloropropene
Concen: 1.093 ug/L
RT: 8.951 min Scan# 11
Delta R.T. -0.024 min
Lab File: VX043886.D
Acq: 15 Nov 2024 19:08

Instrument :
MSVOA_X
ClientSampleId :

Tgt Ion: 75 Resp: 2247
Ion Ratio Lower Upper
75 100
77 43.8 22.5 41.7#

