

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043878.D
 Acq On : 15 Nov 2024 16:03
 Operator : JC/MD
 Sample : P4785-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P1

Quant Time: Nov 16 00:12:39 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Nov 15 03:21:47 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.757	114	217142	50.000	ug/L	0.00
28) Chlorobenzene-d5	10.055	117	187612	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	12.024	152	133665	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.368	65	61407	45.544	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	91.080%	
7) Chloroethane-d5	1.648	69	46879	51.599	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	103.200%	
11) 1,1-Dichloroethene-d2	2.294	65	31231	51.338	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	102.680%	
21) 2-Butanone-d5	4.459	46	78814	109.923	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	109.920%	
24) Chloroform-d	5.050	84	142365	49.627	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.260%	
26) 1,2-Dichloroethane-d4	5.952	65	96889	52.889	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	105.780%	
32) Benzene-d6	5.964	84	277265	53.119	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	106.240%	
36) 1,2-Dichloropropane-d6	7.306	67	79321	53.358	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	106.720%	
41) Toluene-d8	8.647	98	256286	51.926	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	103.860%	
43) trans-1,3-Dichloroprop...	8.952	79	35954	47.990	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	95.980%	
47) 2-Hexanone-d5	9.385	63	63173	115.362	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	115.360%	
56) 1,1,2,2-Tetrachloroeth...	11.189	84	115443	56.436	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	112.880%	
66) 1,2-Dichlorobenzene-d4	12.317	152	155139	55.636	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	111.280%	
Target Compounds					Qvalue	
13) Acetone	2.386	43	4404	5.119	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043878.D
Acq On : 15 Nov 2024 16:03
Operator : JC/MD
Sample : P4785-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P1

Quant Time: Nov 16 00:12:39 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Nov 15 03:21:47 2024
Response via : Initial Calibration

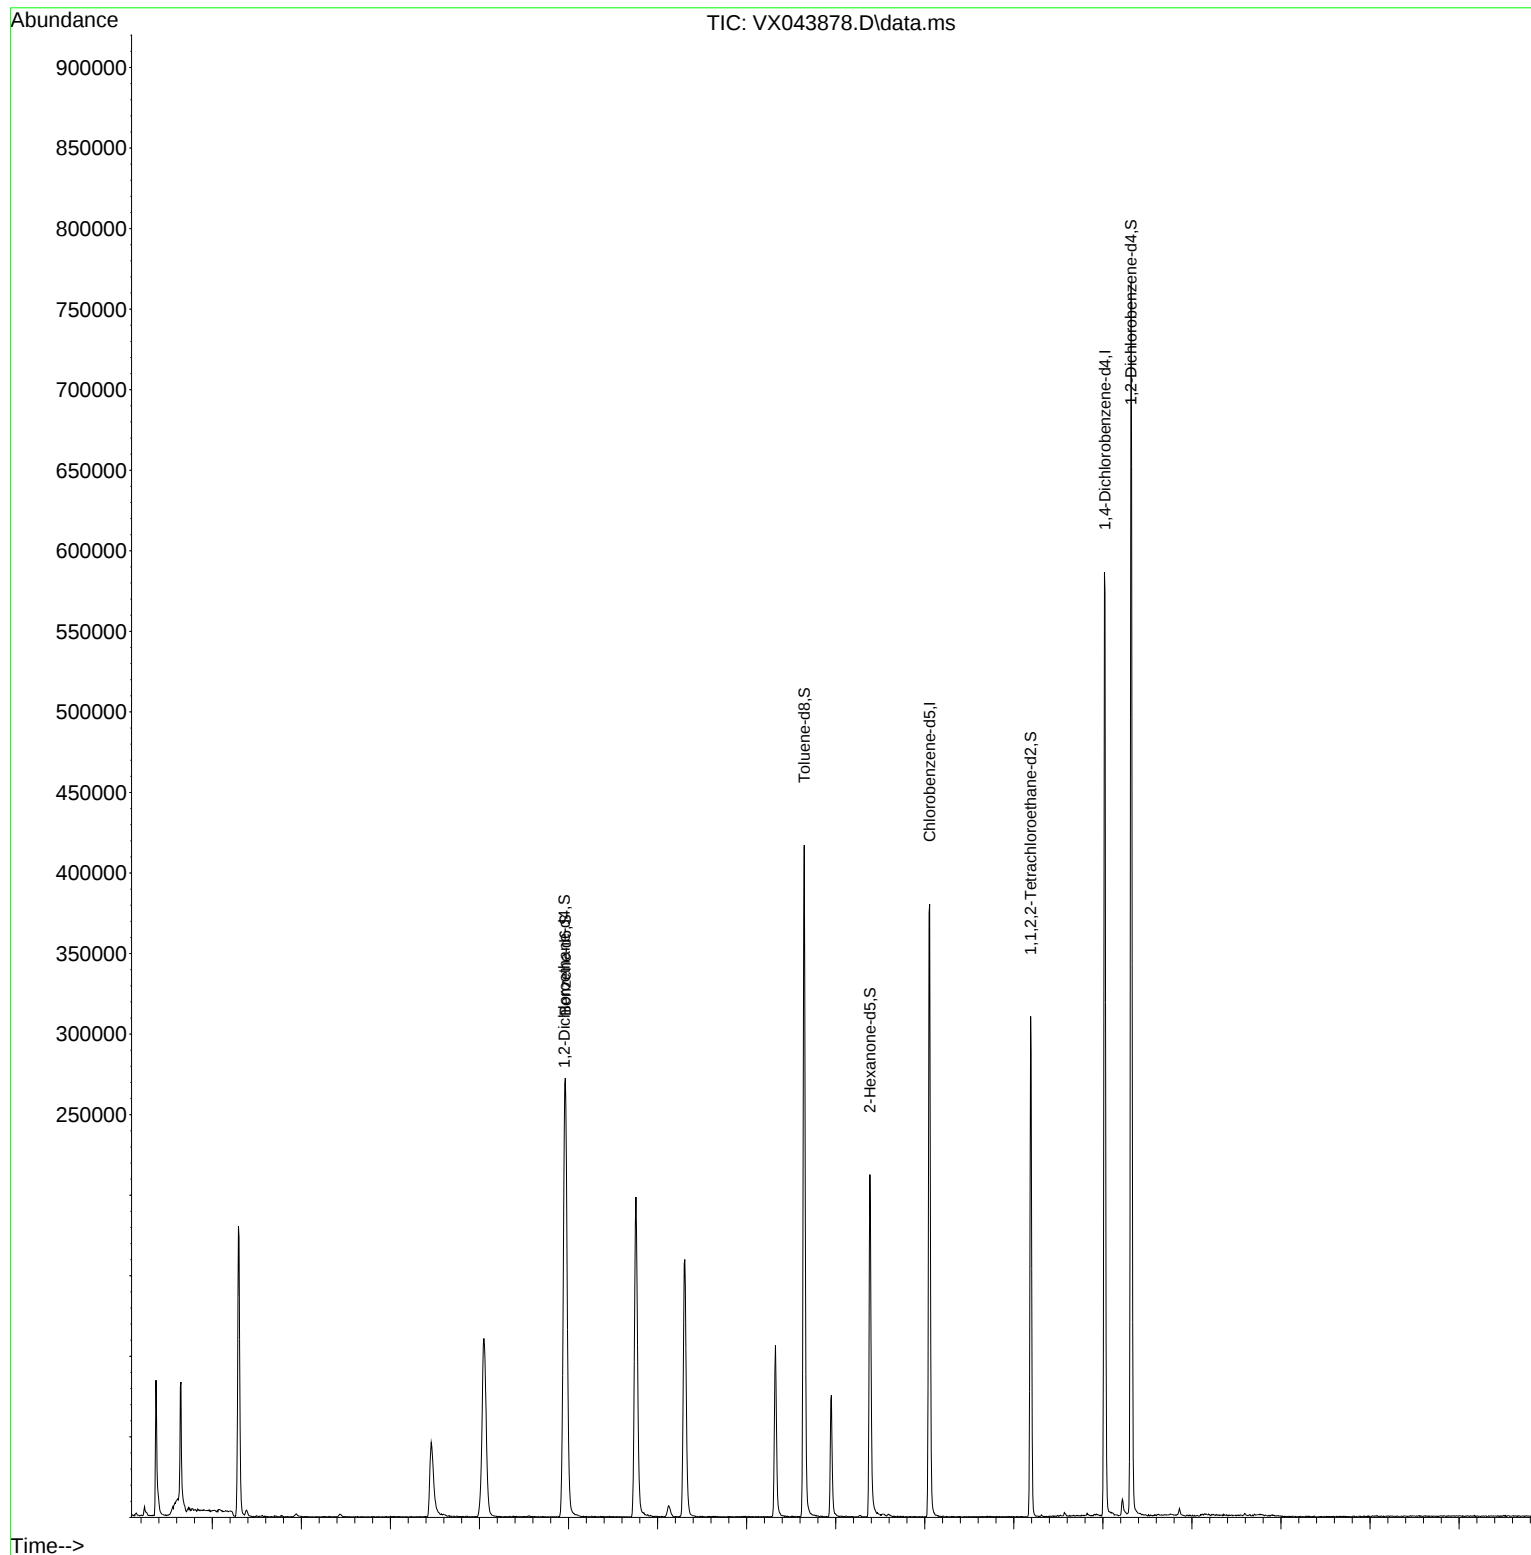

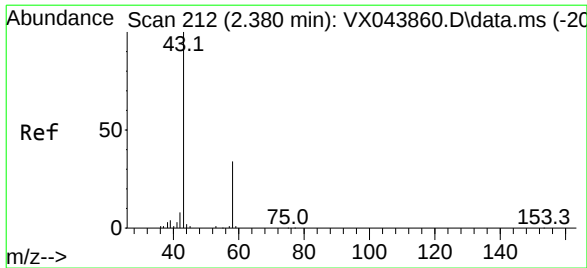

#13
 Acetone
 Concen: 5.119 ug/L
 RT: 2.386 min Scan# 21
 Delta R.T. 0.000 min
 Lab File: VX043878.D
 Acq: 15 Nov 2024 16:03

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P1

Tgt Ion: 43 Resp: 4404
 Ion Ratio Lower Upper
 43 100
 58 29.7 0.0 66.2

