

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043861.D
 Acq On : 15 Nov 2024 09:25
 Operator : JC/MD
 Sample : VX1115MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	23	25	28	rBV2	2625	2754	0.34%	0.045%
2	1.368	43	46	61	rVB	85266	116111	14.19%	1.896%
3	1.648	88	92	104	rVB	71513	112817	13.79%	1.842%
4	2.294	192	198	210	rVB	186552	295499	36.11%	4.825%
5	2.502	228	232	239	rVB2	1364	2400	0.29%	0.039%
6	2.709	264	266	268	rVB	308	215	0.03%	0.004%
7	2.782	274	278	282	rVB3	1082	1682	0.21%	0.027%
8	3.056	320	323	324	rBV	394	379	0.05%	0.006%
9	3.081	324	327	330	rBV2	912	1240	0.15%	0.020%
10	3.282	358	360	364	rBV3	215	262	0.03%	0.004%
11	3.428	379	384	385	rBV3	2823	4044	0.49%	0.066%
12	3.514	396	398	402	rBV2	249	285	0.03%	0.005%
13	3.611	412	414	417	rVB2	306	320	0.04%	0.005%
14	3.861	454	455	457	rVB2	473	271	0.03%	0.004%
15	3.892	457	460	461	rBV2	273	279	0.03%	0.005%
16	4.026	479	482	483	rBV2	281	218	0.03%	0.004%
17	4.148	500	502	507	rBV2	429	470	0.06%	0.008%
18	4.203	509	511	513	rBV2	245	244	0.03%	0.004%
19	4.306	526	528	530	rBV2	324	288	0.04%	0.005%
20	4.446	543	551	567	rBV	45100	143467	17.53%	2.343%
21	4.629	580	581	582	rVB	603	221	0.03%	0.004%
22	4.812	608	611	613	rBV3	258	334	0.04%	0.005%
23	4.952	631	634	635	rBV	341	228	0.03%	0.004%
24	5.044	638	649	665	rVV	112021	337810	41.28%	5.516%
25	5.385	699	705	709	rBV3	593	962	0.12%	0.016%
26	5.434	711	713	714	rBV	335	202	0.02%	0.003%
27	5.623	741	744	745	rVB2	279	266	0.03%	0.004%
28	5.672	748	752	754	rBV	244	282	0.03%	0.005%
29	5.806	772	774	777	rBV	412	315	0.04%	0.005%
30	5.958	787	799	819	rBV3	272091	818259	100.00%	13.361%
31	6.531	891	893	895	rBV	341	295	0.04%	0.005%
32	6.617	905	907	909	rBV2	312	288	0.04%	0.005%
33	6.751	918	929	944	rBV	203574	497808	60.84%	8.129%
34	7.123	982	990	1001	rBV5	15644	37680	4.60%	0.615%
35	7.300	1010	1019	1035	rBV	160353	361482	44.18%	5.903%
36	7.495	1050	1051	1053	rVB	627	306	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043861.D
 Acq On : 15 Nov 2024 09:25
 Operator : JC/MD
 Sample : VX1115MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	7.592	1065	1067	1069	rBV	495	618	0.08%	0.010%
38	7.696	1082	1084	1086	rBV2	289	259	0.03%	0.004%
39	7.739	1090	1091	1093	rVB	371	247	0.03%	0.004%
40	7.964	1125	1128	1130	rVB3	286	322	0.04%	0.005%
41	8.086	1146	1148	1150	rVB2	357	253	0.03%	0.004%
42	8.110	1150	1152	1154	rBV2	330	238	0.03%	0.004%
43	8.159	1158	1160	1162	rBV2	228	223	0.03%	0.004%
44	8.318	1181	1186	1201	rBV	106027	182524	22.31%	2.980%
45	8.641	1233	1239	1251	rBV	416885	669517	81.82%	10.932%
46	8.891	1275	1280	1282	rBV2	383	565	0.07%	0.009%
47	8.946	1284	1289	1296	rBV	75668	117334	14.34%	1.916%
48	9.165	1323	1325	1327	rBV2	476	370	0.05%	0.006%
49	9.269	1339	1342	1346	rVB4	1590	1942	0.24%	0.032%
50	9.385	1356	1361	1387	rVV	207719	321412	39.28%	5.248%
51	9.592	1393	1395	1396	rBV2	437	389	0.05%	0.006%
52	9.671	1406	1408	1410	rBV	354	248	0.03%	0.004%
53	9.933	1449	1451	1454	rVB2	320	275	0.03%	0.004%
54	10.049	1465	1470	1482	rBV	417299	571147	69.80%	9.326%
55	10.305	1510	1512	1518	rVB2	1619	2022	0.25%	0.033%
56	10.561	1552	1554	1556	rBV3	284	351	0.04%	0.006%
57	10.640	1563	1567	1570	rBV5	1163	1904	0.23%	0.031%
58	10.701	1576	1577	1581	rVB	429	247	0.03%	0.004%
59	10.769	1587	1588	1591	rBV	294	205	0.03%	0.003%
60	11.189	1651	1657	1667	rBV	304862	385601	47.12%	6.296%
61	11.384	1688	1689	1690	rBV	585	242	0.03%	0.004%
62	11.451	1696	1700	1704	rBV3	1129	2006	0.25%	0.033%
63	11.756	1746	1750	1753	rVB4	1240	1767	0.22%	0.029%
64	11.817	1759	1760	1766	rVB2	348	486	0.06%	0.008%
65	11.860	1766	1767	1770	rBV2	333	294	0.04%	0.005%
66	11.976	1782	1786	1788	rBV2	1958	2397	0.29%	0.039%
67	12.018	1788	1793	1811	rVB	400105	519516	63.49%	8.483%
68	12.250	1830	1831	1834	rBV3	321	274	0.03%	0.004%
69	12.317	1837	1842	1860	rVB	446637	575305	70.31%	9.394%
70	12.579	1883	1885	1887	rBV	214	234	0.03%	0.004%
71	12.634	1892	1894	1897	rVB2	353	262	0.03%	0.004%
72	12.658	1897	1898	1900	rBV2	244	205	0.03%	0.003%
73	12.762	1913	1915	1916	rVB2	451	286	0.03%	0.005%
74	12.780	1916	1918	1921	rBV2	338	486	0.06%	0.008%
75	12.811	1921	1923	1925	rVB2	287	230	0.03%	0.004%
76	12.902	1936	1938	1940	rBV	347	241	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043861.D
 Acq On : 15 Nov 2024 09:25
 Operator : JC/MD
 Sample : VX1115MBL01
 Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK727

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.921	1940	1941	1943	rBV2	290	286	0.03%	0.005%
78	13.122	1969	1974	1978	rVV6	1753	2306	0.28%	0.038%
79	13.152	1978	1979	1985	rVB3	362	581	0.07%	0.009%
80	13.225	1988	1991	1994	rBV2	282	397	0.05%	0.006%
81	13.366	2012	2014	2016	rBV2	259	249	0.03%	0.004%
82	13.402	2019	2020	2022	rBV2	224	205	0.03%	0.003%
83	13.597	2048	2052	2057	rBV5	2122	3120	0.38%	0.051%
84	13.701	2068	2069	2072	rBV2	297	295	0.04%	0.005%
85	13.756	2076	2078	2079	rBV	530	478	0.06%	0.008%
86	13.780	2079	2082	2087	rVB2	2765	3989	0.49%	0.065%
87	13.963	2109	2112	2120	rBV5	2302	3663	0.45%	0.060%
88	14.402	2181	2184	2185	rBV2	344	315	0.04%	0.005%
89	14.561	2209	2210	2213	rBV2	380	324	0.04%	0.005%
90	14.792	2246	2248	2252	rBV2	308	298	0.04%	0.005%
91	14.859	2258	2259	2262	rBV3	326	249	0.03%	0.004%
92	14.951	2272	2274	2275	rBV	445	294	0.04%	0.005%
93	15.554	2371	2373	2376	rBV2	604	790	0.10%	0.013%
94	15.579	2376	2377	2382	rVB3	595	596	0.07%	0.010%
95	15.615	2382	2383	2384	rBV	539	257	0.03%	0.004%
96	16.292	2492	2494	2497	rBV2	497	625	0.08%	0.010%
97	16.524	2529	2532	2533	rBV	608	524	0.06%	0.009%
98	16.560	2536	2538	2540	rBV2	605	488	0.06%	0.008%
99	16.658	2552	2554	2556	rVB2	909	790	0.10%	0.013%
100	16.682	2556	2558	2560	rBV	533	560	0.07%	0.009%

Sum of corrected areas: 6124106




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043861.D
Acq On : 15 Nov 2024 09:25
Operator : JC/MD
Sample : VX1115MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK727

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

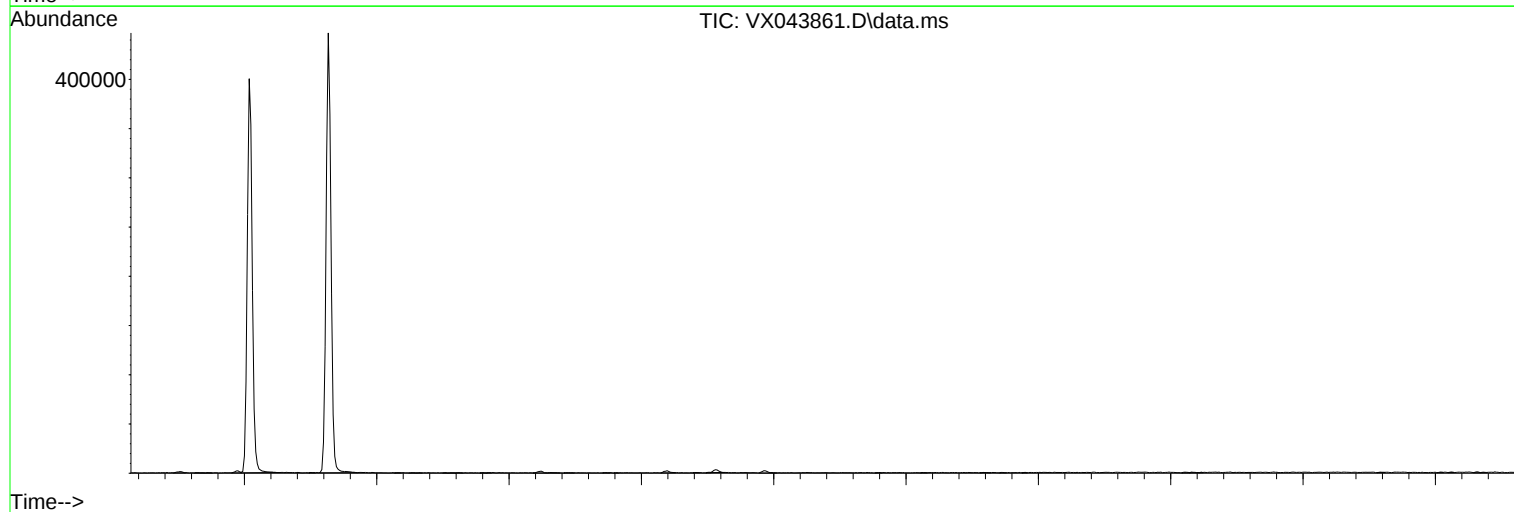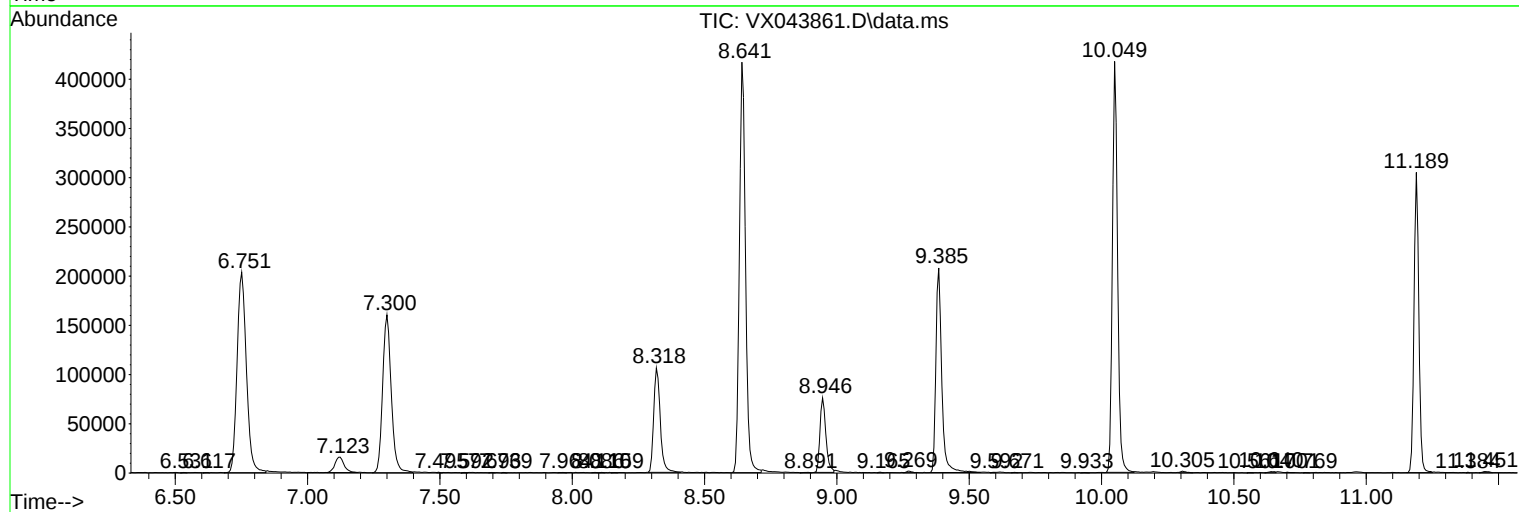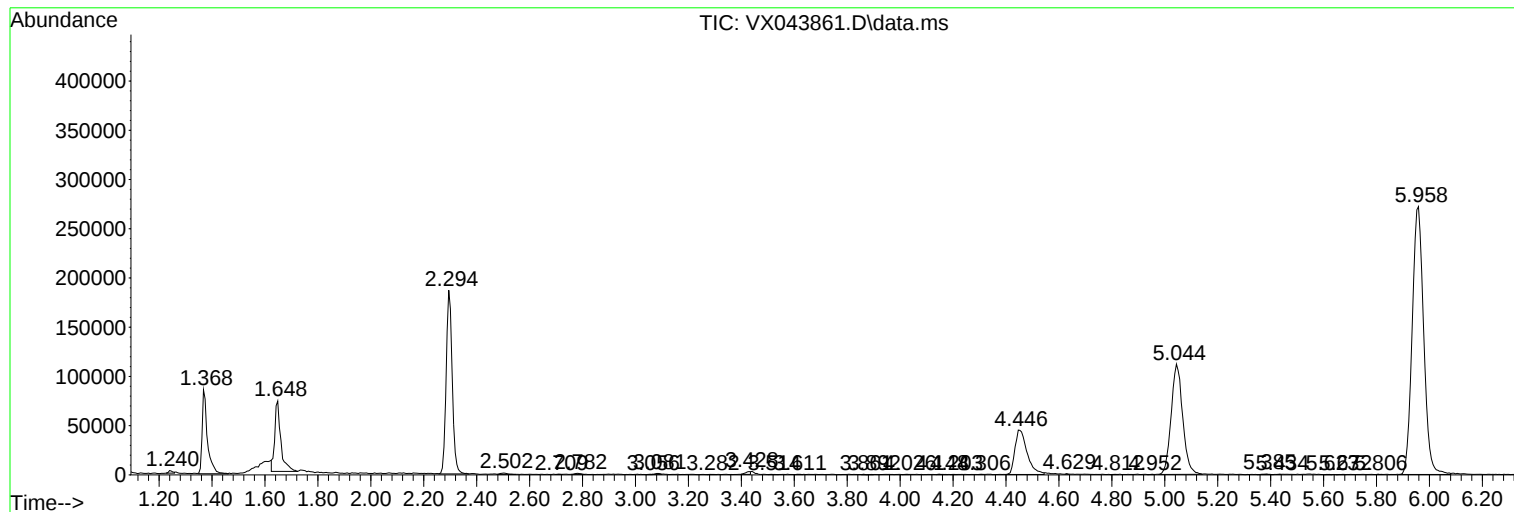

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043861.D
Acq On : 15 Nov 2024 09:25
Operator : JC/MD
Sample : VX1115MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK727

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043861.D
Acq On : 15 Nov 2024 09:25
Operator : JC/MD
Sample : VX1115MBL01
Misc : 5.00g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK727

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
