

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043862.D
 Acq On : 15 Nov 2024 09:47
 Operator : JC/MD
 Sample : VX1115WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK728

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	28	rBV	3593	4350	0.49%	0.067%
2	1.367	43	46	60	rVB	85734	114709	13.04%	1.770%
3	1.648	89	92	106	rVB	78727	126164	14.34%	1.946%
4	2.294	192	198	210	rVB	197845	305608	34.73%	4.714%
5	2.446	221	223	225	rBV2	621	545	0.06%	0.008%
6	2.483	228	229	230	rBV	584	366	0.04%	0.006%
7	2.635	252	254	258	rVB3	319	422	0.05%	0.007%
8	2.678	258	261	263	rBV	385	453	0.05%	0.007%
9	2.782	274	278	281	rBV3	940	1554	0.18%	0.024%
10	2.824	284	285	289	rVB2	345	303	0.03%	0.005%
11	2.940	303	304	305	rBV	482	291	0.03%	0.004%
12	3.020	315	317	321	rVB2	426	469	0.05%	0.007%
13	3.087	326	328	331	rVB2	390	488	0.06%	0.008%
14	3.172	340	342	347	rBV2	180	263	0.03%	0.004%
15	3.239	351	353	356	rVB2	308	291	0.03%	0.004%
16	3.312	364	365	368	rVB	308	259	0.03%	0.004%
17	3.343	368	370	371	rBV2	289	242	0.03%	0.004%
18	3.434	378	385	391	rBV4	2081	4677	0.53%	0.072%
19	3.660	420	422	423	rVB	331	225	0.03%	0.003%
20	3.721	429	432	433	rVB	359	286	0.03%	0.004%
21	3.733	433	434	436	rBV	248	261	0.03%	0.004%
22	4.263	519	521	526	rVB2	310	424	0.05%	0.007%
23	4.458	545	553	570	rVV	43643	138973	15.79%	2.144%
24	4.592	573	575	578	rVV4	883	1004	0.11%	0.015%
25	4.647	582	584	588	rVB3	580	530	0.06%	0.008%
26	4.934	630	631	636	rVB2	255	259	0.03%	0.004%
27	5.044	636	649	667	rBV	116159	364908	41.47%	5.629%
28	5.214	675	677	681	rVB2	362	357	0.04%	0.006%
29	5.312	691	693	696	rVB2	314	266	0.03%	0.004%
30	5.379	701	704	705	rBV2	487	459	0.05%	0.007%
31	5.537	728	730	731	rBV	430	351	0.04%	0.005%
32	5.726	757	761	762	rVB2	324	407	0.05%	0.006%
33	5.958	788	799	821	rBV2	291058	879954	100.00%	13.574%
34	6.348	860	863	865	rBV2	437	483	0.05%	0.007%
35	6.373	865	867	869	rVV2	369	312	0.04%	0.005%
36	6.421	874	875	876	rBV2	381	233	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043862.D
 Acq On : 15 Nov 2024 09:47
 Operator : JC/MD
 Sample : VX1115WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK728

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Title : VOC Analysis

37	6.458	879	881	883	rBV2	249	224	0.03%	0.003%
38	6.659	912	914	920	rBV2	191	247	0.03%	0.004%
39	6.751	920	929	946	rBV	220237	553238	62.87%	8.534%
40	7.043	975	977	980	rBV2	297	323	0.04%	0.005%
41	7.122	980	990	1002	rVV5	9996	25317	2.88%	0.391%
42	7.305	1011	1020	1037	rBV	172729	388959	44.20%	6.000%
43	7.805	1099	1102	1103	rBV2	559	604	0.07%	0.009%
44	7.854	1107	1110	1111	rBV	312	275	0.03%	0.004%
45	7.878	1113	1114	1117	rVB	347	289	0.03%	0.004%
46	7.909	1117	1119	1121	rBV2	395	389	0.04%	0.006%
47	8.025	1136	1138	1140	rVB2	291	252	0.03%	0.004%
48	8.153	1157	1159	1161	rVB2	479	345	0.04%	0.005%
49	8.183	1161	1164	1165	rBV2	244	233	0.03%	0.004%
50	8.323	1181	1187	1200	rBV	116362	198785	22.59%	3.066%
51	8.537	1220	1222	1225	rBV2	333	347	0.04%	0.005%
52	8.647	1233	1240	1251	rBV	437074	706774	80.32%	10.903%
53	8.890	1278	1280	1284	rBV2	296	327	0.04%	0.005%
54	8.945	1284	1289	1301	rBV	79399	126957	14.43%	1.958%
55	9.232	1332	1336	1337	rBV2	324	337	0.04%	0.005%
56	9.275	1341	1343	1347	rVB3	617	923	0.10%	0.014%
57	9.384	1356	1361	1380	rBV	214131	323353	36.75%	4.988%
58	9.604	1396	1397	1402	rBV3	470	552	0.06%	0.009%
59	9.665	1405	1407	1410	rVB	265	253	0.03%	0.004%
60	10.049	1465	1470	1481	rBV	448710	627829	71.35%	9.685%
61	10.280	1506	1508	1510	rBV	296	254	0.03%	0.004%
62	10.390	1522	1526	1527	rBV	384	427	0.05%	0.007%
63	10.469	1536	1539	1540	rBV2	644	544	0.06%	0.008%
64	10.591	1557	1559	1563	rVB2	304	300	0.03%	0.005%
65	10.854	1599	1602	1604	rBV2	351	538	0.06%	0.008%
66	11.189	1652	1657	1668	rBV	322470	403672	45.87%	6.227%
67	11.360	1683	1685	1688	rVB	408	316	0.04%	0.005%
68	11.396	1688	1691	1692	rBV	398	294	0.03%	0.005%
69	11.573	1716	1720	1721	rBV3	256	251	0.03%	0.004%
70	11.591	1721	1723	1725	rBV	283	258	0.03%	0.004%
71	11.750	1747	1749	1752	rBV2	513	585	0.07%	0.009%
72	11.817	1757	1760	1763	rBV3	262	269	0.03%	0.004%
73	11.975	1783	1786	1788	rVB3	691	780	0.09%	0.012%
74	12.018	1788	1793	1803	rBV	447287	559395	63.57%	8.629%
75	12.256	1830	1832	1834	rBV	338	279	0.03%	0.004%
76	12.317	1837	1842	1854	rVV	452547	595771	67.70%	9.190%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043862.D
 Acq On : 15 Nov 2024 09:47
 Operator : JC/MD
 Sample : VX1115WBL01
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VBLK728

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.457	1863	1865	1866	rBV	435	242	0.03%	0.004%
78	12.603	1886	1889	1890	rBV	317	360	0.04%	0.006%
79	12.731	1909	1910	1913	rVB	397	284	0.03%	0.004%
80	13.566	2045	2047	2048	rBV	392	296	0.03%	0.005%
81	13.652	2058	2061	2063	rBV2	324	440	0.05%	0.007%
82	13.786	2080	2083	2089	rVB4	845	1316	0.15%	0.020%
83	13.938	2105	2108	2110	rBV2	269	240	0.03%	0.004%
84	13.963	2110	2112	2115	rBV	448	534	0.06%	0.008%
85	14.048	2125	2126	2132	rVB2	235	266	0.03%	0.004%
86	14.121	2136	2138	2139	rBV2	399	247	0.03%	0.004%
87	14.231	2153	2156	2158	rBV3	327	443	0.05%	0.007%
88	14.255	2158	2160	2163	rVV3	218	243	0.03%	0.004%
89	14.475	2193	2196	2200	rVB3	415	481	0.05%	0.007%
90	14.511	2200	2202	2204	rBV2	414	469	0.05%	0.007%
91	14.615	2214	2219	2220	rBV3	549	706	0.08%	0.011%
92	14.633	2220	2222	2223	rVB	392	247	0.03%	0.004%
93	14.786	2245	2247	2249	rVB2	388	264	0.03%	0.004%
94	15.030	2285	2287	2288	rBV	442	410	0.05%	0.006%
95	15.231	2318	2320	2322	rVB2	408	327	0.04%	0.005%
96	15.438	2352	2354	2356	rBV2	392	243	0.03%	0.004%
97	15.475	2358	2360	2363	rVB3	621	460	0.05%	0.007%
98	15.499	2363	2364	2369	rVB3	480	601	0.07%	0.009%
99	16.304	2495	2496	2502	rVB3	769	811	0.09%	0.013%
100	16.694	2558	2560	2561	rBV2	437	378	0.04%	0.006%

Sum of corrected areas: 6482519




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043862.D
Acq On : 15 Nov 2024 09:47
Operator : JC/MD
Sample : VX1115WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK728

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

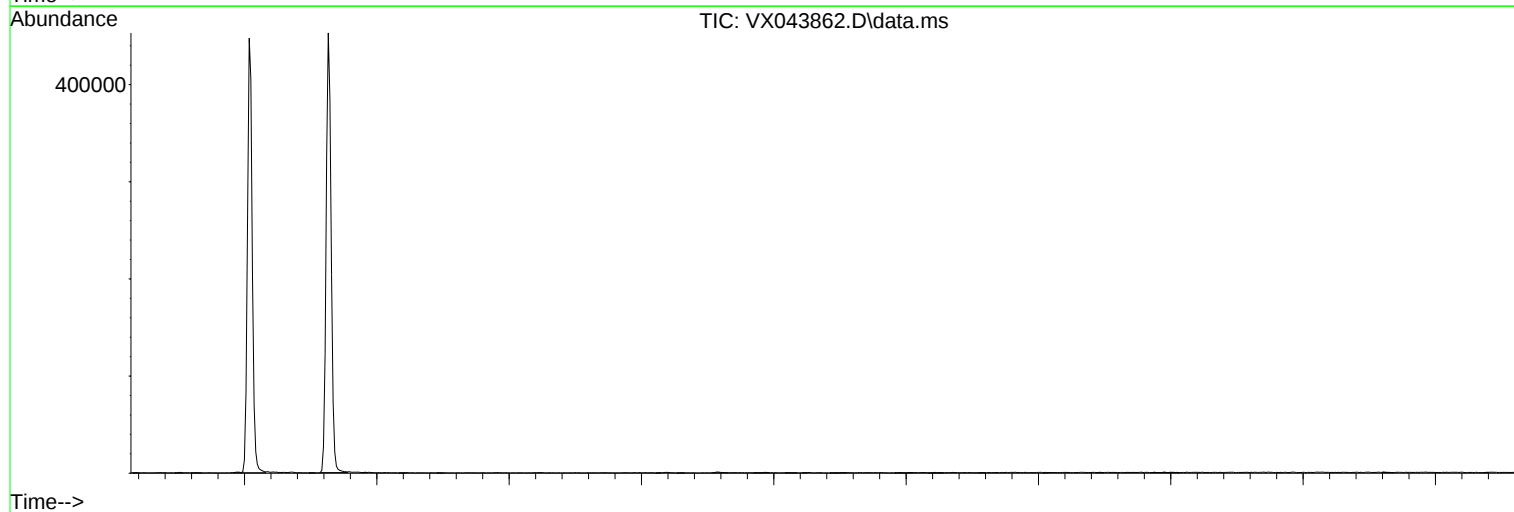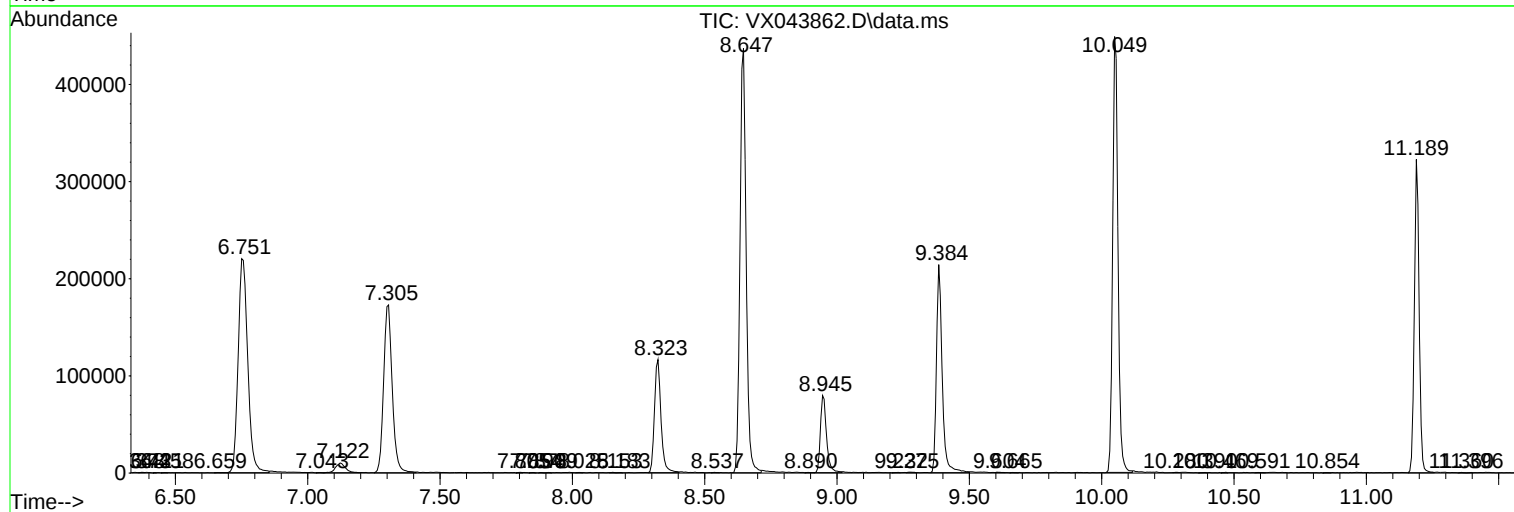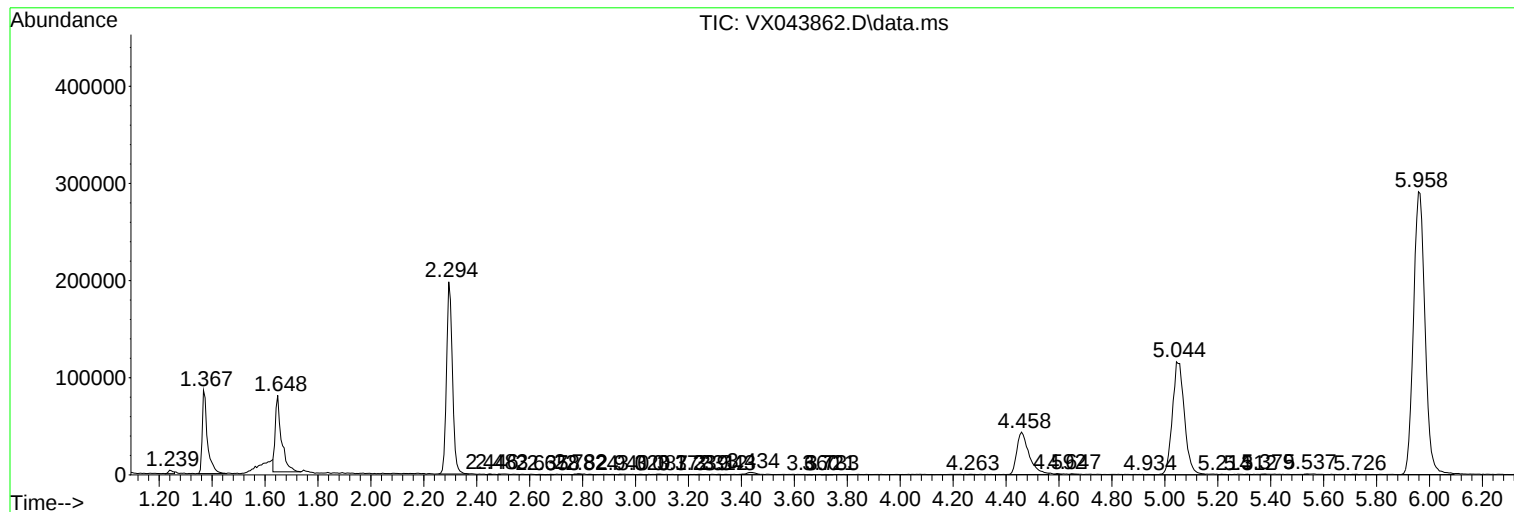

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043862.D
Acq On : 15 Nov 2024 09:47
Operator : JC/MD
Sample : VX1115WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK728

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043862.D
Acq On : 15 Nov 2024 09:47
Operator : JC/MD
Sample : VX1115WBL01
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VBLK728

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc