

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043865.D
 Acq On : 15 Nov 2024 11:05
 Operator : JC/MD
 Sample : P4782-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	27	rBV	4653	5153	0.62%	0.084%
2	1.368	43	46	57	rVB	87605	106601	12.85%	1.742%
3	1.648	88	92	103	rVB	76877	104776	12.63%	1.713%
4	2.294	192	198	210	rVV	182836	292749	35.29%	4.785%
5	2.380	210	212	218	rVB4	761	934	0.11%	0.015%
6	2.496	227	231	232	rBV3	421	589	0.07%	0.010%
7	2.630	250	253	256	rBV3	392	651	0.08%	0.011%
8	2.697	262	264	267	rVB2	253	303	0.04%	0.005%
9	2.782	274	278	281	rVB	723	730	0.09%	0.012%
10	2.922	299	301	302	rBV	396	260	0.03%	0.004%
11	3.404	379	380	381	rVV	597	312	0.04%	0.005%
12	3.428	381	384	391	rVB4	1912	4075	0.49%	0.067%
13	3.483	391	393	396	rBV	434	342	0.04%	0.006%
14	3.526	396	400	403	rBV2	230	368	0.04%	0.006%
15	3.739	432	435	436	rVB	316	250	0.03%	0.004%
16	3.764	436	439	441	rBV2	356	353	0.04%	0.006%
17	3.831	447	450	451	rVV	380	341	0.04%	0.006%
18	3.849	451	453	455	rVV2	384	225	0.03%	0.004%
19	3.928	464	466	468	rBV2	454	454	0.05%	0.007%
20	3.971	470	473	474	rBV	200	245	0.03%	0.004%
21	4.294	524	526	530	rBV2	484	447	0.05%	0.007%
22	4.453	544	552	568	rBV	43248	137155	16.53%	2.242%
23	4.806	608	610	612	rBV	418	372	0.04%	0.006%
24	5.044	635	649	669	rBV	107376	343654	41.43%	5.617%
25	5.373	698	703	704	rBV3	674	950	0.11%	0.016%
26	5.452	715	716	719	rVB3	472	348	0.04%	0.006%
27	5.532	727	729	730	rBV	602	508	0.06%	0.008%
28	5.666	750	751	755	rVB2	218	224	0.03%	0.004%
29	5.843	778	780	785	rVB2	205	255	0.03%	0.004%
30	5.964	788	800	817	rBV3	277444	829486	100.00%	13.558%
31	6.294	853	854	856	rBV	320	296	0.04%	0.005%
32	6.757	919	930	948	rBV	193800	477037	57.51%	7.797%
33	7.117	982	989	1002	rBV	55653	130392	15.72%	2.131%
34	7.306	1011	1020	1030	rBV	163817	365672	44.08%	5.977%
35	7.440	1040	1042	1044	rBV3	251	269	0.03%	0.004%
36	7.934	1120	1123	1124	rBV	352	270	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043865.D
 Acq On : 15 Nov 2024 11:05
 Operator : JC/MD
 Sample : P4782-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	8.165	1159	1161	1162	rBV	251	214	0.03%	0.003%
38	8.263	1173	1177	1180	rBV3	232	324	0.04%	0.005%
39	8.324	1180	1187	1197	rBV	106963	186749	22.51%	3.052%
40	8.647	1233	1240	1251	rBV	410940	673748	81.22%	11.012%
41	8.946	1284	1289	1301	rVV	75321	118501	14.29%	1.937%
42	9.183	1326	1328	1330	rBV	268	220	0.03%	0.004%
43	9.275	1339	1343	1348	rVB2	1348	2070	0.25%	0.034%
44	9.385	1356	1361	1372	rBV	205674	313951	37.85%	5.132%
45	9.793	1426	1428	1432	rBV2	230	248	0.03%	0.004%
46	9.952	1453	1454	1457	rVB2	408	234	0.03%	0.004%
47	10.049	1465	1470	1483	rBV	380035	543245	65.49%	8.879%
48	10.305	1509	1512	1515	rBV2	742	900	0.11%	0.015%
49	10.464	1536	1538	1539	rBV2	303	276	0.03%	0.005%
50	10.586	1556	1558	1562	rVB	422	380	0.05%	0.006%
51	10.622	1562	1564	1565	rBV	342	244	0.03%	0.004%
52	10.647	1565	1568	1571	rBV4	470	637	0.08%	0.010%
53	10.823	1595	1597	1599	rVB	466	266	0.03%	0.004%
54	10.854	1599	1602	1604	rBV3	304	325	0.04%	0.005%
55	10.964	1618	1620	1623	rVB	511	431	0.05%	0.007%
56	11.031	1630	1631	1634	rBV	346	246	0.03%	0.004%
57	11.055	1634	1635	1638	rBV2	202	250	0.03%	0.004%
58	11.189	1651	1657	1666	rBV	312132	400165	48.24%	6.541%
59	11.311	1674	1677	1680	rVB3	1421	1531	0.18%	0.025%
60	11.342	1680	1682	1686	rVB2	320	343	0.04%	0.006%
61	11.439	1695	1698	1700	rBV2	361	331	0.04%	0.005%
62	11.457	1700	1701	1703	rVV	463	332	0.04%	0.005%
63	11.506	1707	1709	1711	rBV	348	275	0.03%	0.004%
64	11.531	1711	1713	1715	rBV	348	372	0.04%	0.006%
65	11.762	1747	1751	1756	rBV3	660	805	0.10%	0.013%
66	11.811	1757	1759	1761	rVB	399	311	0.04%	0.005%
67	11.841	1761	1764	1766	rBV2	226	316	0.04%	0.005%
68	11.976	1783	1786	1788	rBV3	365	460	0.06%	0.008%
69	12.018	1788	1793	1803	rBV	370526	479696	57.83%	7.841%
70	12.140	1811	1813	1816	rBV3	506	582	0.07%	0.010%
71	12.226	1824	1827	1828	rVB	701	527	0.06%	0.009%
72	12.317	1837	1842	1853	rBV	449971	570199	68.74%	9.320%
73	12.463	1864	1866	1869	rVB3	559	526	0.06%	0.009%
74	12.494	1869	1871	1872	rBV	437	291	0.04%	0.005%
75	12.768	1910	1916	1921	rBV3	522	1155	0.14%	0.019%
76	12.847	1925	1929	1932	rBV	237	385	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043865.D
 Acq On : 15 Nov 2024 11:05
 Operator : JC/MD
 Sample : P4782-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E1H29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	13.000	1951	1954	1957	rBV2	430	426	0.05%	0.007%
78	13.103	1970	1971	1974	rBV2	316	301	0.04%	0.005%
79	13.225	1989	1991	1993	rBV2	405	492	0.06%	0.008%
80	13.292	2001	2002	2006	rVB2	363	343	0.04%	0.006%
81	13.353	2011	2012	2014	rBV2	373	265	0.03%	0.004%
82	13.390	2017	2018	2021	rVB	484	328	0.04%	0.005%
83	13.457	2027	2029	2032	rVB3	262	267	0.03%	0.004%
84	13.494	2032	2035	2036	rBV2	442	479	0.06%	0.008%
85	13.609	2052	2054	2056	rVB	429	319	0.04%	0.005%
86	13.725	2071	2073	2076	rVB	471	302	0.04%	0.005%
87	14.000	2115	2118	2119	rBV2	284	260	0.03%	0.004%
88	14.152	2141	2143	2146	rVB2	434	312	0.04%	0.005%
89	14.341	2172	2174	2177	rVB	314	239	0.03%	0.004%
90	14.396	2179	2183	2184	rBV3	246	341	0.04%	0.006%
91	14.567	2209	2211	2216	rVB2	575	581	0.07%	0.009%
92	14.670	2225	2228	2230	rBV4	475	449	0.05%	0.007%
93	14.798	2247	2249	2251	rBV3	265	219	0.03%	0.004%
94	14.817	2251	2252	2255	rVB3	562	447	0.05%	0.007%
95	14.938	2270	2272	2274	rBV	370	371	0.04%	0.006%
96	15.182	2310	2312	2314	rBV2	542	481	0.06%	0.008%
97	15.286	2326	2329	2333	rBV3	383	558	0.07%	0.009%
98	16.383	2507	2509	2510	rBV2	449	296	0.04%	0.005%
99	16.591	2541	2543	2544	rBV2	630	349	0.04%	0.006%
100	16.652	2551	2553	2554	rBV2	602	520	0.06%	0.008%

Sum of corrected areas: 6118052




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043865.D
Acq On : 15 Nov 2024 11:05
Operator : JC/MD
Sample : P4782-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

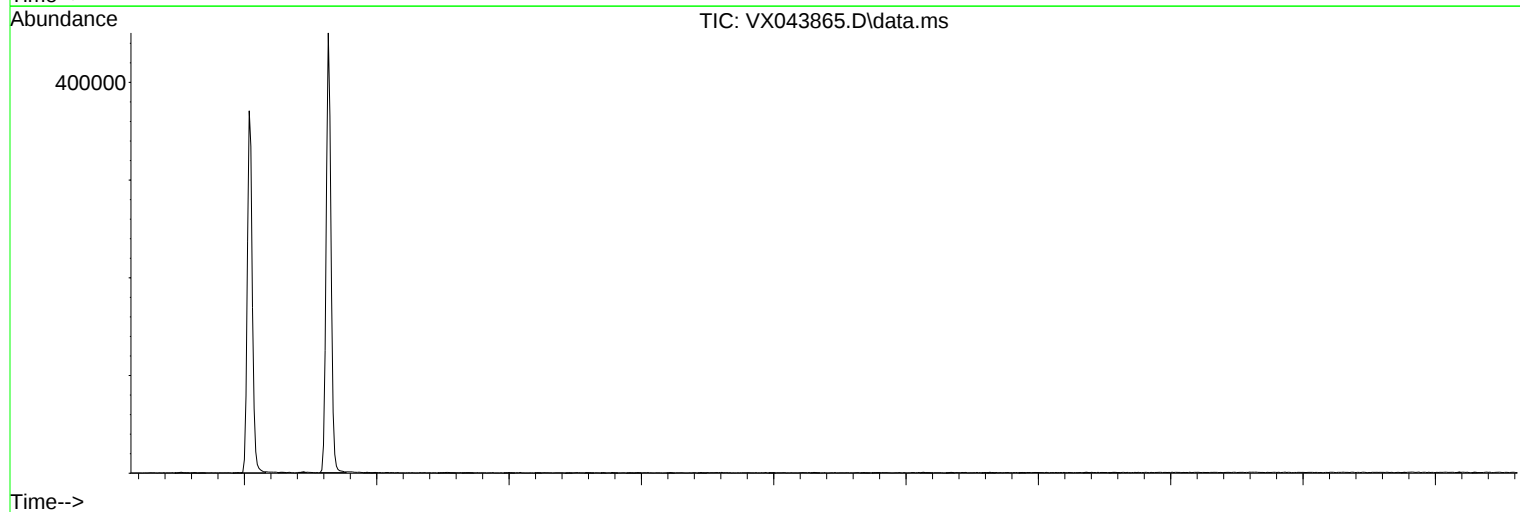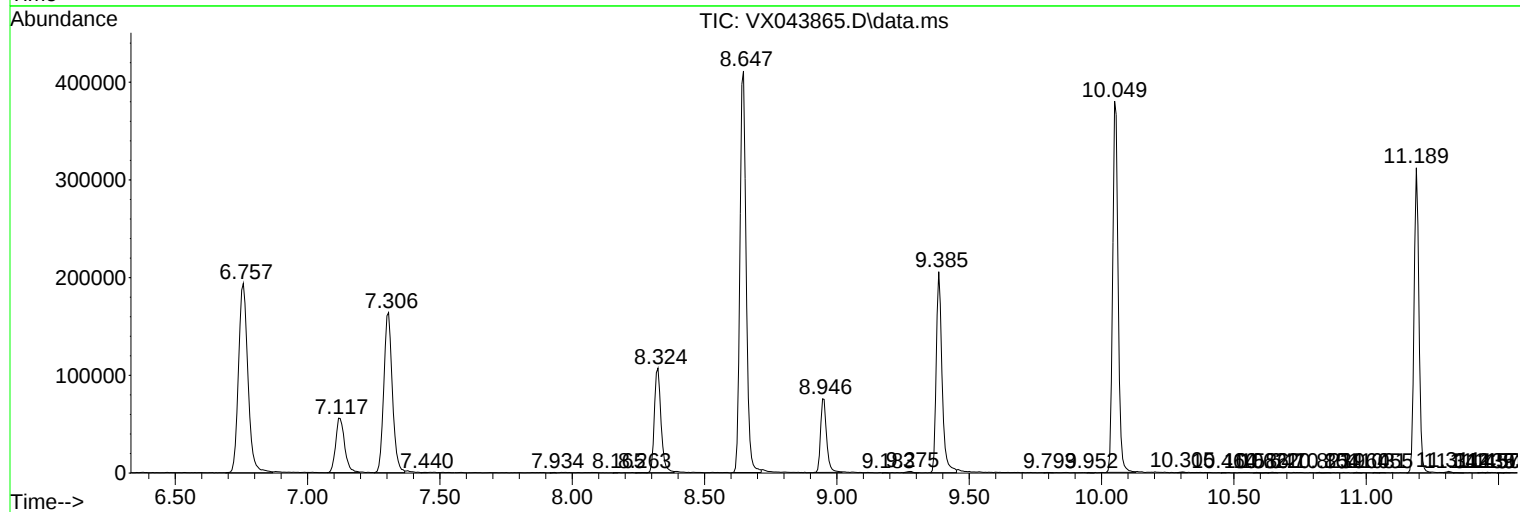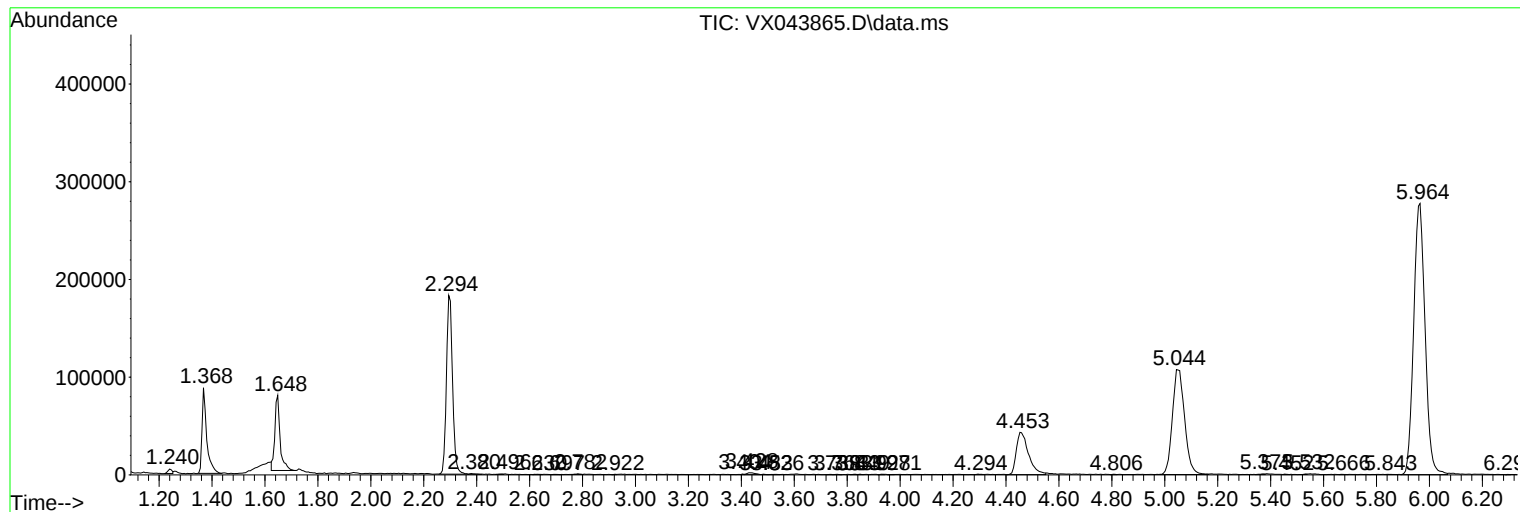

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043865.D
Acq On : 15 Nov 2024 11:05
Operator : JC/MD
Sample : P4782-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043865.D
Acq On : 15 Nov 2024 11:05
Operator : JC/MD
Sample : P4782-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E1H29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc
