

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043868.D
 Acq On : 15 Nov 2024 12:13
 Operator : JC/MD
 Sample : P4785-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043868.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	5799	8905	1.07%	0.142%
2	1.368	42	46	57	rVB	87678	106856	12.83%	1.704%
3	1.642	88	91	103	rVB	80754	106147	12.75%	1.692%
4	2.294	192	198	207	rBV	186740	291104	34.96%	4.641%
5	2.386	208	213	221	rVB	10472	18142	2.18%	0.289%
6	2.483	227	229	230	rBV2	417	428	0.05%	0.007%
7	2.569	237	243	244	rBV2	499	751	0.09%	0.012%
8	2.630	247	253	254	rBV2	383	512	0.06%	0.008%
9	2.697	260	264	272	rBV2	996	2150	0.26%	0.034%
10	2.776	275	277	283	rBV4	679	1286	0.15%	0.021%
11	2.940	297	304	308	rBV3	2433	4873	0.59%	0.078%
12	3.172	340	342	345	rBV2	343	367	0.04%	0.006%
13	3.325	364	367	371	rBV3	297	342	0.04%	0.005%
14	3.379	371	376	377	rVB3	277	405	0.05%	0.006%
15	3.440	377	386	391	rBV3	2120	4252	0.51%	0.068%
16	3.648	417	420	424	rBV2	445	642	0.08%	0.010%
17	3.739	433	435	437	rBV2	336	313	0.04%	0.005%
18	4.038	481	484	486	rBV	288	305	0.04%	0.005%
19	4.062	486	488	491	rVB2	398	362	0.04%	0.006%
20	4.093	491	493	496	rBV2	427	448	0.05%	0.007%
21	4.215	509	513	515	rBV2	236	398	0.05%	0.006%
22	4.239	515	517	521	rVB2	396	455	0.05%	0.007%
23	4.458	542	553	567	rBV	46906	142081	17.06%	2.265%
24	4.757	599	602	604	rBV2	345	365	0.04%	0.006%
25	5.050	637	650	668	rBV2	113352	350701	42.12%	5.591%
26	5.391	699	706	710	rBV3	543	1364	0.16%	0.022%
27	5.422	710	711	714	rVB2	500	319	0.04%	0.005%
28	5.477	718	720	722	rBV3	321	354	0.04%	0.006%
29	5.556	727	733	740	rVB4	1082	2637	0.32%	0.042%
30	5.702	753	757	759	rBV2	395	616	0.07%	0.010%
31	5.958	788	799	822	rBV3	274932	832610	100.00%	13.274%
32	6.245	844	846	850	rBV2	291	517	0.06%	0.008%
33	6.318	855	858	860	rVB3	302	384	0.05%	0.006%
34	6.336	860	861	864	rBV2	247	317	0.04%	0.005%
35	6.373	864	867	870	rVB3	501	742	0.09%	0.012%
36	6.428	873	876	878	rVB2	306	320	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043868.D
 Acq On : 15 Nov 2024 12:13
 Operator : JC/MD
 Sample : P4785-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	6.757	922	930	947	rVV	215188	520472	62.51%	8.298%
38	7.123	984	990	1001	rVV7	5987	15245	1.83%	0.243%
39	7.306	1010	1020	1042	rBV	159096	366173	43.98%	5.838%
40	7.458	1042	1045	1046	rBV2	460	307	0.04%	0.005%
41	7.476	1046	1048	1050	rBV2	361	448	0.05%	0.007%
42	7.684	1081	1082	1085	rBV3	338	386	0.05%	0.006%
43	7.854	1106	1110	1112	rBV3	682	934	0.11%	0.015%
44	7.909	1116	1119	1120	rBV	346	387	0.05%	0.006%
45	8.055	1142	1143	1148	rVB2	374	390	0.05%	0.006%
46	8.269	1176	1178	1180	rVB2	424	339	0.04%	0.005%
47	8.324	1180	1187	1206	rBV	107581	185062	22.23%	2.950%
48	8.647	1233	1240	1256	rBV	427420	683634	82.11%	10.899%
49	8.903	1279	1282	1284	rBV2	322	470	0.06%	0.007%
50	8.945	1284	1289	1302	rBV	75872	119304	14.33%	1.902%
51	9.110	1315	1316	1322	rVB2	488	469	0.06%	0.007%
52	9.220	1330	1334	1337	rBV2	308	571	0.07%	0.009%
53	9.269	1339	1342	1346	rVB3	1084	1564	0.19%	0.025%
54	9.384	1356	1361	1381	rBV	215291	330354	39.68%	5.267%
55	9.598	1392	1396	1401	rVB5	1208	2304	0.28%	0.037%
56	9.701	1412	1413	1417	rVB	468	351	0.04%	0.006%
57	9.823	1428	1433	1435	rVB2	258	348	0.04%	0.006%
58	10.049	1465	1470	1486	rBV	419697	598874	71.93%	9.548%
59	10.701	1576	1577	1580	rVB	422	316	0.04%	0.005%
60	10.738	1580	1583	1585	rBV	360	411	0.05%	0.007%
61	11.006	1626	1627	1630	rBV2	306	314	0.04%	0.005%
62	11.030	1630	1631	1634	rVV2	408	357	0.04%	0.006%
63	11.128	1645	1647	1650	rBV2	239	306	0.04%	0.005%
64	11.189	1652	1657	1666	rBV	309683	396723	47.65%	6.325%
65	11.311	1674	1677	1681	rVV3	1287	1450	0.17%	0.023%
66	11.573	1716	1720	1724	rBV4	739	1254	0.15%	0.020%
67	11.689	1738	1739	1741	rBV	523	315	0.04%	0.005%
68	11.756	1747	1750	1752	rVB	505	408	0.05%	0.007%
69	11.799	1752	1757	1758	rBV2	478	644	0.08%	0.010%
70	11.829	1759	1762	1767	rVB3	1100	1131	0.14%	0.018%
71	11.896	1769	1773	1779	rBV6	2037	4168	0.50%	0.066%
72	12.018	1788	1793	1804	rBV	410603	527005	63.30%	8.402%
73	12.219	1821	1826	1832	rBV2	12564	20947	2.52%	0.334%
74	12.317	1837	1842	1851	rVB	460555	587361	70.54%	9.364%
75	12.475	1864	1868	1873	rVB6	1260	1990	0.24%	0.032%
76	12.536	1877	1878	1881	rVB	483	477	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043868.D
 Acq On : 15 Nov 2024 12:13
 Operator : JC/MD
 Sample : P4785-12
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27L9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.762	1913	1915	1917	rBV3	611	648	0.08%	0.010%
78	12.859	1925	1931	1939	rVB7	2012	3963	0.48%	0.063%
79	13.067	1962	1965	1968	rBV2	319	415	0.05%	0.007%
80	13.122	1968	1974	1975	rBV4	395	710	0.09%	0.011%
81	13.170	1980	1982	1986	rVB	425	335	0.04%	0.005%
82	13.274	1997	1999	2003	rVB2	348	323	0.04%	0.005%
83	13.725	2071	2073	2074	rBV	501	371	0.04%	0.006%
84	13.792	2078	2084	2087	rVV3	626	1185	0.14%	0.019%
85	13.823	2087	2089	2092	rVV2	350	428	0.05%	0.007%
86	13.853	2092	2094	2096	rVV2	346	373	0.04%	0.006%
87	13.902	2100	2102	2104	rVV2	406	413	0.05%	0.007%
88	13.975	2113	2114	2117	rVB3	583	391	0.05%	0.006%
89	14.225	2153	2155	2157	rBV	411	375	0.05%	0.006%
90	14.292	2164	2166	2169	rBV2	498	508	0.06%	0.008%
91	14.396	2179	2183	2185	rVB3	267	318	0.04%	0.005%
92	14.670	2224	2228	2229	rBV	367	382	0.05%	0.006%
93	14.688	2229	2231	2233	rBV2	466	380	0.05%	0.006%
94	14.853	2256	2258	2260	rVB2	460	331	0.04%	0.005%
95	15.335	2335	2337	2338	rBV2	526	343	0.04%	0.005%
96	15.597	2378	2380	2382	rBV2	493	451	0.05%	0.007%
97	15.682	2392	2394	2397	rBV2	479	349	0.04%	0.006%
98	15.944	2434	2437	2441	rBV2	822	1184	0.14%	0.019%
99	16.280	2488	2492	2494	rBV4	751	864	0.10%	0.014%
100	16.408	2511	2513	2516	rBV2	612	530	0.06%	0.008%

Sum of corrected areas: 6272303




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043868.D
Acq On : 15 Nov 2024 12:13
Operator : JC/MD
Sample : P4785-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

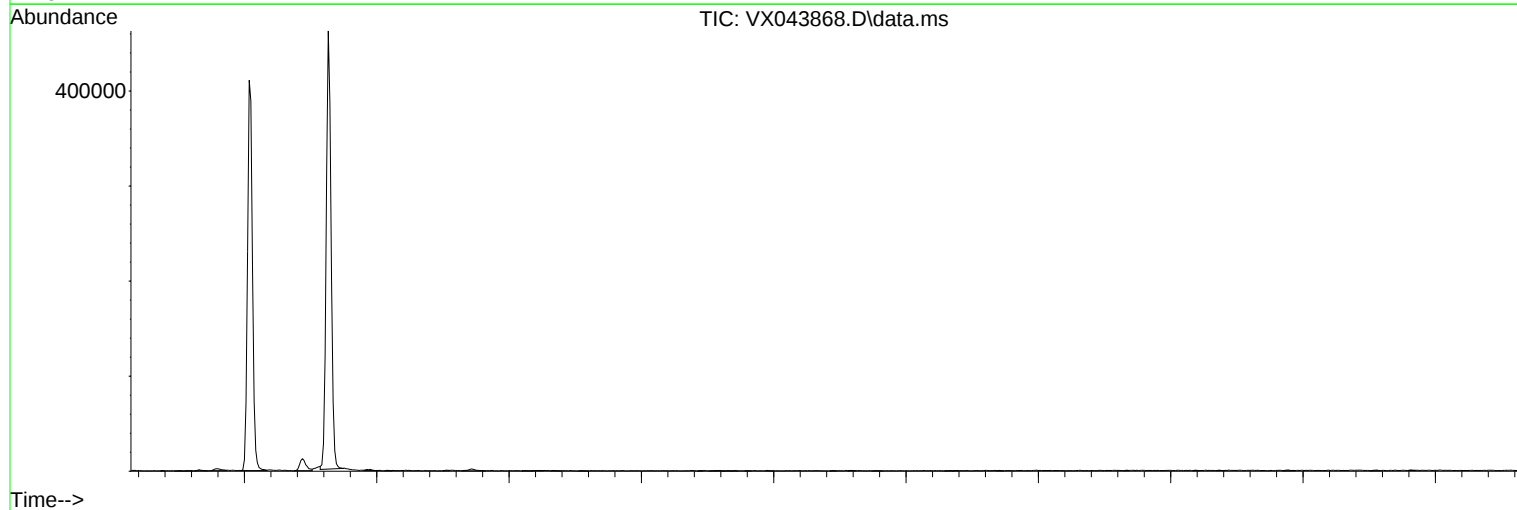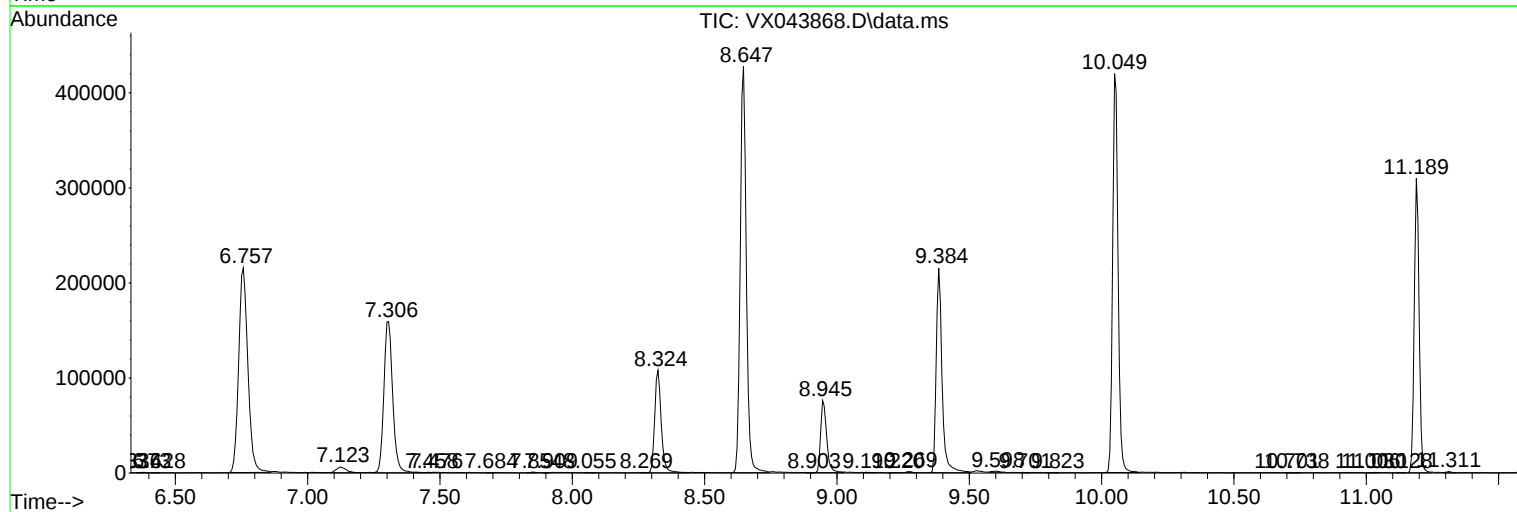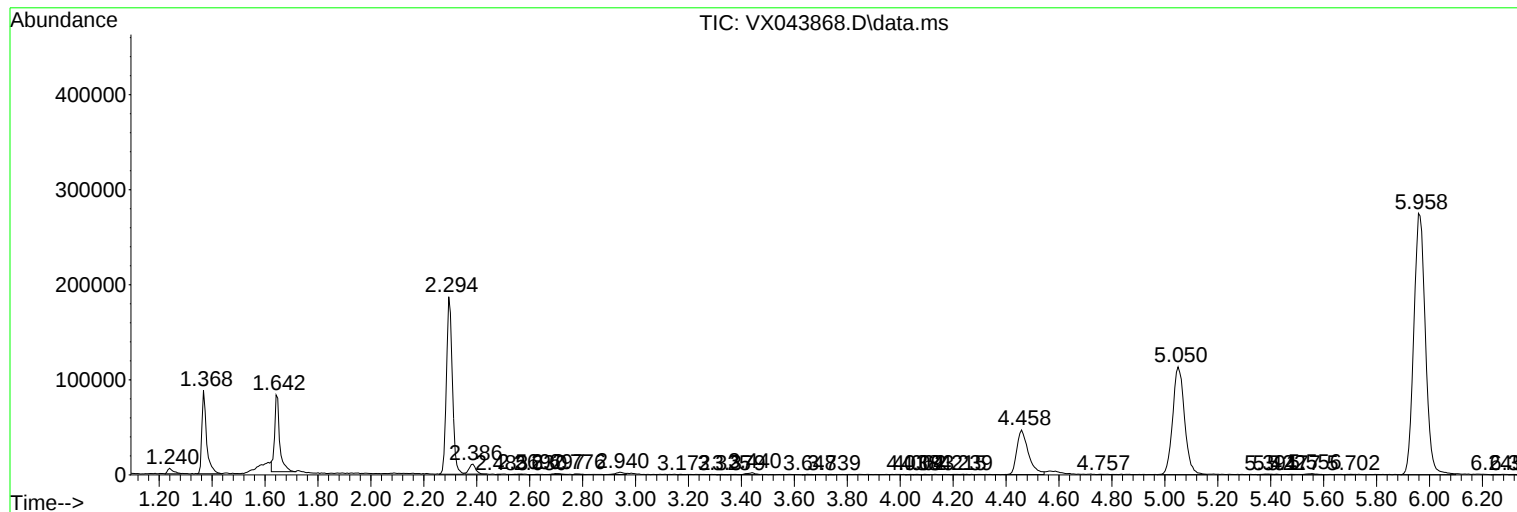

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043868.D
Acq On : 15 Nov 2024 12:13
Operator : JC/MD
Sample : P4785-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043868.D
Acq On : 15 Nov 2024 12:13
Operator : JC/MD
Sample : P4785-12
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27L9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
