

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043869.D
 Acq On : 15 Nov 2024 12:36
 Operator : JC/MD
 Sample : P4785-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	35	rVB2	6395	8599	1.03%	0.143%
2	1.368	42	46	58	rBV	95043	109071	13.00%	1.811%
3	1.642	88	91	102	rVB	76814	103902	12.39%	1.725%
4	2.294	192	198	209	rBV	184987	297623	35.48%	4.942%
5	2.502	228	232	236	rVB3	682	770	0.09%	0.013%
6	2.538	236	238	239	rBV2	472	431	0.05%	0.007%
7	2.782	276	278	279	rBV	426	283	0.03%	0.005%
8	2.941	297	304	309	rBV3	2966	6982	0.83%	0.116%
9	3.190	344	345	348	rBV2	296	271	0.03%	0.005%
10	3.440	380	386	391	rVV5	1957	3891	0.46%	0.065%
11	3.696	425	428	430	rBV	507	389	0.05%	0.006%
12	3.745	433	436	440	rBV2	304	530	0.06%	0.009%
13	3.971	469	473	475	rVV2	209	252	0.03%	0.004%
14	3.989	475	476	479	rVB2	466	376	0.04%	0.006%
15	4.026	479	482	483	rBV2	220	257	0.03%	0.004%
16	4.044	483	485	487	rVV2	321	242	0.03%	0.004%
17	4.087	490	492	496	rVB2	352	453	0.05%	0.008%
18	4.123	496	498	500	rBV2	276	318	0.04%	0.005%
19	4.391	540	542	544	rBV	378	297	0.04%	0.005%
20	4.459	544	553	570	rBV2	44611	137912	16.44%	2.290%
21	5.050	639	650	664	rBV	112452	347558	41.43%	5.771%
22	5.367	700	702	703	rBV	385	382	0.05%	0.006%
23	5.458	715	717	719	rBV	458	296	0.04%	0.005%
24	5.544	727	731	733	rBV2	898	1118	0.13%	0.019%
25	5.653	747	749	753	rBV2	349	418	0.05%	0.007%
26	5.842	778	780	783	rBV2	312	348	0.04%	0.006%
27	5.964	789	800	815	rBV2	278142	838837	100.00%	13.929%
28	6.294	851	854	856	rVB2	308	304	0.04%	0.005%
29	6.544	894	895	898	rBV2	191	234	0.03%	0.004%
30	6.623	906	908	910	rBV	391	338	0.04%	0.006%
31	6.757	921	930	946	rBV	194096	470727	56.12%	7.817%
32	7.007	969	971	976	rVB3	374	477	0.06%	0.008%
33	7.050	976	978	980	rBV	293	296	0.04%	0.005%
34	7.129	984	991	997	rBV8	6981	15457	1.84%	0.257%
35	7.214	1004	1005	1007	rVB2	480	257	0.03%	0.004%
36	7.306	1011	1020	1032	rBV	166837	370596	44.18%	6.154%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043869.D
 Acq On : 15 Nov 2024 12:36
 Operator : JC/MD
 Sample : P4785-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	7.769	1094	1096	1097	rVB	385	244	0.03%	0.004%
38	7.964	1124	1128	1129	rBV2	413	470	0.06%	0.008%
39	8.049	1140	1142	1143	rBV2	312	235	0.03%	0.004%
40	8.110	1149	1152	1154	rBV2	273	369	0.04%	0.006%
41	8.183	1162	1164	1167	rBV2	227	267	0.03%	0.004%
42	8.269	1174	1178	1181	rBV2	269	473	0.06%	0.008%
43	8.324	1181	1187	1197	rBV	108687	184651	22.01%	3.066%
44	8.464	1209	1210	1212	rVB2	566	262	0.03%	0.004%
45	8.519	1217	1219	1221	rBV	333	245	0.03%	0.004%
46	8.561	1225	1226	1228	rVB	449	232	0.03%	0.004%
47	8.586	1228	1230	1232	rBV	368	347	0.04%	0.006%
48	8.647	1233	1240	1258	rBV	437218	691954	82.49%	11.490%
49	8.866	1272	1276	1278	rBV2	397	434	0.05%	0.007%
50	8.952	1284	1290	1300	rBV	74475	120036	14.31%	1.993%
51	9.104	1312	1315	1316	rBV2	284	285	0.03%	0.005%
52	9.269	1339	1342	1345	rBV3	1045	1408	0.17%	0.023%
53	9.384	1356	1361	1379	rBV	208976	317963	37.91%	5.280%
54	9.836	1433	1435	1437	rVB	375	269	0.03%	0.004%
55	9.945	1449	1453	1455	rBV2	274	384	0.05%	0.006%
56	10.055	1465	1471	1490	rBV	365301	539328	64.29%	8.956%
57	10.396	1525	1527	1529	rVV2	220	253	0.03%	0.004%
58	10.738	1580	1583	1585	rBV	264	239	0.03%	0.004%
59	10.811	1591	1595	1597	rBV2	246	350	0.04%	0.006%
60	10.902	1609	1610	1614	rBV	252	259	0.03%	0.004%
61	10.939	1614	1616	1619	rBV3	273	253	0.03%	0.004%
62	11.189	1652	1657	1664	rBV	313469	388492	46.31%	6.451%
63	11.311	1672	1677	1684	rBV4	1077	1929	0.23%	0.032%
64	11.482	1703	1705	1706	rVB	431	288	0.03%	0.005%
65	11.500	1706	1708	1709	rBV	386	330	0.04%	0.005%
66	11.591	1719	1723	1726	rVB2	356	491	0.06%	0.008%
67	11.640	1727	1731	1732	rBV2	332	292	0.03%	0.005%
68	11.658	1732	1734	1735	rBV2	316	232	0.03%	0.004%
69	11.756	1748	1750	1752	rBV2	390	334	0.04%	0.006%
70	11.829	1759	1762	1767	rVB	493	603	0.07%	0.010%
71	11.915	1772	1776	1777	rBV	313	350	0.04%	0.006%
72	12.018	1788	1793	1803	rBV	358266	461524	55.02%	7.664%
73	12.317	1837	1842	1854	rVV	445935	574659	68.51%	9.542%
74	12.506	1869	1873	1875	rVB3	420	525	0.06%	0.009%
75	12.573	1882	1884	1885	rBV	358	344	0.04%	0.006%
76	12.622	1890	1892	1896	rVB2	417	400	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043869.D
 Acq On : 15 Nov 2024 12:36
 Operator : JC/MD
 Sample : P4785-19
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.658	1896	1898	1901	rBV2	257	267	0.03%	0.004%
78	12.762	1912	1915	1922	rBV4	461	929	0.11%	0.015%
79	13.195	1984	1986	1988	rVB2	379	326	0.04%	0.005%
80	13.219	1988	1990	1991	rBV	486	320	0.04%	0.005%
81	13.311	2001	2005	2006	rVB2	275	267	0.03%	0.004%
82	13.396	2017	2019	2025	rVB2	272	522	0.06%	0.009%
83	13.445	2025	2027	2029	rBV2	329	317	0.04%	0.005%
84	13.743	2074	2076	2078	rVB2	405	356	0.04%	0.006%
85	13.792	2083	2084	2089	rBV3	261	314	0.04%	0.005%
86	14.079	2129	2131	2134	rBV	354	244	0.03%	0.004%
87	14.225	2154	2155	2157	rVV2	309	233	0.03%	0.004%
88	14.262	2160	2161	2165	rVB2	388	353	0.04%	0.006%
89	14.298	2165	2167	2169	rBV	270	249	0.03%	0.004%
90	14.518	2201	2203	2207	rBV	263	327	0.04%	0.005%
91	14.560	2209	2210	2214	rBV3	357	461	0.05%	0.008%
92	14.591	2214	2215	2217	rVB	528	283	0.03%	0.005%
93	14.621	2217	2220	2225	rBV3	570	1087	0.13%	0.018%
94	15.030	2285	2287	2289	rBV	272	227	0.03%	0.004%
95	15.243	2321	2322	2325	rBV3	437	375	0.04%	0.006%
96	15.310	2332	2333	2334	rBV	432	263	0.03%	0.004%
97	16.310	2495	2497	2500	rBV2	784	720	0.09%	0.012%
98	16.408	2512	2513	2515	rBV	609	371	0.04%	0.006%
99	16.462	2520	2522	2523	rBV	497	304	0.04%	0.005%
100	16.560	2537	2538	2542	rBV2	586	605	0.07%	0.010%

Sum of corrected areas: 6022215




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043869.D
Acq On : 15 Nov 2024 12:36
Operator : JC/MD
Sample : P4785-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

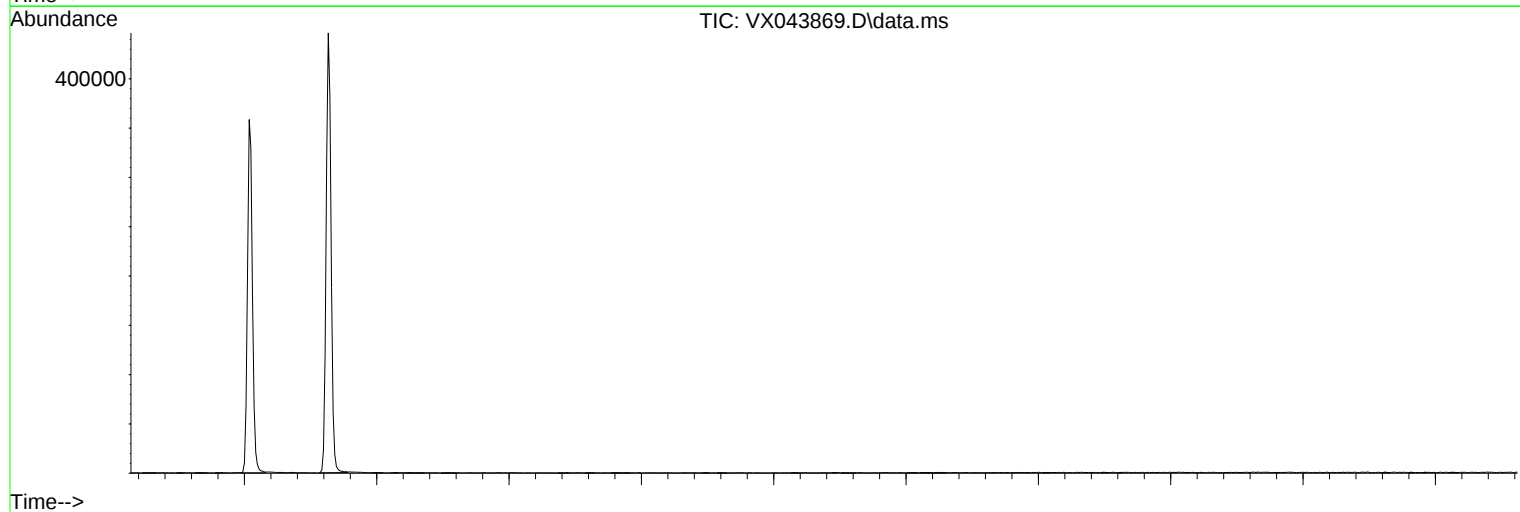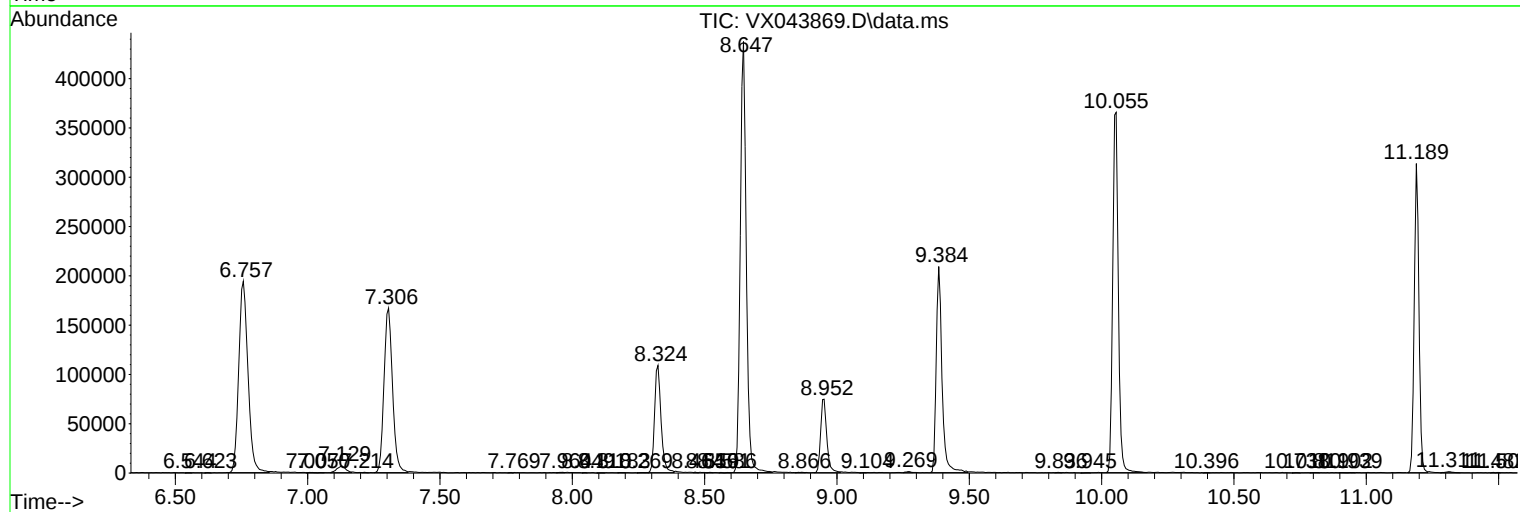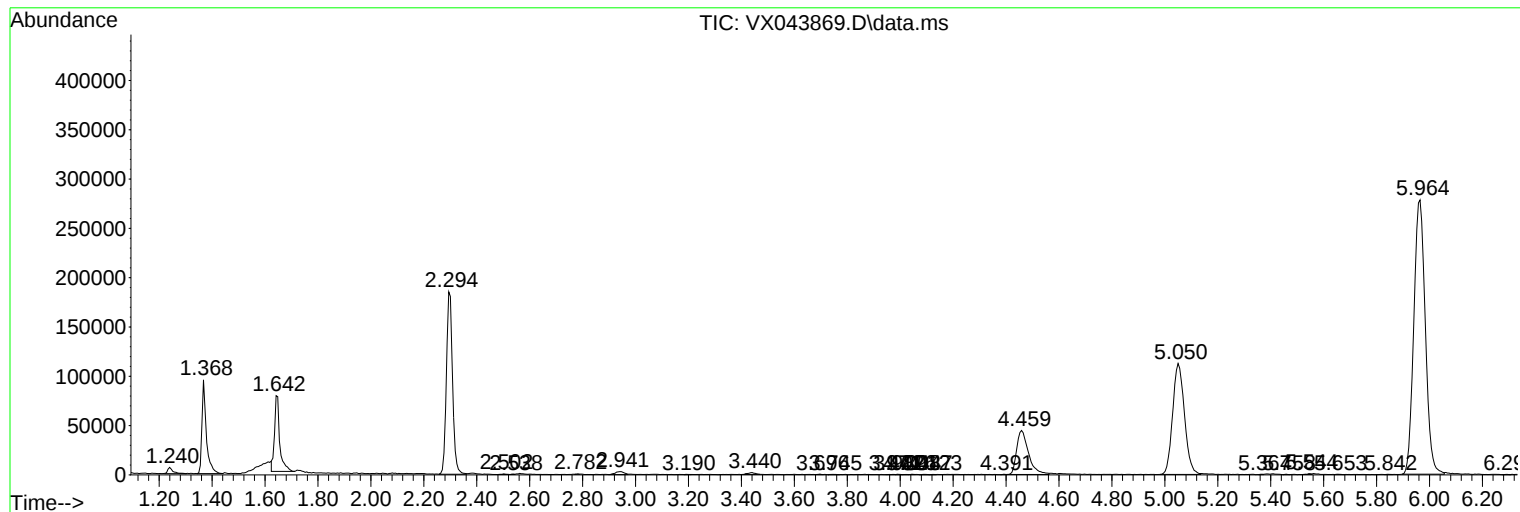

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043869.D
Acq On : 15 Nov 2024 12:36
Operator : JC/MD
Sample : P4785-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043869.D
Acq On : 15 Nov 2024 12:36
Operator : JC/MD
Sample : P4785-19
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc