

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043870.D
 Acq On : 15 Nov 2024 13:00
 Operator : JC/MD
 Sample : P4724-16ME
 Misc : 5.79g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9G6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043870.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	37	rBV2	5195	11880	0.96%	0.148%
2	1.368	42	46	49	rBV	64276	80906	6.57%	1.009%
3	1.648	89	92	94	rBV	28791	36525	2.96%	0.455%
4	2.276	189	195	208	rBV	234440	394767	32.03%	4.923%
5	2.477	226	228	231	rBV3	294	349	0.03%	0.004%
6	2.776	272	277	284	rBV4	1455	3346	0.27%	0.042%
7	2.904	296	298	299	rBV	253	207	0.02%	0.003%
8	2.995	311	313	314	rBV2	363	346	0.03%	0.004%
9	3.038	319	320	323	rVB2	361	253	0.02%	0.003%
10	3.075	323	326	328	rBV2	299	345	0.03%	0.004%
11	3.203	344	347	352	rBV3	374	740	0.06%	0.009%
12	3.245	352	354	358	rVB2	281	284	0.02%	0.004%
13	3.416	377	382	389	rBV2	1928	3805	0.31%	0.047%
14	3.581	407	409	412	rVV	252	266	0.02%	0.003%
15	3.770	438	440	444	rVB2	358	332	0.03%	0.004%
16	3.837	449	451	454	rVB	331	288	0.02%	0.004%
17	3.867	454	456	460	rBV2	233	323	0.03%	0.004%
18	3.910	460	463	464	rBV	290	312	0.03%	0.004%
19	4.172	504	506	511	rVB	429	468	0.04%	0.006%
20	4.483	548	557	575	rBV	48402	189462	15.37%	2.363%
21	4.934	629	631	633	rBV2	267	224	0.02%	0.003%
22	5.056	638	651	668	rVV	159929	499434	40.53%	6.228%
23	5.489	720	722	724	rBV	300	326	0.03%	0.004%
24	5.696	754	756	757	rBV2	438	293	0.02%	0.004%
25	5.781	769	770	773	rBV	395	373	0.03%	0.005%
26	5.830	776	778	785	rVB2	234	195	0.02%	0.002%
27	5.958	787	799	827	rBV2	424484	1232310	100.00%	15.366%
28	6.367	862	866	868	rBV4	1226	1866	0.15%	0.023%
29	6.757	920	930	949	rBV	186174	461817	37.48%	5.759%
30	7.019	971	973	976	rBV	512	541	0.04%	0.007%
31	7.129	982	991	998	rVB7	6097	17277	1.40%	0.215%
32	7.208	998	1004	1005	rBV3	1494	2164	0.18%	0.027%
33	7.306	1010	1020	1041	rVB	236504	544641	44.20%	6.791%
34	7.470	1045	1047	1049	rBV	375	336	0.03%	0.004%
35	7.488	1049	1050	1052	rVB2	635	349	0.03%	0.004%
36	7.598	1066	1068	1069	rBV2	253	250	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043870.D
 Acq On : 15 Nov 2024 13:00
 Operator : JC/MD
 Sample : P4724-16ME
 Misc : 5.79g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9G6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	7.708	1085	1086	1088	rVB	342	236	0.02%	0.003%
38	7.732	1088	1090	1092	rBV2	317	268	0.02%	0.003%
39	7.818	1102	1104	1107	rBV2	263	204	0.02%	0.003%
40	7.958	1123	1127	1136	rBV5	1397	2625	0.21%	0.033%
41	8.019	1136	1137	1139	rVB	472	256	0.02%	0.003%
42	8.037	1139	1140	1142	rBV	323	225	0.02%	0.003%
43	8.324	1181	1187	1199	rBV	163773	274127	22.24%	3.418%
44	8.531	1220	1221	1226	rVB2	593	465	0.04%	0.006%
45	8.647	1233	1240	1255	rBV	620974	1035004	83.99%	12.906%
46	8.952	1284	1290	1302	rBV	109378	179042	14.53%	2.233%
47	9.269	1340	1342	1343	rBV	570	436	0.04%	0.005%
48	9.391	1356	1362	1380	rBV	243390	467136	37.91%	5.825%
49	9.586	1392	1394	1400	rVB4	468	688	0.06%	0.009%
50	9.836	1432	1435	1441	rBV2	467	815	0.07%	0.010%
51	9.884	1441	1443	1444	rBV2	285	235	0.02%	0.003%
52	9.958	1453	1455	1457	rVB2	422	344	0.03%	0.004%
53	10.000	1460	1462	1464	rBV	301	186	0.02%	0.002%
54	10.049	1465	1470	1485	rVV	365764	539824	43.81%	6.731%
55	10.256	1501	1504	1506	rBV2	273	348	0.03%	0.004%
56	10.299	1510	1511	1515	rVB2	527	417	0.03%	0.005%
57	10.476	1538	1540	1542	rBV2	302	258	0.02%	0.003%
58	10.774	1587	1589	1592	rVB2	262	183	0.01%	0.002%
59	10.835	1596	1599	1601	rBV2	209	267	0.02%	0.003%
60	10.866	1601	1604	1606	rBV	235	270	0.02%	0.003%
61	10.939	1614	1616	1619	rBV3	304	308	0.02%	0.004%
62	10.970	1619	1621	1623	rVV2	323	279	0.02%	0.003%
63	11.006	1626	1627	1629	rVB2	376	204	0.02%	0.003%
64	11.116	1644	1645	1650	rBV3	315	499	0.04%	0.006%
65	11.189	1652	1657	1669	rVV	439791	589430	47.83%	7.350%
66	11.287	1671	1673	1676	rVV3	384	397	0.03%	0.005%
67	11.311	1676	1677	1682	rVB	533	541	0.04%	0.007%
68	11.348	1682	1683	1687	rBV2	190	184	0.01%	0.002%
69	11.476	1700	1704	1707	rBV2	702	855	0.07%	0.011%
70	11.634	1728	1730	1732	rVB2	254	224	0.02%	0.003%
71	11.658	1732	1734	1737	rBV	330	331	0.03%	0.004%
72	11.707	1740	1742	1744	rVB2	440	376	0.03%	0.005%
73	11.768	1751	1752	1757	rBV2	342	290	0.02%	0.004%
74	11.811	1757	1759	1762	rVV	307	246	0.02%	0.003%
75	12.018	1788	1793	1804	rVV	375033	499725	40.55%	6.231%
76	12.238	1827	1829	1831	rBV	223	219	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043870.D
 Acq On : 15 Nov 2024 13:00
 Operator : JC/MD
 Sample : P4724-16ME
 Misc : 5.79g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9G6ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.317	1837	1842	1855	rBV	716696	927350	75.25%	11.564%
78	12.762	1913	1915	1916	rBV	324	248	0.02%	0.003%
79	12.841	1926	1928	1932	rVB2	287	258	0.02%	0.003%
80	12.920	1940	1941	1943	rVB	398	201	0.02%	0.003%
81	13.012	1952	1956	1957	rBV2	303	270	0.02%	0.003%
82	13.091	1967	1969	1971	rBV2	284	266	0.02%	0.003%
83	13.359	2010	2013	2014	rBV2	418	358	0.03%	0.004%
84	13.378	2014	2016	2017	rBV	238	191	0.02%	0.002%
85	13.420	2021	2023	2027	rVB2	375	442	0.04%	0.006%
86	13.530	2040	2041	2044	rVB2	318	241	0.02%	0.003%
87	13.573	2045	2048	2050	rVV	325	314	0.03%	0.004%
88	13.609	2052	2054	2055	rVV	477	273	0.02%	0.003%
89	13.725	2071	2073	2075	rBV	227	217	0.02%	0.003%
90	13.853	2092	2094	2095	rVV	313	183	0.01%	0.002%
91	13.871	2095	2097	2102	rVB2	387	439	0.04%	0.005%
92	13.914	2102	2104	2108	rBV2	361	509	0.04%	0.006%
93	14.134	2138	2140	2142	rBV2	419	232	0.02%	0.003%
94	14.548	2207	2208	2210	rVB	280	203	0.02%	0.003%
95	14.603	2215	2217	2219	rBV3	280	189	0.02%	0.002%
96	14.676	2228	2229	2232	rBV2	215	284	0.02%	0.004%
97	14.853	2255	2258	2259	rBV2	382	360	0.03%	0.004%
98	15.140	2302	2305	2306	rBV	368	319	0.03%	0.004%
99	15.591	2377	2379	2380	rBV	333	251	0.02%	0.003%
100	16.286	2491	2493	2494	rBV	416	295	0.02%	0.004%

Sum of corrected areas: 8019460




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043870.D
Acq On : 15 Nov 2024 13:00
Operator : JC/MD
Sample : P4724-16ME
Misc : 5.79g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9G6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

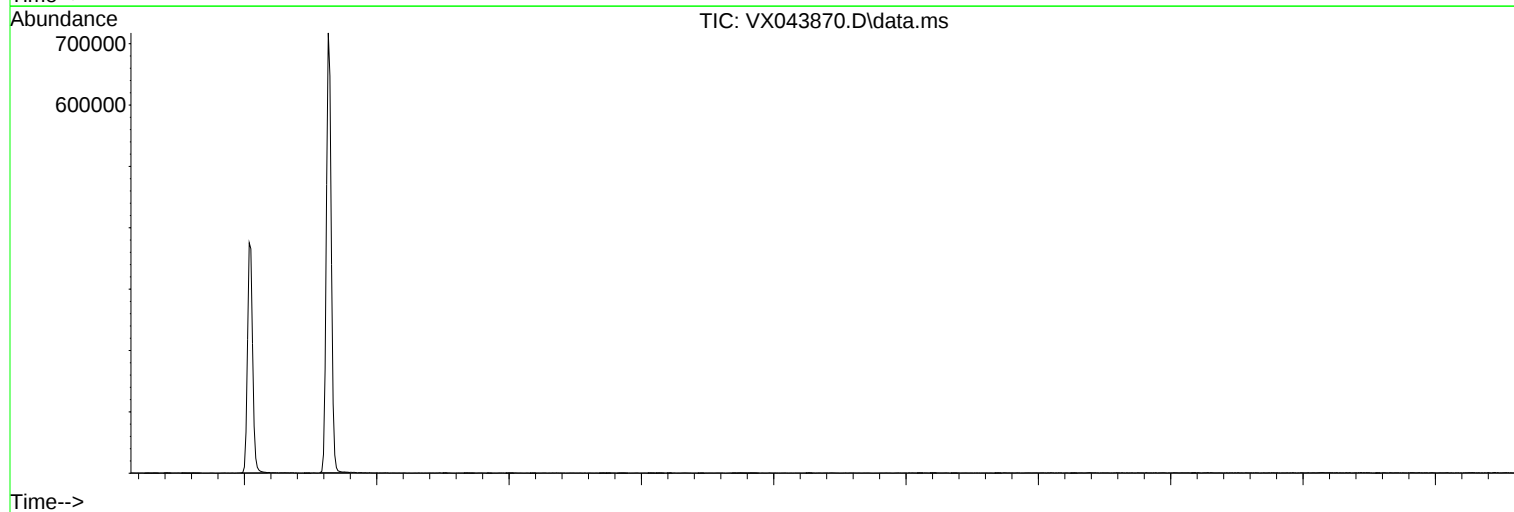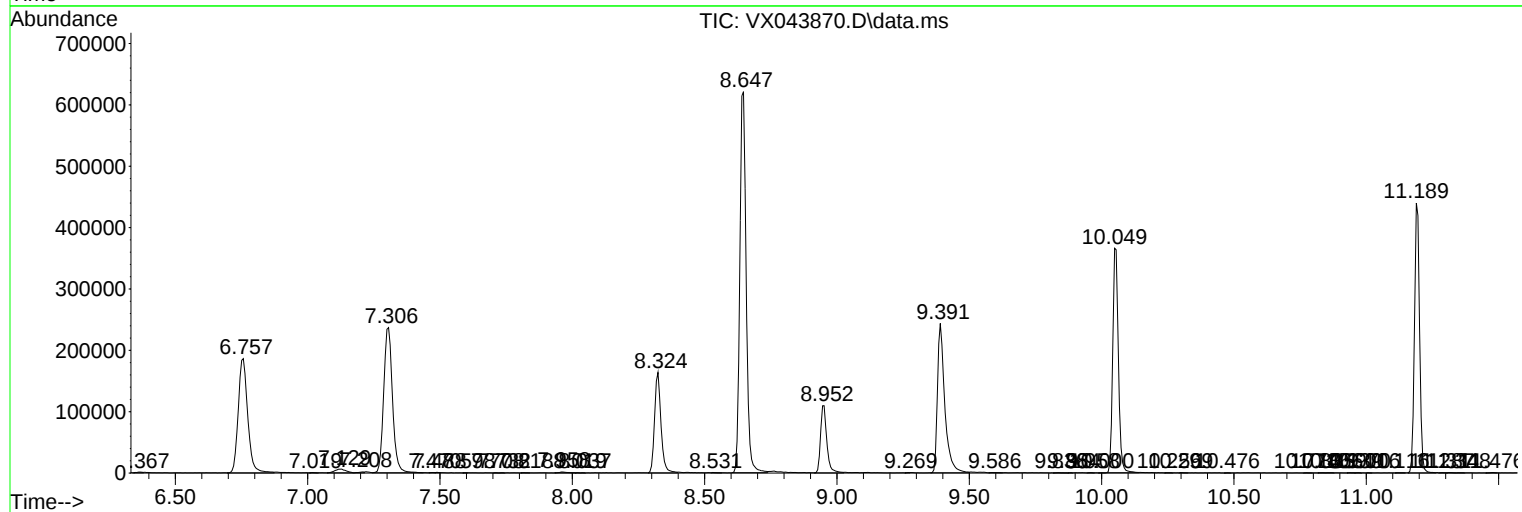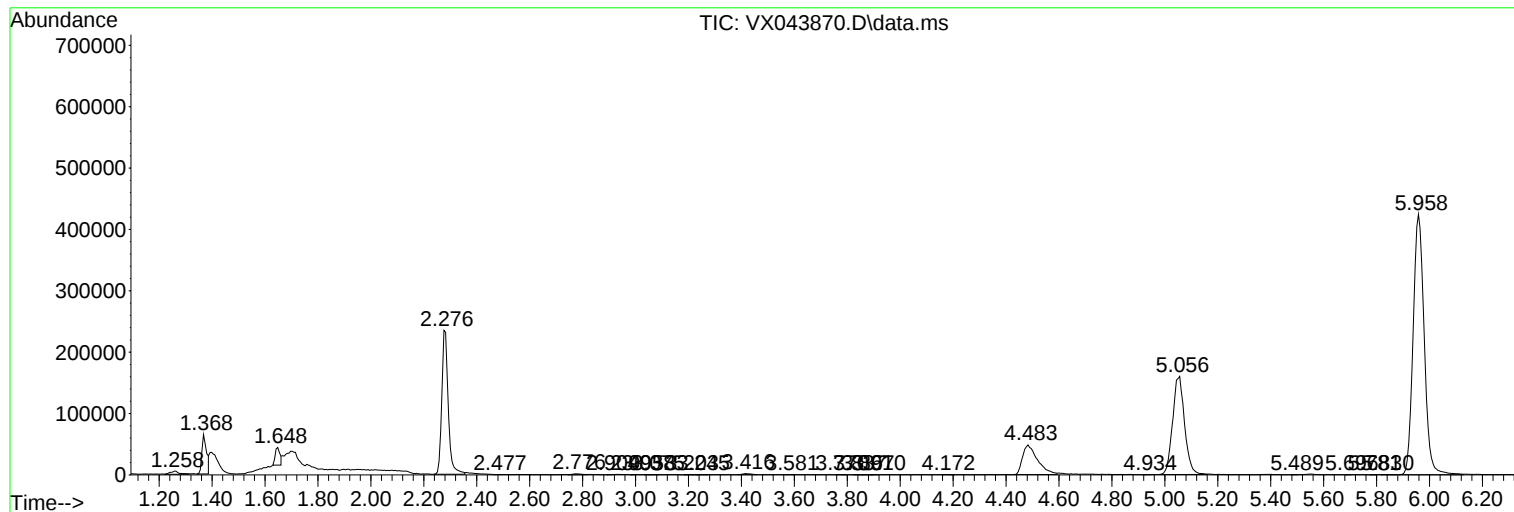

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043870.D
Acq On : 15 Nov 2024 13:00
Operator : JC/MD
Sample : P4724-16ME
Misc : 5.79g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9G6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043870.D
Acq On : 15 Nov 2024 13:00
Operator : JC/MD
Sample : P4724-16ME
Misc : 5.79g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9G6ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
