

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043872.D
 Acq On : 15 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4724-24ME
 Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043872.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.258	22	28	33	rBV2	6115	11322	1.45%	0.199%
2	1.368	43	46	48	rBV	36946	41043	5.25%	0.722%
3	2.276	189	195	207	rBV	151243	247941	31.73%	4.362%
4	2.581	243	245	246	rBV	348	263	0.03%	0.005%
5	2.654	256	257	259	rBV	391	311	0.04%	0.005%
6	2.709	264	266	267	rBV	389	248	0.03%	0.004%
7	2.776	274	277	283	rVB5	1157	1950	0.25%	0.034%
8	3.361	371	373	374	rBV	355	292	0.04%	0.005%
9	3.373	374	375	377	rVV2	484	315	0.04%	0.006%
10	3.416	377	382	388	rVB4	1809	3849	0.49%	0.068%
11	3.556	403	405	409	rBV2	266	327	0.04%	0.006%
12	3.636	414	418	419	rBV3	171	251	0.03%	0.004%
13	3.709	429	430	433	rBV	231	224	0.03%	0.004%
14	3.788	440	443	445	rBV	392	394	0.05%	0.007%
15	3.940	466	468	475	rBV2	270	429	0.05%	0.008%
16	4.123	494	498	500	rBV2	235	352	0.05%	0.006%
17	4.215	511	513	517	rVV2	317	356	0.05%	0.006%
18	4.489	549	558	575	rVV2	28825	116759	14.94%	2.054%
19	5.050	639	650	668	rVV2	104439	319831	40.93%	5.627%
20	5.227	678	679	683	rBV2	434	612	0.08%	0.011%
21	5.367	698	702	703	rBV2	379	450	0.06%	0.008%
22	5.538	726	730	731	rBV2	576	803	0.10%	0.014%
23	5.611	740	742	746	rVB2	509	534	0.07%	0.009%
24	5.672	748	752	757	rBV2	258	577	0.07%	0.010%
25	5.763	766	767	769	rBV	342	306	0.04%	0.005%
26	5.958	788	799	820	rBV3	273115	781376	100.00%	13.747%
27	6.190	835	837	839	rBV2	290	367	0.05%	0.006%
28	6.361	863	865	866	rBV	672	507	0.06%	0.009%
29	6.586	900	902	904	rBV2	402	232	0.03%	0.004%
30	6.757	921	930	944	rBV	192076	482317	61.73%	8.486%
31	7.123	983	990	999	rVV9	5483	15659	2.00%	0.276%
32	7.214	1001	1005	1011	rVV4	1969	4457	0.57%	0.078%
33	7.306	1011	1020	1036	rVB	152026	345561	44.22%	6.080%
34	7.775	1095	1097	1100	rVB	250	259	0.03%	0.005%
35	7.842	1104	1108	1111	rBV2	345	512	0.07%	0.009%
36	7.885	1111	1115	1117	rBV	298	386	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043872.D
 Acq On : 15 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4724-24ME
 Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	7.970	1123	1129	1132	rBV3	1099	1625	0.21%	0.029%
38	8.074	1144	1146	1147	rBV	343	337	0.04%	0.006%
39	8.123	1153	1154	1157	rBV2	252	346	0.04%	0.006%
40	8.324	1180	1187	1199	rBV	96601	166539	21.31%	2.930%
41	8.531	1219	1221	1225	rVB3	602	524	0.07%	0.009%
42	8.647	1233	1240	1254	rBV	395465	661628	84.67%	11.641%
43	8.952	1284	1290	1304	rBV	67590	110643	14.16%	1.947%
44	9.214	1331	1333	1339	rVB3	307	454	0.06%	0.008%
45	9.257	1339	1340	1342	rBV2	308	256	0.03%	0.005%
46	9.275	1342	1343	1346	rVB	546	330	0.04%	0.006%
47	9.318	1348	1350	1351	rBV2	252	253	0.03%	0.004%
48	9.391	1357	1362	1385	rBV	142678	297422	38.06%	5.233%
49	9.708	1411	1414	1415	rBV	299	245	0.03%	0.004%
50	9.860	1436	1439	1441	rBV	266	338	0.04%	0.006%
51	9.976	1456	1458	1460	rVB3	287	235	0.03%	0.004%
52	10.000	1460	1462	1465	rBV2	458	463	0.06%	0.008%
53	10.055	1465	1471	1488	rVV	386563	568652	72.78%	10.005%
54	10.543	1550	1551	1554	rBV2	390	310	0.04%	0.005%
55	10.647	1564	1568	1570	rBV2	333	367	0.05%	0.006%
56	10.671	1570	1572	1575	rVB	255	237	0.03%	0.004%
57	10.793	1591	1592	1596	rBV2	253	319	0.04%	0.006%
58	10.848	1598	1601	1604	rBV2	318	510	0.07%	0.009%
59	10.933	1613	1615	1619	rVV3	301	411	0.05%	0.007%
60	11.067	1636	1637	1640	rVB2	453	361	0.05%	0.006%
61	11.092	1640	1641	1643	rBV	311	249	0.03%	0.004%
62	11.189	1652	1657	1666	rBV	273890	365536	46.78%	6.431%
63	11.354	1682	1684	1687	rBV	293	318	0.04%	0.006%
64	11.482	1703	1705	1707	rVB2	403	282	0.04%	0.005%
65	11.787	1753	1755	1758	rVB2	366	340	0.04%	0.006%
66	11.841	1762	1764	1766	rBV2	400	256	0.03%	0.005%
67	11.927	1775	1778	1779	rBV2	227	245	0.03%	0.004%
68	12.018	1788	1793	1806	rBV	394615	521796	66.78%	9.180%
69	12.152	1813	1815	1817	rVB	591	350	0.04%	0.006%
70	12.250	1829	1831	1834	rBV2	302	326	0.04%	0.006%
71	12.317	1837	1842	1857	rBV	449583	588281	75.29%	10.350%
72	12.530	1874	1877	1879	rBV2	321	358	0.05%	0.006%
73	12.750	1910	1913	1914	rBV2	393	496	0.06%	0.009%
74	12.963	1947	1948	1951	rVB2	424	327	0.04%	0.006%
75	13.006	1951	1955	1961	rBV2	249	626	0.08%	0.011%
76	13.378	2014	2016	2018	rVB	339	278	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043872.D
 Acq On : 15 Nov 2024 13:45
 Operator : JC/MD
 Sample : P4724-24ME
 Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BH9E4ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	13.756	2074	2078	2079	rBV	301	240	0.03%	0.004%
78	13.774	2079	2081	2086	rVB	370	387	0.05%	0.007%
79	14.042	2123	2125	2129	rBV	304	408	0.05%	0.007%
80	14.097	2131	2134	2137	rBV3	345	562	0.07%	0.010%
81	14.128	2137	2139	2144	rVB2	594	749	0.10%	0.013%
82	14.298	2165	2167	2171	rVB	567	453	0.06%	0.008%
83	14.597	2214	2216	2218	rVB2	558	387	0.05%	0.007%
84	14.628	2218	2221	2222	rBV2	371	347	0.04%	0.006%
85	14.646	2222	2224	2227	rBV3	419	520	0.07%	0.009%
86	14.719	2234	2236	2237	rBV2	378	265	0.03%	0.005%
87	14.853	2256	2258	2261	rBV2	360	438	0.06%	0.008%
88	14.957	2273	2275	2276	rBV	411	224	0.03%	0.004%
89	15.207	2313	2316	2317	rBV	748	663	0.08%	0.012%
90	15.371	2342	2343	2344	rBV	695	412	0.05%	0.007%
91	15.451	2354	2356	2357	rVB	547	250	0.03%	0.004%
92	15.573	2374	2376	2378	rBV	374	260	0.03%	0.005%
93	15.713	2397	2399	2400	rBV2	464	327	0.04%	0.006%
94	16.091	2460	2461	2463	rVB	432	247	0.03%	0.004%
95	16.158	2470	2472	2474	rBV2	420	321	0.04%	0.006%
96	16.207	2478	2480	2481	rBV	615	504	0.06%	0.009%
97	16.517	2530	2531	2534	rVB2	373	292	0.04%	0.005%
98	16.554	2534	2537	2539	rBV2	562	534	0.07%	0.009%
99	16.621	2546	2548	2549	rBV	397	257	0.03%	0.005%
100	16.780	2570	2574	2575	rBV2	415	513	0.07%	0.009%

Sum of corrected areas: 5683801




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043872.D
Acq On : 15 Nov 2024 13:45
Operator : JC/MD
Sample : P4724-24ME
Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

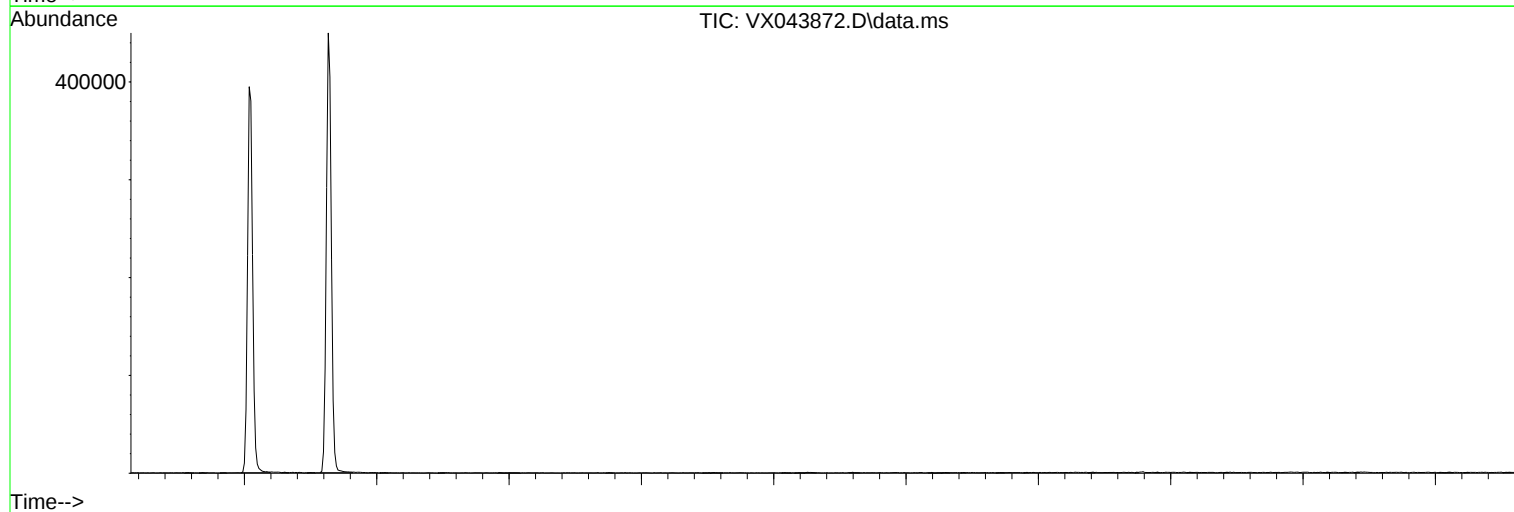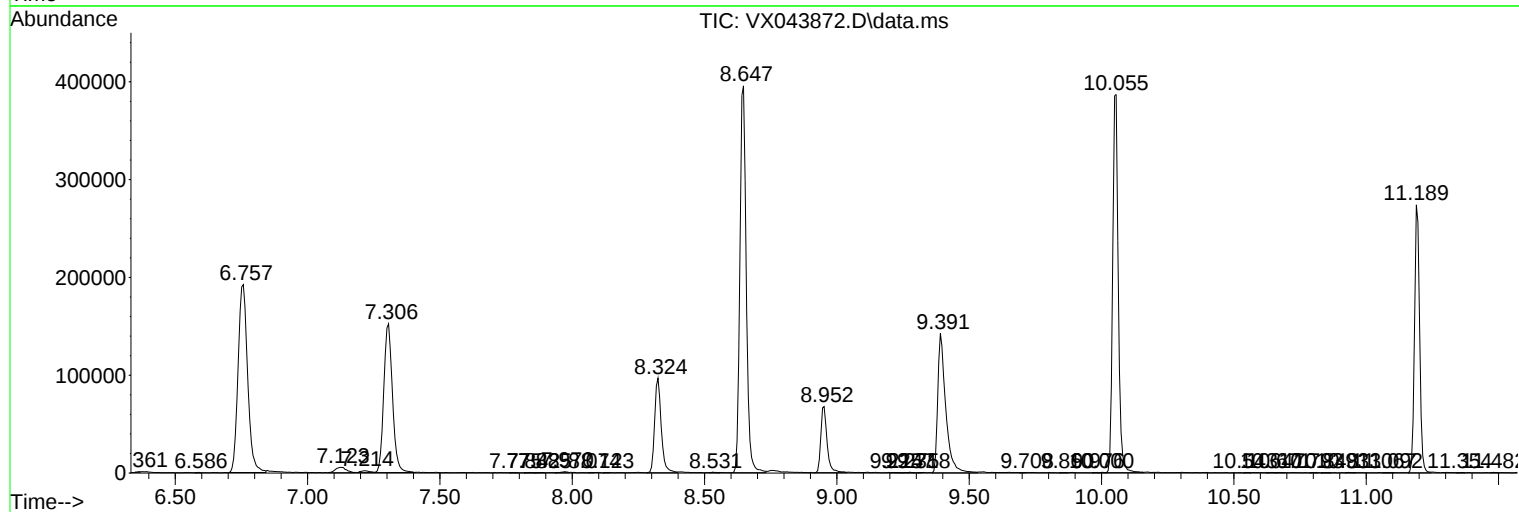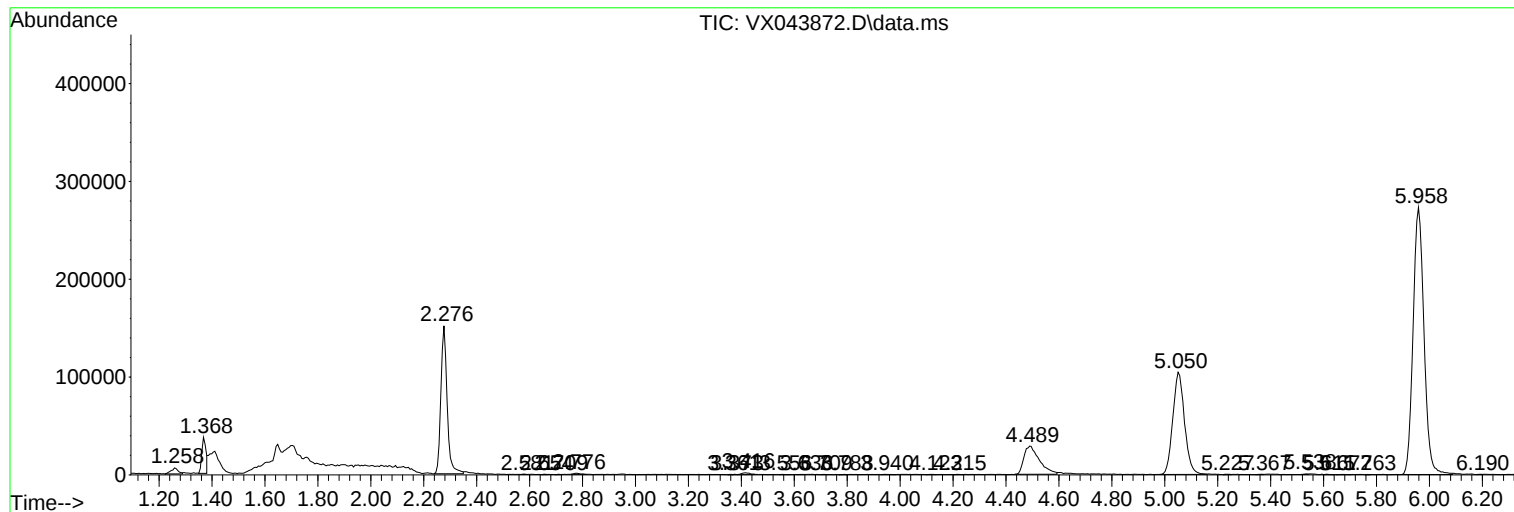

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043872.D
Acq On : 15 Nov 2024 13:45
Operator : JC/MD
Sample : P4724-24ME
Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043872.D
Acq On : 15 Nov 2024 13:45
Operator : JC/MD
Sample : P4724-24ME
Misc : 4.77g/5mL/100uL/5.00mL/MSVOA_X/MEOH
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BH9E4ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
