

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043875.D
 Acq On : 15 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4785-18DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043875.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.239	22	25	32	rVB3	6028	7798	0.95%	0.123%
2	1.367	42	46	62	rVB	84758	101507	12.37%	1.607%
3	1.642	88	91	100	rVB	79020	103263	12.59%	1.634%
4	2.294	192	198	209	rBV	178907	281961	34.37%	4.463%
5	2.385	211	213	218	rVB2	937	1020	0.12%	0.016%
6	2.562	237	242	251	rVB2	2598	4961	0.60%	0.079%
7	2.660	256	258	261	rVB2	500	521	0.06%	0.008%
8	2.745	268	272	273	rBV	292	417	0.05%	0.007%
9	2.782	275	278	283	rVB3	678	966	0.12%	0.015%
10	2.940	297	304	315	rVV2	7100	17395	2.12%	0.275%
11	3.074	319	326	328	rBV2	333	634	0.08%	0.010%
12	3.099	328	330	332	rBV	353	245	0.03%	0.004%
13	3.221	343	350	353	rBV2	565	587	0.07%	0.009%
14	3.434	379	385	394	rVB5	2338	4436	0.54%	0.070%
15	3.556	402	405	407	rBV	206	279	0.03%	0.004%
16	3.678	423	425	427	rBV2	290	286	0.03%	0.005%
17	3.769	438	440	443	rVB2	260	233	0.03%	0.004%
18	3.903	459	462	463	rBV	340	247	0.03%	0.004%
19	3.946	467	469	471	rBV2	267	258	0.03%	0.004%
20	4.044	483	485	487	rVB2	312	234	0.03%	0.004%
21	4.153	500	503	505	rBV	425	374	0.05%	0.006%
22	4.318	528	530	533	rVB2	557	546	0.07%	0.009%
23	4.385	540	541	545	rBV3	214	246	0.03%	0.004%
24	4.458	545	553	570	rBV2	43580	140738	17.15%	2.228%
25	4.830	613	614	617	rBV2	263	256	0.03%	0.004%
26	4.861	617	619	621	rBV	235	256	0.03%	0.004%
27	5.050	638	650	669	rBV2	111499	340481	41.50%	5.389%
28	5.263	683	685	689	rVB2	503	431	0.05%	0.007%
29	5.306	689	692	695	rBV2	498	659	0.08%	0.010%
30	5.367	698	702	703	rBV2	272	296	0.04%	0.005%
31	5.556	728	733	737	rBV4	594	1348	0.16%	0.021%
32	5.653	747	749	752	rBV2	176	259	0.03%	0.004%
33	5.726	760	761	765	rBV2	179	230	0.03%	0.004%
34	5.769	765	768	771	rVV3	231	226	0.03%	0.004%
35	5.860	782	783	786	rBV2	309	283	0.03%	0.004%
36	5.964	786	800	817	rBV2	273337	813869	99.20%	12.881%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043875.D
 Acq On : 15 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4785-18DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	6.269	848	850	853	rBV2	266	263	0.03%	0.004%
38	6.379	864	868	870	rBV2	262	433	0.05%	0.007%
39	6.452	878	880	882	rVB	382	294	0.04%	0.005%
40	6.757	918	930	947	rBV2	209152	511268	62.32%	8.092%
41	6.958	961	963	967	rVB2	226	253	0.03%	0.004%
42	7.049	976	978	979	rBV	397	295	0.04%	0.005%
43	7.128	984	991	1001	rVB7	4658	11591	1.41%	0.183%
44	7.305	1011	1020	1039	rBV	163139	359111	43.77%	5.684%
45	7.433	1039	1041	1043	rVB	449	306	0.04%	0.005%
46	7.549	1058	1060	1064	rVB2	418	387	0.05%	0.006%
47	7.622	1070	1072	1073	rBV2	288	253	0.03%	0.004%
48	7.732	1086	1090	1092	rBV3	196	284	0.03%	0.004%
49	7.769	1092	1096	1098	rVB2	252	328	0.04%	0.005%
50	8.025	1135	1138	1139	rBV2	291	313	0.04%	0.005%
51	8.140	1154	1157	1159	rBV	323	267	0.03%	0.004%
52	8.323	1181	1187	1196	rBV	105520	178507	21.76%	2.825%
53	8.445	1205	1207	1209	rBV3	454	256	0.03%	0.004%
54	8.512	1214	1218	1219	rBV2	244	249	0.03%	0.004%
55	8.646	1234	1240	1255	rBV	415800	663314	80.85%	10.498%
56	8.951	1284	1290	1303	rBV	73219	117389	14.31%	1.858%
57	9.171	1324	1326	1328	rBV	244	218	0.03%	0.003%
58	9.201	1329	1331	1334	rVV	372	269	0.03%	0.004%
59	9.274	1340	1343	1349	rVB3	565	1068	0.13%	0.017%
60	9.384	1356	1361	1384	rBV	210580	329250	40.13%	5.211%
61	9.640	1401	1403	1405	rBV2	255	247	0.03%	0.004%
62	9.774	1422	1425	1426	rBV2	220	219	0.03%	0.003%
63	9.957	1453	1455	1457	rVB2	351	248	0.03%	0.004%
64	10.055	1465	1471	1484	rBV	401248	582614	71.01%	9.221%
65	10.238	1500	1501	1506	rBV2	435	594	0.07%	0.009%
66	10.280	1506	1508	1510	rVV2	394	336	0.04%	0.005%
67	10.366	1520	1522	1525	rVB3	391	427	0.05%	0.007%
68	10.390	1525	1526	1528	rBV	296	249	0.03%	0.004%
69	10.427	1531	1532	1537	rBV3	241	237	0.03%	0.004%
70	10.482	1537	1541	1543	rVB2	248	328	0.04%	0.005%
71	10.585	1556	1558	1562	rVB2	280	344	0.04%	0.005%
72	10.805	1589	1594	1596	rBV	325	461	0.06%	0.007%
73	10.981	1622	1623	1625	rVB2	370	238	0.03%	0.004%
74	11.073	1635	1638	1639	rBV2	266	296	0.04%	0.005%
75	11.189	1652	1657	1671	rBV	299498	389466	47.47%	6.164%
76	11.305	1674	1676	1682	rVB3	428	531	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043875.D
 Acq On : 15 Nov 2024 14:54
 Operator : JC/MD
 Sample : P4785-18DL 4X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N9DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	11.384	1687	1689	1693	rVB2	307	310	0.04%	0.005%
78	11.439	1693	1698	1700	rBV	235	444	0.05%	0.007%
79	11.512	1707	1710	1711	rBV2	245	259	0.03%	0.004%
80	11.640	1730	1731	1735	rVV2	233	278	0.03%	0.004%
81	11.847	1763	1765	1767	rVV2	221	243	0.03%	0.004%
82	11.865	1767	1768	1771	rVV2	314	289	0.04%	0.005%
83	11.920	1774	1777	1779	rVB2	194	240	0.03%	0.004%
84	12.018	1788	1793	1804	rBV	379283	506505	61.74%	8.017%
85	12.317	1837	1842	1855	rBV	609595	820435	100.00%	12.985%
86	12.646	1894	1896	1897	rBV	591	543	0.07%	0.009%
87	13.121	1973	1974	1975	rBV	674	284	0.03%	0.004%
88	13.249	1993	1995	1999	rVB	495	413	0.05%	0.007%
89	14.993	2276	2281	2283	rBV2	884	1484	0.18%	0.023%
90	15.090	2296	2297	2300	rBV2	683	483	0.06%	0.008%
91	15.493	2362	2363	2367	rBV3	690	641	0.08%	0.010%
92	15.523	2367	2368	2370	rBV2	368	271	0.03%	0.004%
93	15.548	2370	2372	2374	rVV3	559	365	0.04%	0.006%
94	15.596	2379	2380	2381	rBV	478	254	0.03%	0.004%
95	15.676	2391	2393	2396	rBV2	423	337	0.04%	0.005%
96	15.968	2437	2441	2444	rBV4	1235	1845	0.22%	0.029%
97	15.993	2444	2445	2446	rVB	795	291	0.04%	0.005%
98	16.200	2477	2479	2482	rVB3	642	446	0.05%	0.007%
99	16.371	2505	2507	2508	rBV2	463	346	0.04%	0.005%
100	16.755	2568	2570	2572	rBV2	434	427	0.05%	0.007%

Sum of corrected areas: 6318180




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043875.D
Acq On : 15 Nov 2024 14:54
Operator : JC/MD
Sample : P4785-18DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

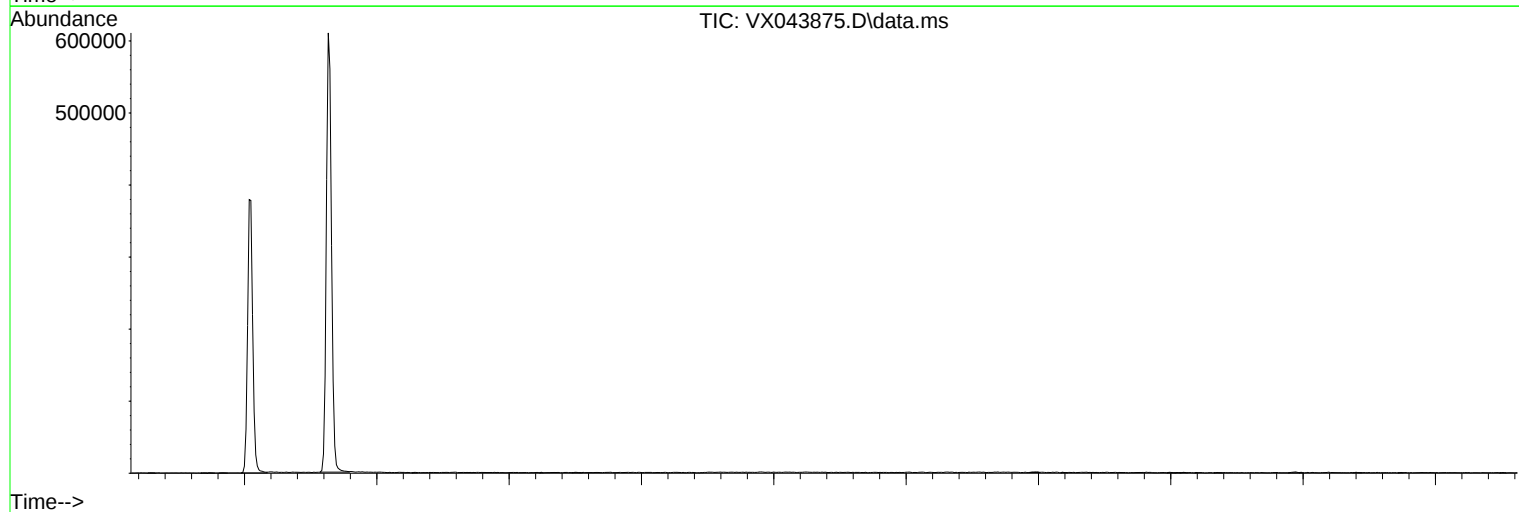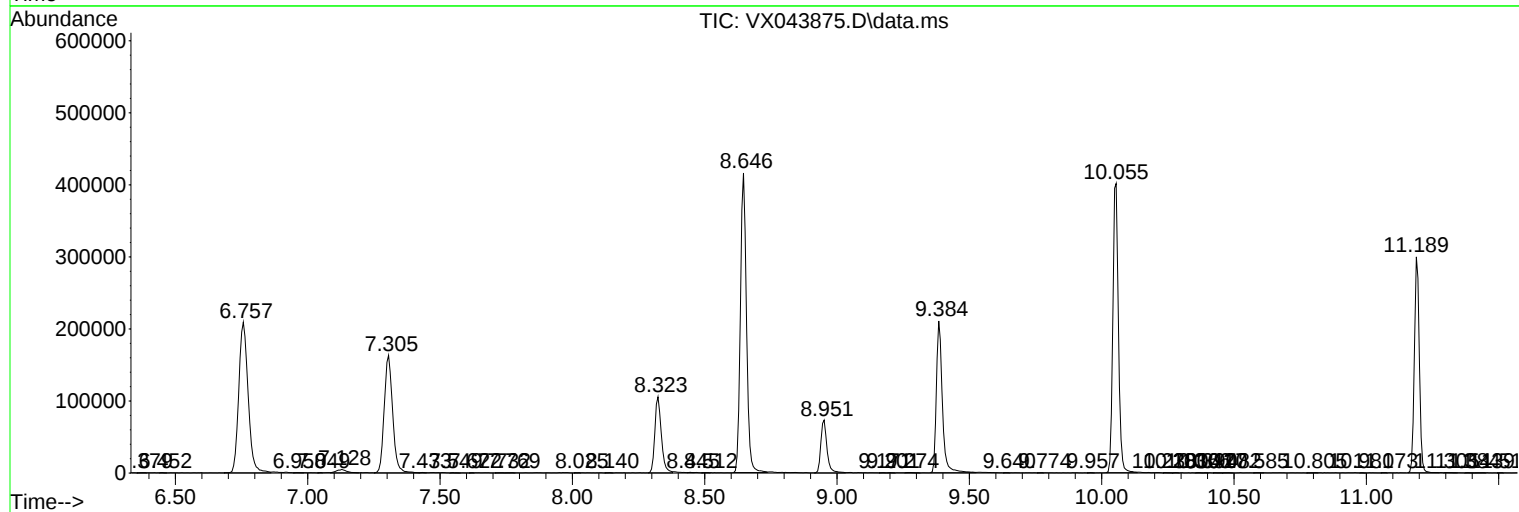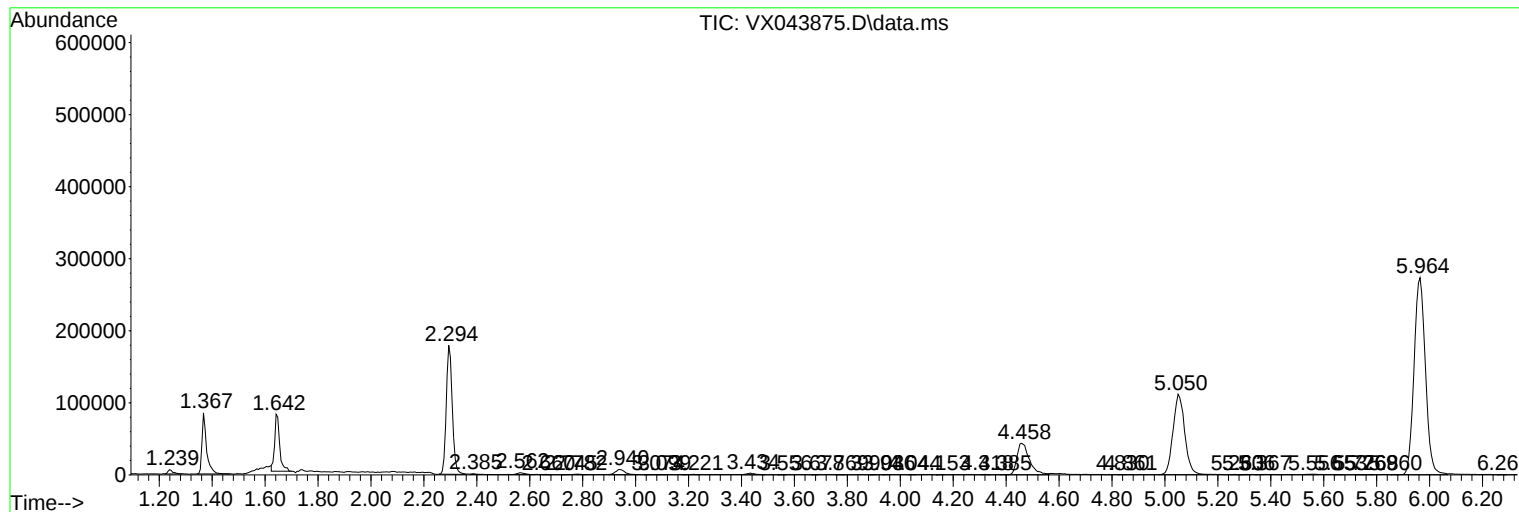

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043875.D
Acq On : 15 Nov 2024 14:54
Operator : JC/MD
Sample : P4785-18DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043875.D
Acq On : 15 Nov 2024 14:54
Operator : JC/MD
Sample : P4785-18DL 4X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N9DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc