

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043876.D
 Acq On : 15 Nov 2024 15:17
 Operator : JC/MD
 Sample : P4785-16DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043876.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	28	rBV	5735	6491	0.65%	0.084%
2	1.368	42	46	59	rBV	82074	102379	10.32%	1.326%
3	1.642	88	91	102	rVB	76979	104175	10.50%	1.350%
4	1.727	102	105	109	rBV4	6262	10632	1.07%	0.138%
5	2.294	192	198	210	rBV	183778	286611	28.89%	3.713%
6	2.502	230	232	234	rBV2	341	319	0.03%	0.004%
7	2.550	238	240	242	rVV	377	278	0.03%	0.004%
8	2.660	254	258	260	rBV2	357	581	0.06%	0.008%
9	2.788	274	279	283	rBV2	854	1292	0.13%	0.017%
10	2.867	289	292	293	rBV	258	228	0.02%	0.003%
11	2.934	300	303	305	rBV3	428	480	0.05%	0.006%
12	3.221	346	350	352	rVB2	267	323	0.03%	0.004%
13	3.312	361	365	369	rVB	294	386	0.04%	0.005%
14	3.434	381	385	390	rVB4	1334	2553	0.26%	0.033%
15	3.550	402	404	407	rVB2	268	286	0.03%	0.004%
16	3.587	407	410	411	rBV	273	276	0.03%	0.004%
17	3.648	417	420	422	rVB2	258	247	0.02%	0.003%
18	3.684	422	426	428	rBV2	289	406	0.04%	0.005%
19	3.892	456	460	465	rVB	377	624	0.06%	0.008%
20	3.934	465	467	470	rBV2	351	438	0.04%	0.006%
21	4.074	486	490	492	rVB2	301	274	0.03%	0.004%
22	4.361	536	537	542	rVB2	303	241	0.02%	0.003%
23	4.465	544	554	571	rBV	49137	163381	16.47%	2.117%
24	4.690	587	591	593	rBV2	359	525	0.05%	0.007%
25	4.879	620	622	623	rBV	281	292	0.03%	0.004%
26	4.958	633	635	638	rBV2	425	384	0.04%	0.005%
27	5.050	638	650	666	rBV	113235	346392	34.92%	4.488%
28	5.312	691	693	695	rBV2	370	403	0.04%	0.005%
29	5.367	700	702	703	rBV	806	588	0.06%	0.008%
30	5.550	724	732	737	rBV3	802	2175	0.22%	0.028%
31	5.861	781	783	786	rVV2	257	216	0.02%	0.003%
32	5.958	788	799	819	rBV3	282666	842081	84.89%	10.909%
33	6.281	851	852	855	rBV2	294	357	0.04%	0.005%
34	6.373	863	867	871	rBV2	265	511	0.05%	0.007%
35	6.464	878	882	883	rBV2	334	364	0.04%	0.005%
36	6.507	887	889	890	rBV	382	269	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043876.D
 Acq On : 15 Nov 2024 15:17
 Operator : JC/MD
 Sample : P4785-16DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Title : VOC Analysis

37	6.568	897	899	901	rVB	387	277	0.03%	0.004%
38	6.605	901	905	906	rBV2	293	351	0.04%	0.005%
39	6.617	906	907	909	rBV2	313	219	0.02%	0.003%
40	6.684	915	918	919	rBV2	282	239	0.02%	0.003%
41	6.757	921	930	944	rBV	206704	512278	51.65%	6.637%
42	7.123	981	990	1005	rBV	445939	991916	100.00%	12.851%
43	7.306	1012	1020	1037	rVB	163239	364166	36.71%	4.718%
44	7.476	1045	1048	1049	rBV2	513	495	0.05%	0.006%
45	7.592	1063	1067	1068	rVB	260	272	0.03%	0.004%
46	7.623	1071	1072	1077	rVV3	215	326	0.03%	0.004%
47	7.866	1110	1112	1114	rVB2	330	300	0.03%	0.004%
48	7.897	1114	1117	1119	rBV	313	425	0.04%	0.006%
49	7.940	1122	1124	1127	rBV2	410	461	0.05%	0.006%
50	7.964	1127	1128	1130	rVB	476	266	0.03%	0.003%
51	8.196	1164	1166	1168	rVB2	308	257	0.03%	0.003%
52	8.324	1181	1187	1197	rBV	109187	181672	18.32%	2.354%
53	8.488	1213	1214	1217	rVB2	602	339	0.03%	0.004%
54	8.525	1217	1220	1222	rBV2	468	524	0.05%	0.007%
55	8.543	1222	1223	1226	rVB	382	344	0.03%	0.004%
56	8.568	1226	1227	1230	rBV2	277	290	0.03%	0.004%
57	8.647	1233	1240	1258	rBV	428835	676467	68.20%	8.764%
58	8.952	1284	1290	1298	rBV	74154	116205	11.72%	1.505%
59	9.049	1305	1306	1311	rBV3	465	544	0.05%	0.007%
60	9.183	1326	1328	1331	rBV2	169	264	0.03%	0.003%
61	9.275	1341	1343	1346	rBV3	722	694	0.07%	0.009%
62	9.385	1356	1361	1374	rBV	210475	332954	33.57%	4.314%
63	9.738	1416	1419	1420	rBV2	210	220	0.02%	0.003%
64	10.049	1465	1470	1484	rBV	412421	592810	59.76%	7.680%
65	10.183	1490	1492	1495	rBV3	551	463	0.05%	0.006%
66	10.299	1510	1511	1514	rBV2	262	302	0.03%	0.004%
67	10.403	1526	1528	1531	rBV2	346	444	0.04%	0.006%
68	10.586	1556	1558	1560	rVB	318	229	0.02%	0.003%
69	10.622	1560	1564	1565	rBV2	306	320	0.03%	0.004%
70	10.988	1622	1624	1625	rBV	383	267	0.03%	0.003%
71	11.189	1652	1657	1669	rBV	303836	404021	40.73%	5.234%
72	11.445	1697	1699	1700	rBV	369	307	0.03%	0.004%
73	11.768	1750	1752	1753	rBV	471	305	0.03%	0.004%
74	11.866	1765	1768	1769	rBV2	593	624	0.06%	0.008%
75	11.896	1771	1773	1775	rVV	589	410	0.04%	0.005%
76	11.945	1779	1781	1782	rBV	684	502	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043876.D
 Acq On : 15 Nov 2024 15:17
 Operator : JC/MD
 Sample : P4785-16DL 1000X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27N7DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.018	1788	1793	1804	rBV	548401	718466	72.43%	9.308%
78	12.317	1837	1842	1857	rBV	711609	929481	93.71%	12.042%
79	12.920	1940	1941	1942	rBV	471	254	0.03%	0.003%
80	13.134	1974	1976	1977	rBV	528	293	0.03%	0.004%
81	13.530	2039	2041	2043	rBV	545	358	0.04%	0.005%
82	13.548	2043	2044	2046	rBV2	622	483	0.05%	0.006%
83	14.292	2165	2166	2168	rVB	781	411	0.04%	0.005%
84	14.329	2168	2172	2175	rVB2	751	998	0.10%	0.013%
85	14.359	2175	2177	2180	rBV3	601	833	0.08%	0.011%
86	14.432	2187	2189	2192	rBV2	572	534	0.05%	0.007%
87	14.481	2195	2197	2198	rVB	409	230	0.02%	0.003%
88	14.701	2231	2233	2235	rVB2	389	286	0.03%	0.004%
89	14.975	2276	2278	2281	rVB3	374	346	0.03%	0.004%
90	15.012	2281	2284	2287	rBV2	519	648	0.07%	0.008%
91	15.127	2301	2303	2305	rBV2	443	349	0.04%	0.005%
92	15.152	2305	2307	2309	rBV2	415	342	0.03%	0.004%
93	15.231	2317	2320	2322	rBV2	540	504	0.05%	0.007%
94	15.377	2342	2344	2346	rBV2	569	350	0.04%	0.005%
95	15.804	2412	2414	2416	rBV2	452	502	0.05%	0.007%
96	15.993	2444	2445	2449	rBV3	573	382	0.04%	0.005%
97	16.048	2452	2454	2457	rVV3	477	562	0.06%	0.007%
98	16.072	2457	2458	2459	rVB	588	215	0.02%	0.003%
99	16.255	2487	2488	2490	rBV	418	324	0.03%	0.004%
100	16.414	2510	2514	2515	rBV2	411	497	0.05%	0.006%

Sum of corrected areas: 7718875




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043876.D
Acq On : 15 Nov 2024 15:17
Operator : JC/MD
Sample : P4785-16DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

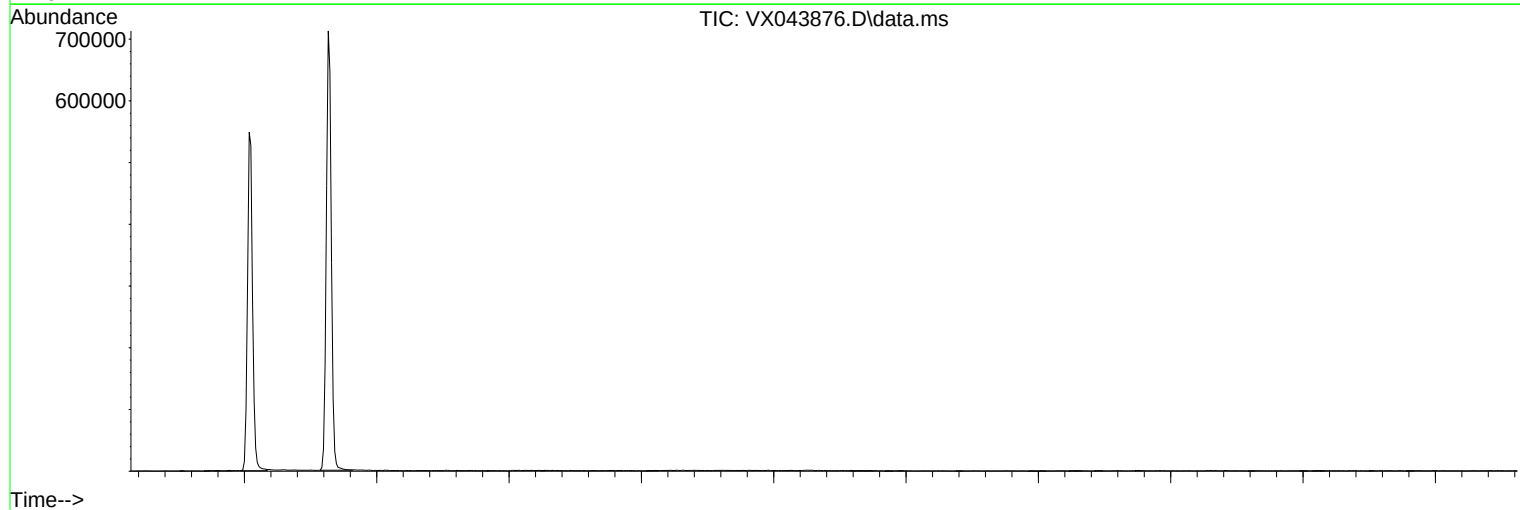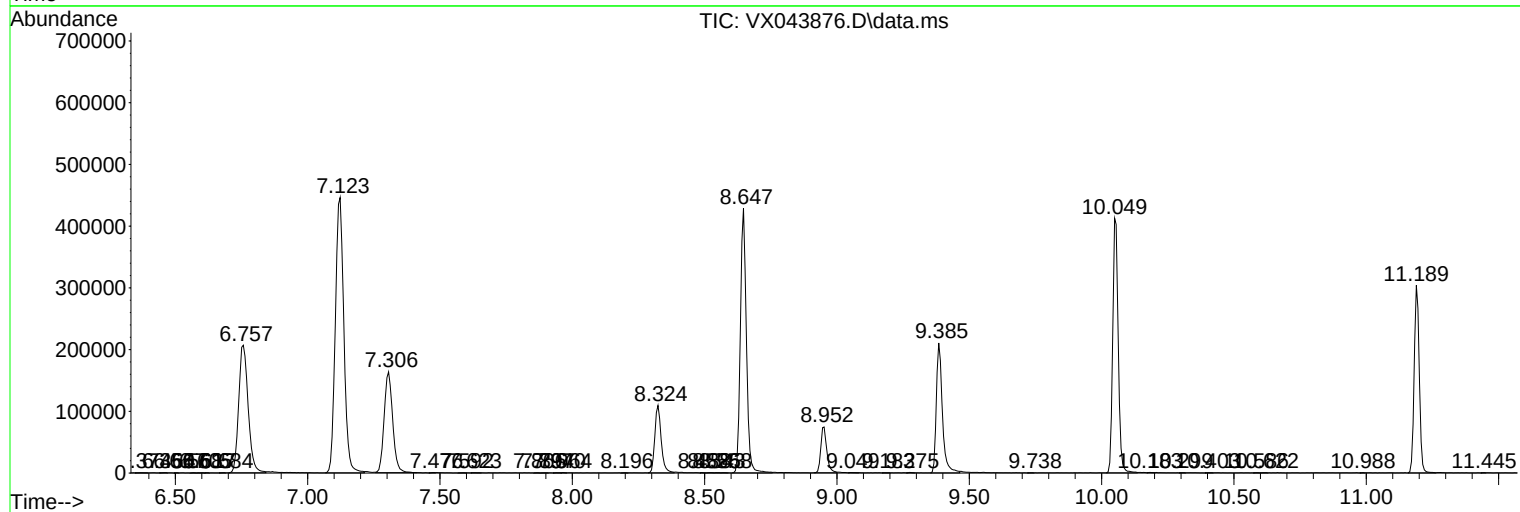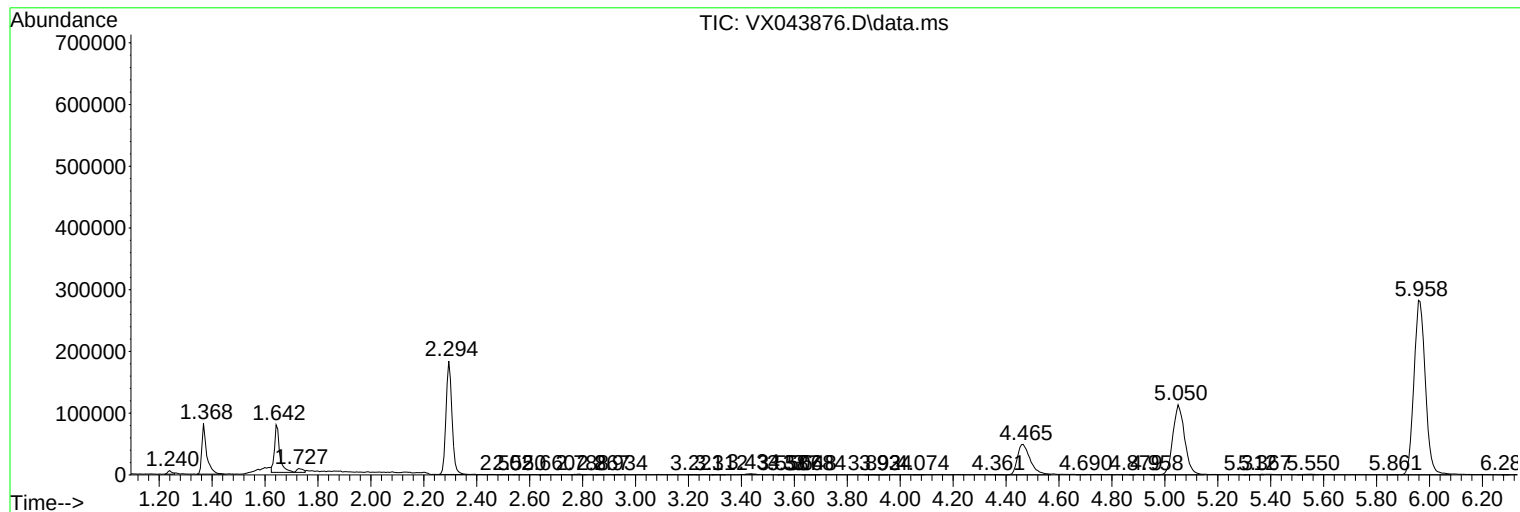

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043876.D
Acq On : 15 Nov 2024 15:17
Operator : JC/MD
Sample : P4785-16DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043876.D
Acq On : 15 Nov 2024 15:17
Operator : JC/MD
Sample : P4785-16DL 1000X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27N7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------