

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043878.D
 Acq On : 15 Nov 2024 16:03
 Operator : JC/MD
 Sample : P4785-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.148	7	10	16	rVB3	1752	2450	0.25%	0.036%
2	1.240	22	25	32	rVB3	5417	7390	0.76%	0.109%
3	1.368	42	46	62	rBV	84082	105640	10.90%	1.560%
4	1.648	88	92	102	rVB	80584	105799	10.92%	1.562%
5	2.294	192	198	209	rBV	180274	289972	29.93%	4.282%
6	2.386	209	213	223	rVB	4031	8049	0.83%	0.119%
7	2.496	229	231	235	rBV3	591	640	0.07%	0.009%
8	2.770	274	276	277	rBV2	525	313	0.03%	0.005%
9	2.886	293	295	298	rBV2	270	271	0.03%	0.004%
10	2.947	298	305	310	rBV3	1804	4073	0.42%	0.060%
11	3.062	322	324	327	rBV2	301	300	0.03%	0.004%
12	3.203	344	347	350	rVB2	342	495	0.05%	0.007%
13	3.251	350	355	358	rBV2	394	820	0.08%	0.012%
14	3.434	380	385	393	rVB4	1677	3677	0.38%	0.054%
15	4.038	483	484	488	rBV	367	416	0.04%	0.006%
16	4.178	505	507	513	rVV2	268	315	0.03%	0.005%
17	4.398	541	543	544	rBV	415	262	0.03%	0.004%
18	4.459	545	553	570	rBV	46075	141903	14.65%	2.095%
19	4.812	609	611	615	rVB4	381	420	0.04%	0.006%
20	4.861	615	619	620	rBV2	468	640	0.07%	0.009%
21	5.050	637	650	667	rBV2	110731	361487	37.31%	5.338%
22	5.282	686	688	689	rBV	296	290	0.03%	0.004%
23	5.501	721	724	725	rBV2	312	338	0.03%	0.005%
24	5.556	729	733	738	rVV3	690	1255	0.13%	0.019%
25	5.964	789	800	818	rBV3	272239	820300	84.67%	12.112%
26	6.294	851	854	855	rVB2	381	324	0.03%	0.005%
27	6.306	855	856	860	rVB2	435	375	0.04%	0.006%
28	6.361	862	865	867	rVB2	432	461	0.05%	0.007%
29	6.409	871	873	875	rBV	321	312	0.03%	0.005%
30	6.458	879	881	883	rVV	392	286	0.03%	0.004%
31	6.544	893	895	899	rBV2	355	422	0.04%	0.006%
32	6.611	903	906	908	rBV2	282	365	0.04%	0.005%
33	6.757	921	930	949	rBV	198474	482544	49.81%	7.125%
34	7.123	983	990	1001	rVB5	6829	17250	1.78%	0.255%
35	7.306	1011	1020	1034	rVV	159598	362767	37.44%	5.357%
36	7.568	1060	1063	1064	rBV2	419	394	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043878.D
 Acq On : 15 Nov 2024 16:03
 Operator : JC/MD
 Sample : P4785-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	7.586	1064	1066	1067	rVV	382	261	0.03%	0.004%
38	7.671	1077	1080	1082	rVB	288	256	0.03%	0.004%
39	7.793	1094	1100	1101	rVV3	352	557	0.06%	0.008%
40	7.842	1106	1108	1112	rVV2	186	269	0.03%	0.004%
41	7.897	1115	1117	1119	rVV	304	309	0.03%	0.005%
42	7.946	1122	1125	1127	rVV2	335	388	0.04%	0.006%
43	7.970	1127	1129	1130	rVV2	383	311	0.03%	0.005%
44	7.988	1130	1132	1133	rVB	425	261	0.03%	0.004%
45	8.025	1136	1138	1141	rVB2	337	324	0.03%	0.005%
46	8.135	1154	1156	1160	rVB3	263	265	0.03%	0.004%
47	8.324	1181	1187	1202	rBV	106191	175986	18.16%	2.599%
48	8.507	1213	1217	1218	rBV2	525	553	0.06%	0.008%
49	8.562	1222	1226	1227	rBV2	326	399	0.04%	0.006%
50	8.647	1233	1240	1258	rBV	416764	673480	69.51%	9.944%
51	8.830	1268	1270	1272	rBV2	277	259	0.03%	0.004%
52	8.952	1284	1290	1304	rBV	75578	116926	12.07%	1.726%
53	9.385	1356	1361	1374	rBV	212463	329751	34.03%	4.869%
54	9.695	1410	1412	1415	rVV	526	472	0.05%	0.007%
55	9.756	1421	1422	1426	rVB2	440	370	0.04%	0.005%
56	10.055	1465	1471	1482	rBV	380257	552206	57.00%	8.154%
57	10.208	1494	1496	1500	rVB2	570	747	0.08%	0.011%
58	10.244	1500	1502	1509	rVB4	420	587	0.06%	0.009%
59	10.299	1509	1511	1512	rBV	394	288	0.03%	0.004%
60	10.445	1531	1535	1537	rBV2	302	390	0.04%	0.006%
61	10.549	1550	1552	1555	rBV2	269	365	0.04%	0.005%
62	10.701	1576	1577	1580	rBV	464	399	0.04%	0.006%
63	10.805	1593	1594	1597	rVB	352	296	0.03%	0.004%
64	10.945	1616	1617	1621	rBV	317	351	0.04%	0.005%
65	11.116	1643	1645	1648	rBV2	303	461	0.05%	0.007%
66	11.189	1652	1657	1667	rVV	310374	412244	42.55%	6.087%
67	11.311	1675	1677	1681	rVB3	1123	998	0.10%	0.015%
68	11.494	1704	1707	1709	rBV2	727	781	0.08%	0.012%
69	11.524	1709	1712	1714	rBV2	735	893	0.09%	0.013%
70	11.567	1717	1719	1723	rVB2	1998	2380	0.25%	0.035%
71	11.628	1728	1729	1731	rVV	535	299	0.03%	0.004%
72	11.823	1759	1761	1768	rVB3	1608	1899	0.20%	0.028%
73	11.902	1772	1774	1777	rBV3	954	1158	0.12%	0.017%
74	12.018	1788	1793	1802	rBV	585910	764831	78.94%	11.293%
75	12.219	1822	1826	1834	rBV3	9876	17134	1.77%	0.253%
76	12.317	1837	1842	1855	rVB	764780	968863	100.00%	14.306%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043878.D
 Acq On : 15 Nov 2024 16:03
 Operator : JC/MD
 Sample : P4785-20
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.512	1872	1874	1876	rVB2	812	432	0.04%	0.006%
78	12.610	1889	1890	1892	rBV	720	746	0.08%	0.011%
79	12.860	1928	1931	1943	rVB4	4656	7152	0.74%	0.106%
80	13.006	1953	1955	1958	rVB2	571	298	0.03%	0.004%
81	13.116	1968	1973	1975	rBV3	1154	1943	0.20%	0.029%
82	13.591	2049	2051	2057	rVB4	1308	1552	0.16%	0.023%
83	13.701	2067	2069	2071	rBV2	1022	993	0.10%	0.015%
84	13.890	2098	2100	2102	rBV3	693	708	0.07%	0.010%
85	14.304	2165	2168	2171	rBV3	434	541	0.06%	0.008%
86	14.371	2177	2179	2181	rBV2	520	376	0.04%	0.006%
87	14.438	2188	2190	2191	rBV	313	265	0.03%	0.004%
88	14.932	2269	2271	2274	rBV	572	459	0.05%	0.007%
89	14.981	2276	2279	2280	rBV	584	446	0.05%	0.007%
90	14.999	2280	2282	2285	rBV2	363	403	0.04%	0.006%
91	15.030	2285	2287	2290	rBV2	467	563	0.06%	0.008%
92	15.182	2308	2312	2313	rBV3	368	463	0.05%	0.007%
93	15.225	2318	2319	2323	rBV2	363	518	0.05%	0.008%
94	15.304	2330	2332	2334	rVB2	372	275	0.03%	0.004%
95	15.572	2374	2376	2379	rBV3	505	381	0.04%	0.006%
96	16.042	2452	2453	2455	rVB	505	259	0.03%	0.004%
97	16.127	2465	2467	2469	rBV3	438	400	0.04%	0.006%
98	16.176	2473	2475	2476	rVB	714	370	0.04%	0.005%
99	16.335	2498	2501	2502	rBV	543	395	0.04%	0.006%
100	16.670	2554	2556	2560	rBV3	459	519	0.05%	0.008%

Sum of corrected areas: 6772439




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043878.D
Acq On : 15 Nov 2024 16:03
Operator : JC/MD
Sample : P4785-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

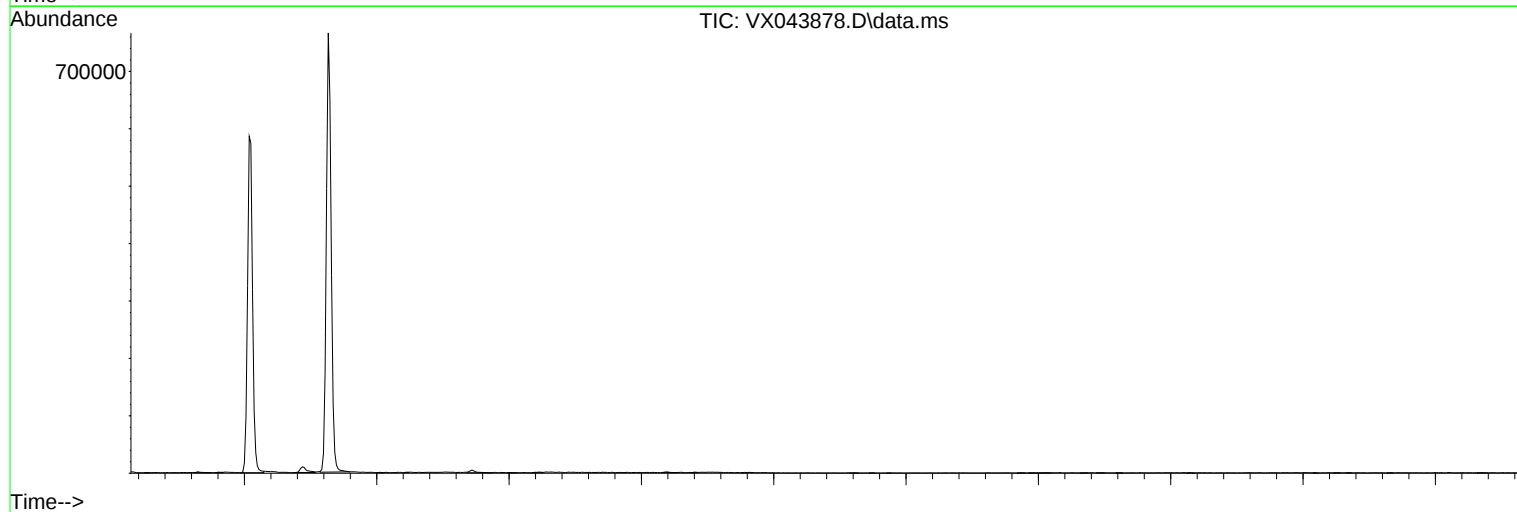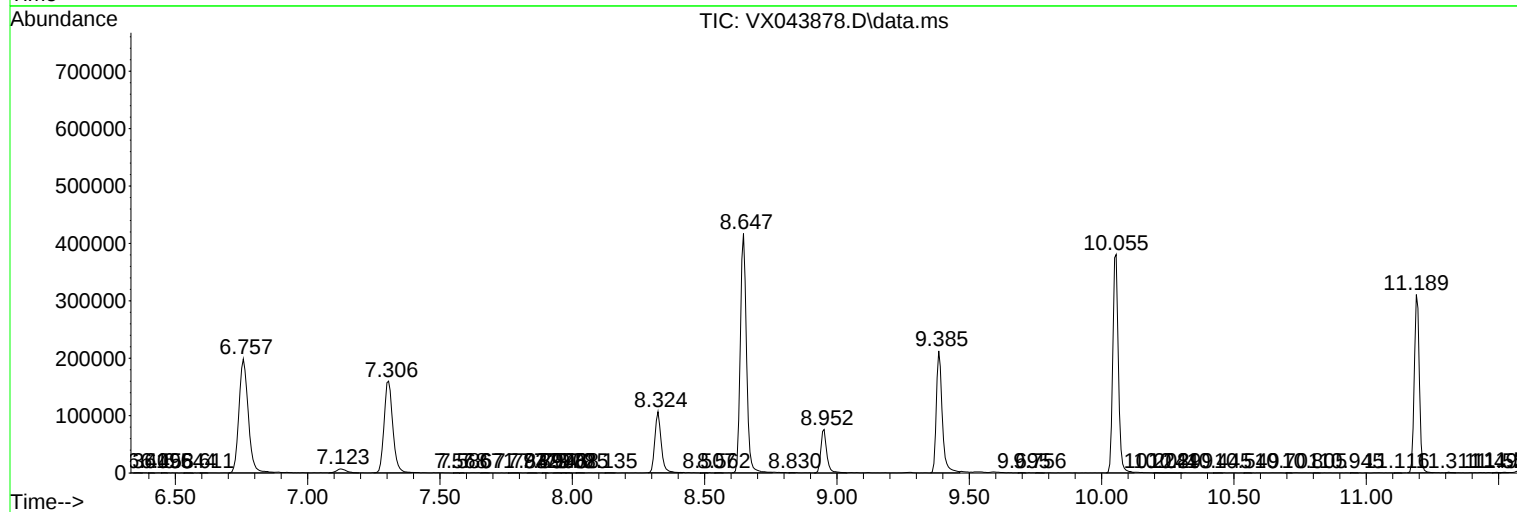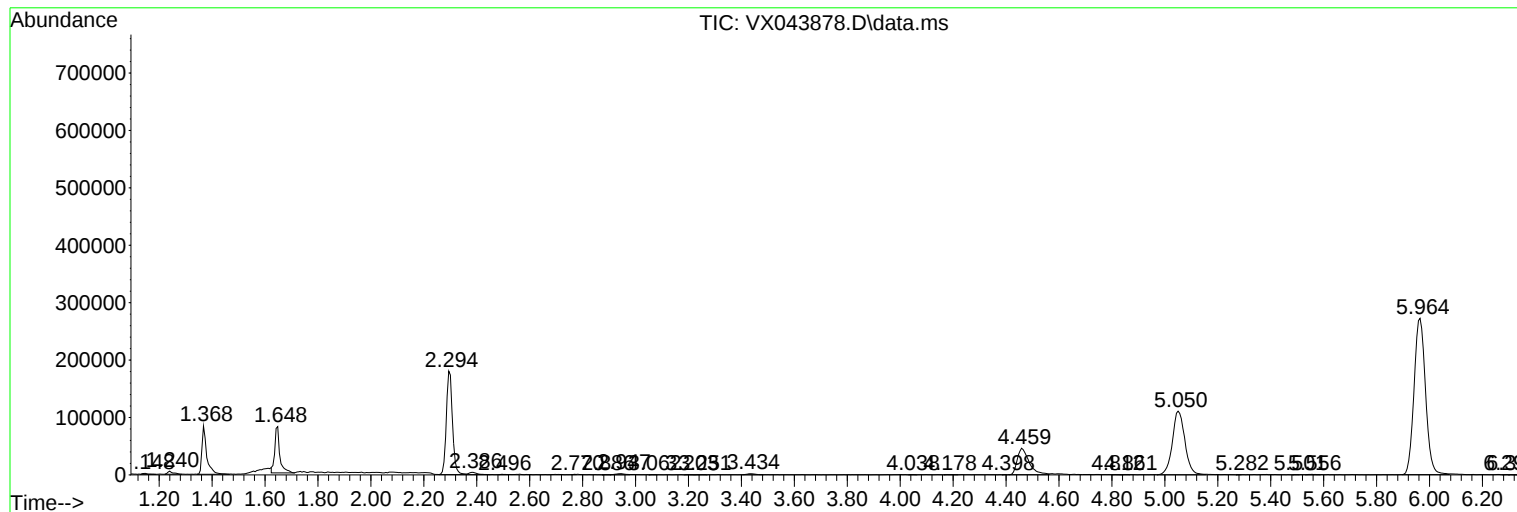

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043878.D
Acq On : 15 Nov 2024 16:03
Operator : JC/MD
Sample : P4785-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043878.D
Acq On : 15 Nov 2024 16:03
Operator : JC/MD
Sample : P4785-20
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc
