

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043880.D
 Acq On : 15 Nov 2024 16:50
 Operator : JC/MD
 Sample : P4785-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXML111424WMA.M
 Title : VOC Analysis

Signal : TIC: VX043880.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.240	22	25	32	rBV2	5720	8295	1.05%	0.141%
2	1.368	43	46	61	rVB	78487	99836	12.60%	1.691%
3	1.618	71	87	88	rBV5	12232	38935	4.91%	0.659%
4	1.648	88	92	104	rVB	68590	108903	13.74%	1.845%
5	1.807	115	118	121	rBV2	4811	7576	0.96%	0.128%
6	2.294	192	198	210	rVV	171423	267078	33.70%	4.524%
7	2.392	210	214	223	rVB5	1327	2592	0.33%	0.044%
8	2.520	234	235	238	rBV2	391	284	0.04%	0.005%
9	2.569	241	243	246	rVB2	638	564	0.07%	0.010%
10	2.703	261	265	267	rBV2	307	370	0.05%	0.006%
11	2.788	272	279	282	rBV5	767	1225	0.15%	0.021%
12	2.940	300	304	310	rVB3	972	1913	0.24%	0.032%
13	3.093	327	329	331	rBV2	239	222	0.03%	0.004%
14	3.203	346	347	350	rBV2	263	257	0.03%	0.004%
15	3.379	373	376	378	rBV2	192	249	0.03%	0.004%
16	3.428	378	384	392	rVV6	1781	4421	0.56%	0.075%
17	3.483	392	393	396	rVV	267	221	0.03%	0.004%
18	3.532	398	401	403	rVV2	435	476	0.06%	0.008%
19	3.556	403	405	407	rVV2	231	216	0.03%	0.004%
20	3.574	407	408	410	rVV	280	213	0.03%	0.004%
21	3.617	413	415	418	rBV3	432	472	0.06%	0.008%
22	3.690	425	427	430	rBV2	325	284	0.04%	0.005%
23	3.818	446	448	452	rBV3	307	468	0.06%	0.008%
24	3.867	452	456	458	rVV2	194	320	0.04%	0.005%
25	3.940	466	468	471	rVV2	369	293	0.04%	0.005%
26	3.983	473	475	478	rVB	241	237	0.03%	0.004%
27	4.123	496	498	501	rBV3	253	294	0.04%	0.005%
28	4.337	532	533	536	rVB	379	219	0.03%	0.004%
29	4.385	536	541	544	rBV2	361	683	0.09%	0.012%
30	4.465	544	554	570	rBV2	42371	135855	17.14%	2.301%
31	5.056	639	651	669	rVV	108268	333862	42.13%	5.655%
32	5.233	678	680	684	rBV2	322	294	0.04%	0.005%
33	5.507	723	725	727	rBV2	282	236	0.03%	0.004%
34	5.538	728	730	731	rBV2	392	244	0.03%	0.004%
35	5.781	767	770	773	rBV2	290	323	0.04%	0.005%
36	5.964	788	800	820	rBV2	264237	792446	100.00%	13.423%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043880.D
 Acq On : 15 Nov 2024 16:50
 Operator : JC/MD
 Sample : P4785-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

37	6.226	842	843	845	rBV	371	295	0.04%	0.005%
38	6.251	845	847	851	rVB2	416	443	0.06%	0.008%
39	6.300	851	855	858	rBV2	425	647	0.08%	0.011%
40	6.361	864	865	868	rBV	392	450	0.06%	0.008%
41	6.598	900	904	905	rVB2	240	231	0.03%	0.004%
42	6.757	921	930	948	rVV	190510	467650	59.01%	7.921%
43	7.129	981	991	1001	rBV7	5504	13960	1.76%	0.236%
44	7.306	1012	1020	1039	rBV	159887	353679	44.63%	5.991%
45	7.470	1045	1047	1048	rVB	486	204	0.03%	0.003%
46	7.580	1063	1065	1066	rBV2	273	249	0.03%	0.004%
47	7.775	1094	1097	1099	rBV	248	299	0.04%	0.005%
48	7.958	1124	1127	1129	rBV2	495	465	0.06%	0.008%
49	8.049	1139	1142	1143	rBV2	258	276	0.03%	0.005%
50	8.324	1181	1187	1200	rBV	99204	169382	21.37%	2.869%
51	8.519	1217	1219	1220	rVB2	506	276	0.03%	0.005%
52	8.647	1234	1240	1257	rBV	403710	643280	81.18%	10.896%
53	8.952	1284	1290	1306	rBV	71108	111758	14.10%	1.893%
54	9.195	1328	1330	1332	rBV	540	277	0.03%	0.005%
55	9.384	1356	1361	1372	rBV	197480	315911	39.87%	5.351%
56	9.598	1394	1396	1399	rBV2	580	556	0.07%	0.009%
57	9.726	1413	1417	1419	rBV3	411	490	0.06%	0.008%
58	9.817	1431	1432	1434	rBV	337	279	0.04%	0.005%
59	9.872	1440	1441	1444	rBV	396	401	0.05%	0.007%
60	9.970	1454	1457	1460	rBV3	343	425	0.05%	0.007%
61	10.055	1465	1471	1483	rBV	380776	551633	69.61%	9.344%
62	10.262	1504	1505	1506	rBV	416	257	0.03%	0.004%
63	10.293	1509	1510	1514	rVV2	501	673	0.08%	0.011%
64	10.604	1558	1561	1563	rBV2	283	312	0.04%	0.005%
65	10.701	1575	1577	1579	rVB	409	336	0.04%	0.006%
66	10.726	1579	1581	1583	rBV2	229	225	0.03%	0.004%
67	10.829	1596	1598	1600	rBV	342	306	0.04%	0.005%
68	10.884	1606	1607	1610	rBV2	410	377	0.05%	0.006%
69	10.957	1615	1619	1620	rVV2	278	236	0.03%	0.004%
70	11.189	1652	1657	1666	rBV	299303	389125	49.10%	6.591%
71	11.311	1675	1677	1681	rBV	989	832	0.10%	0.014%
72	11.396	1689	1691	1693	rVB2	319	239	0.03%	0.004%
73	11.421	1693	1695	1697	rVB	364	284	0.04%	0.005%
74	11.591	1720	1723	1727	rBV3	300	535	0.07%	0.009%
75	11.945	1779	1781	1784	rVV3	250	227	0.03%	0.004%
76	12.018	1788	1793	1804	rBV	373673	486398	61.38%	8.239%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
 Data File : VX043880.D
 Acq On : 15 Nov 2024 16:50
 Operator : JC/MD
 Sample : P4785-22
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 E27P3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
 Title : VOC Analysis

77	12.170	1816	1818	1819	rBV	313	225	0.03%	0.004%
78	12.317	1837	1842	1852	rBV	441161	565386	71.35%	9.577%
79	12.494	1868	1871	1872	rBV2	405	424	0.05%	0.007%
80	12.597	1885	1888	1890	rBV	237	266	0.03%	0.005%
81	12.768	1912	1916	1918	rBV2	484	528	0.07%	0.009%
82	12.805	1920	1922	1925	rBV2	299	245	0.03%	0.004%
83	12.878	1932	1934	1936	rVB2	364	234	0.03%	0.004%
84	12.914	1939	1940	1941	rVV	560	237	0.03%	0.004%
85	12.933	1941	1943	1946	rVV2	722	693	0.09%	0.012%
86	12.963	1946	1948	1953	rVB4	767	1096	0.14%	0.019%
87	13.304	2002	2004	2006	rBV	571	497	0.06%	0.008%
88	13.743	2072	2076	2079	rVB3	482	772	0.10%	0.013%
89	13.768	2079	2080	2083	rBV2	534	389	0.05%	0.007%
90	13.810	2085	2087	2091	rBV4	1538	2339	0.30%	0.040%
91	13.865	2095	2096	2097	rBV	652	405	0.05%	0.007%
92	14.152	2141	2143	2145	rBV2	769	632	0.08%	0.011%
93	15.030	2285	2287	2290	rBV3	1109	1062	0.13%	0.018%
94	15.542	2369	2371	2374	rBV2	763	718	0.09%	0.012%
95	15.591	2377	2379	2381	rBV	811	527	0.07%	0.009%
96	16.023	2449	2450	2451	rBV	1174	576	0.07%	0.010%
97	16.097	2460	2462	2463	rBV	792	371	0.05%	0.006%
98	16.383	2507	2509	2511	rBV3	1026	741	0.09%	0.013%
99	16.456	2519	2521	2523	rBV2	753	566	0.07%	0.010%
100	16.584	2541	2542	2544	rBV2	674	541	0.07%	0.009%

Sum of corrected areas: 5903724




Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043880.D
Acq On : 15 Nov 2024 16:50
Operator : JC/MD
Sample : P4785-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

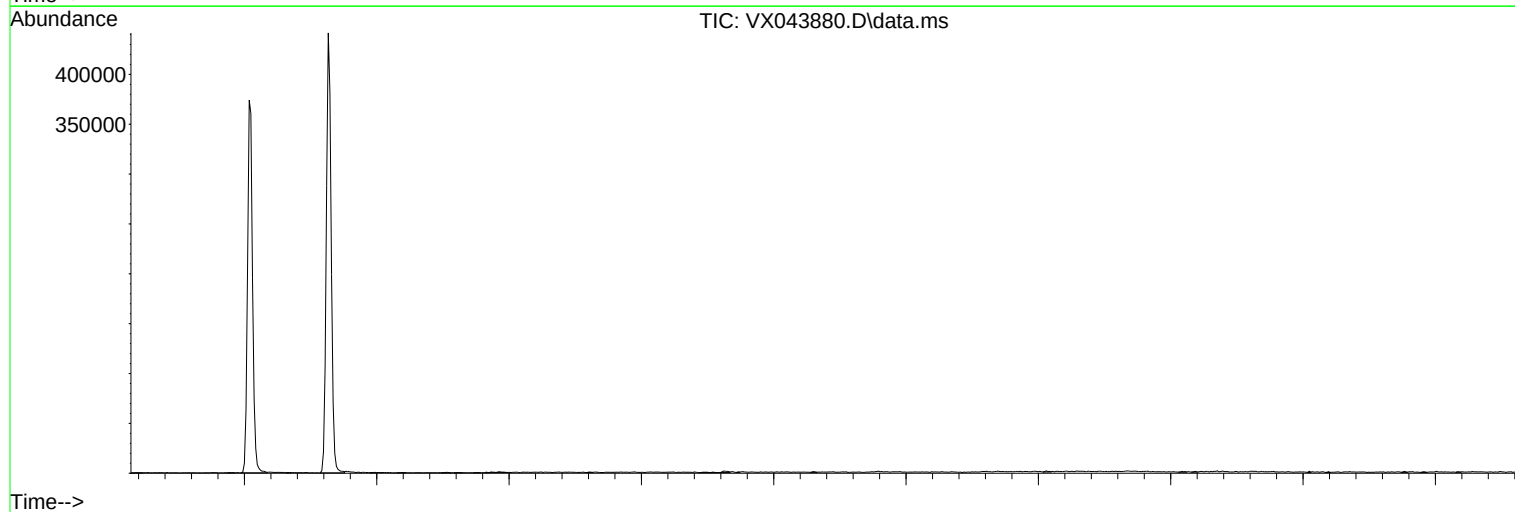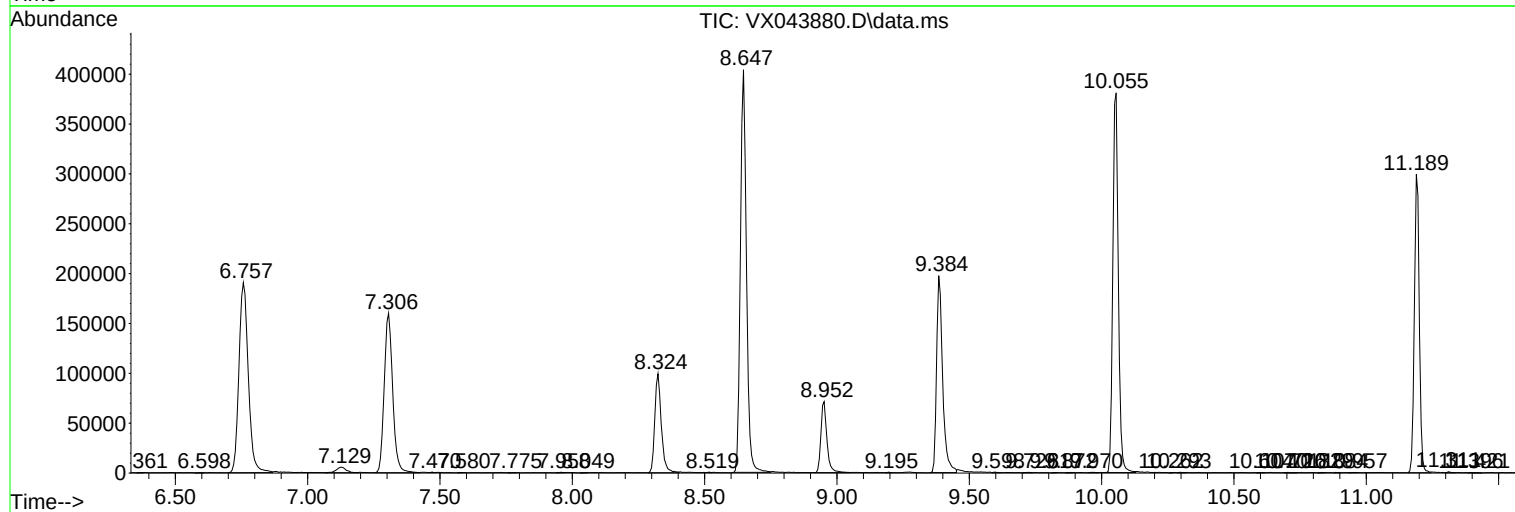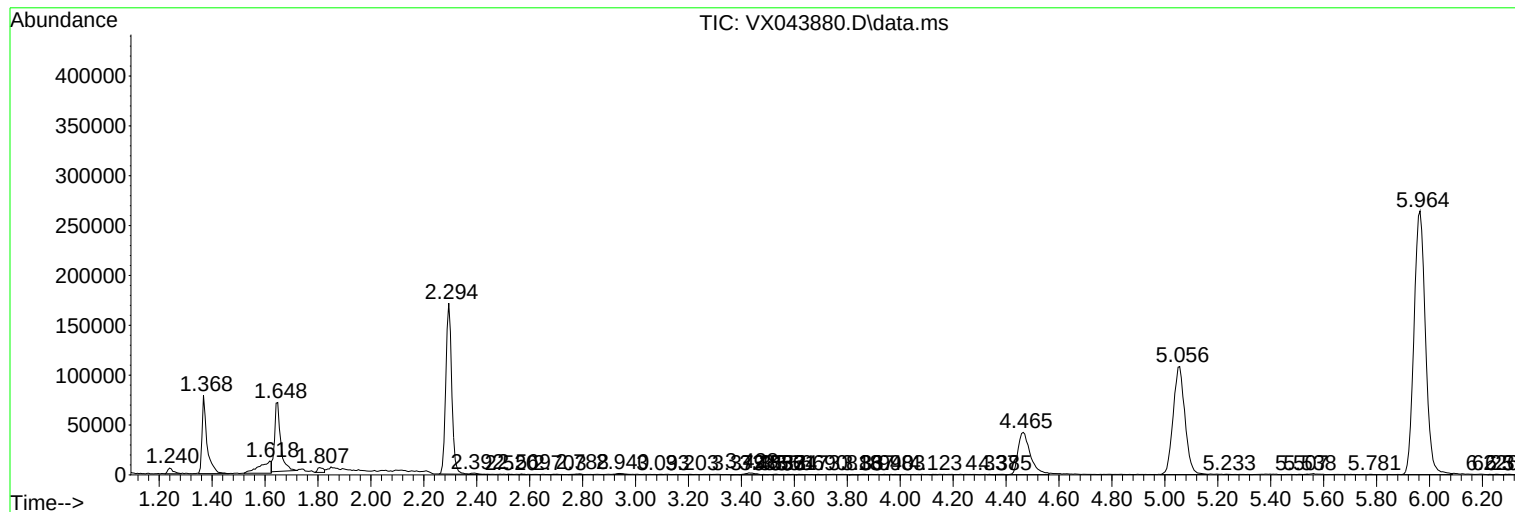

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043880.D
Acq On : 15 Nov 2024 16:50
Operator : JC/MD
Sample : P4785-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111524\
Data File : VX043880.D
Acq On : 15 Nov 2024 16:50
Operator : JC/MD
Sample : P4785-22
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
E27P3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\SFAMXLM111424WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc