


Data Path : Z:\voasrv\HPCHEM1\MSVOA X\Data\VX111620\
Data File : VX019429.D
Acq On : 16 Nov 2020 11:19
Operator : JC/MD
Sample : BFB04
Misc : 25.0mL/MSVOA X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB404

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM111320.M
Title : TRACE VOA SOM01.0
Last Update : Tue Nov 17 04:26:19 2020

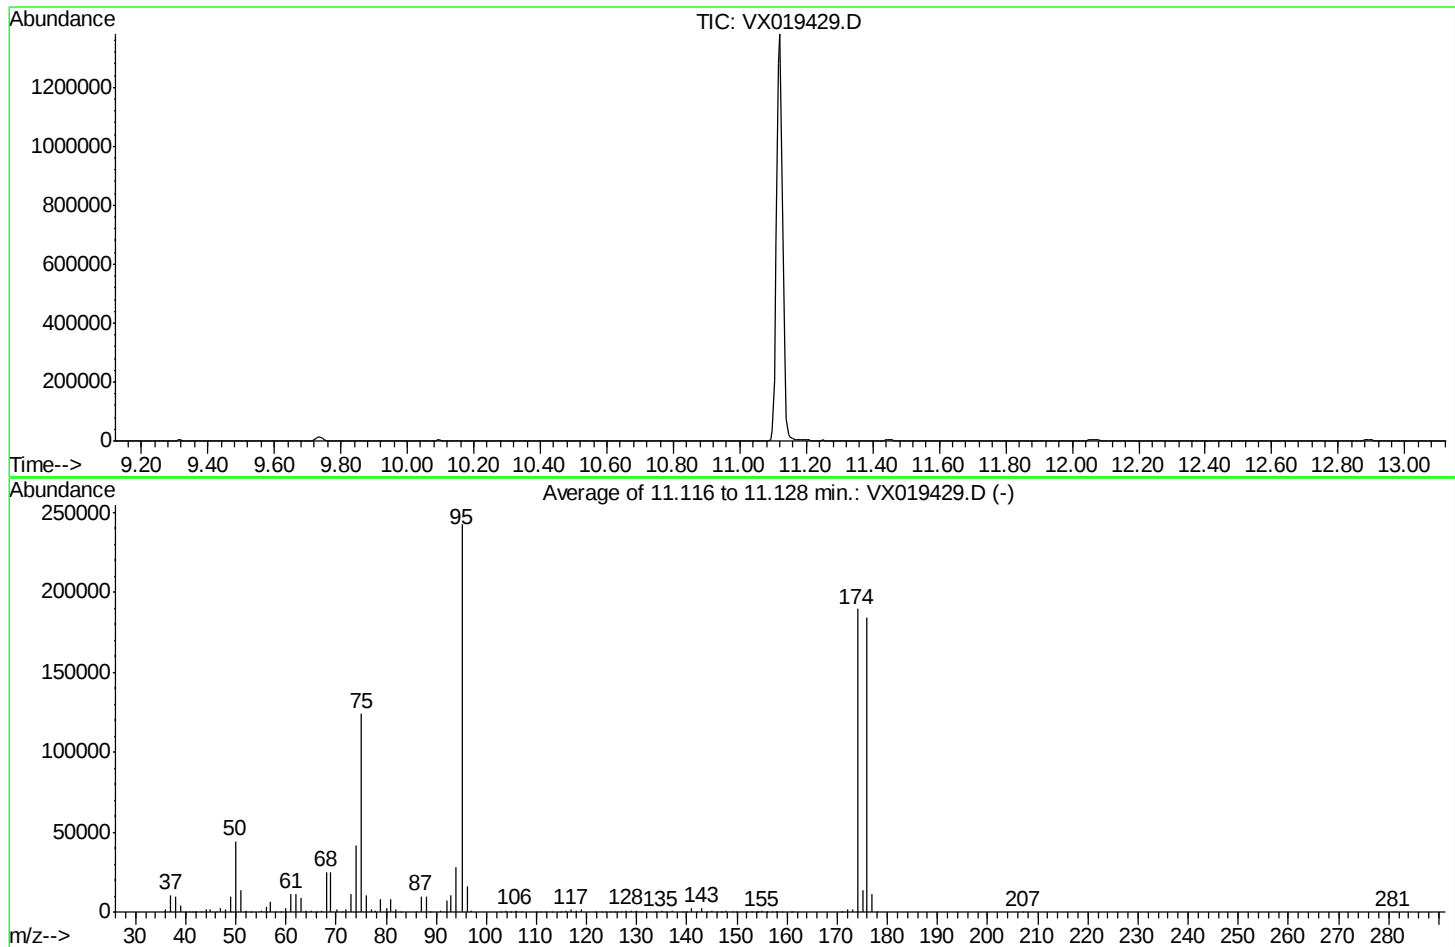

AutoFind: Scans 1645, 1646, 1647; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.2	44085	PASS
75	95	30	80	51.1	123952	PASS
95	95	100	100	100.0	242538	PASS
96	95	5	9	6.6	16087	PASS
173	174	0.00	2	0.9	1629	PASS
174	95	50	120	78.2	189546	PASS
175	174	5	9	7.2	13617	PASS
176	174	95	101	97.1	184042	PASS
177	176	5	9	6.2	11404	PASS

m/z	Abundance
36.00	2336.0
37.00	13596.0
38.00	12484.0
39.00	5169.0
40.00	478.0
40.90	109.0
41.90	101.0
43.00	213.0
44.00	2491.0
45.00	2463.0
46.10	400.0
47.10	3306.0
48.00	1689.0
49.00	11298.0
50.00	54088.0
51.10	17048.0
52.00	822.0
53.10	229.0
55.10	732.0
56.00	4256.0
57.00	7458.0
58.00	389.0
60.00	2706.0
61.00	13967.0
62.00	13242.0
63.00	10195.0
64.10	1150.0
65.00	1491.0
66.00	173.0
67.00	733.0
68.00	29944.0
69.00	29264.0
70.10	2243.0
71.10	103.0
72.00	1544.0
73.00	12552.0
74.00	48800.0
75.10	145408.0
76.10	12591.0
77.00	2078.0
78.00	997.0
78.90	9333.0
80.00	3062.0
80.90	9443.0
82.00	2083.0
83.00	279.0
85.90	435.0
87.00	11719.0
88.00	11206.0
90.90	1149.0
92.00	8080.0
93.00	11977.0
94.00	31848.0
95.10	275264.0
96.10	19216.0
97.10	718.0
102.80	191.0
103.90	1260.0
104.80	348.0
105.90	1258.0
106.90	259.0
109.80	222.0
110.90	226.0
111.90	274.0
113.00	199.0
115.00	306.0
115.90	980.0
117.00	1685.0
117.90	1129.0
118.90	1568.0
121.80	66.0
122.90	77.0
123.90	155.0
124.80	109.0
126.00	146.0
127.00	51.0
127.90	941.0
129.00	500.0
129.90	940.0
130.90	467.0
134.90	419.0
135.90	65.0
136.90	555.0
139.00	65.0
139.80	160.0
141.00	2615.0
143.00	3009.0
144.00	147.0
144.90	415.0
145.80	368.0
147.10	139.0
147.90	747.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404

148.90	140.0
149.90	256.0
151.90	120.0
152.90	124.0
154.10	120.0
155.00	672.0
155.90	164.0
157.00	427.0
157.80	89.0
158.90	278.0
160.80	233.0
171.10	132.0
172.00	1468.0
173.00	1513.0
174.00	182592.0
175.00	14196.0
176.00	177344.0
177.00	11660.0
178.00	317.0
207.10	79.0
280.90	62.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404

m/z	Abundance
36.00	2086.0
37.10	12285.0
38.10	11119.0
39.00	4299.0
40.00	519.0
40.70	135.0
41.30	56.0
42.20	61.0
43.10	171.0
44.00	2299.0
45.00	2064.0
46.00	237.0
47.00	3184.0
48.00	1720.0
49.00	11488.0
50.00	51680.0
51.10	15562.0
52.10	775.0
53.00	147.0
54.90	759.0
56.00	4087.0
57.00	7412.0
58.00	250.0
58.90	73.0
60.00	2777.0
61.00	13074.0
62.00	13097.0
63.00	10595.0
64.00	1166.0
65.10	1110.0
66.10	162.0
67.00	678.0
68.00	28976.0
69.00	29184.0
70.10	2064.0
71.10	88.0
72.10	1428.0
73.00	13151.0
74.10	48184.0
75.00	146880.0
76.10	12293.0
77.10	1865.0
77.90	943.0
79.00	8924.0
80.00	2576.0
81.00	8942.0
82.00	1994.0
83.00	251.0
86.00	438.0
87.00	11353.0
88.00	11793.0
91.00	1058.0
92.00	7962.0
93.00	12667.0
94.00	33872.0
95.10	285760.0
96.10	18736.0
97.00	630.0
102.90	167.0
103.90	1320.0
104.90	449.0
105.90	1198.0
106.90	364.0
109.90	193.0
110.80	274.0
111.80	243.0
112.90	228.0
115.00	278.0
115.90	1112.0
116.90	1868.0
117.90	1043.0
119.00	1536.0
123.00	101.0
123.90	142.0
124.90	99.0
125.60	94.0
126.10	98.0
126.90	67.0
127.90	1062.0
128.90	641.0
129.90	1038.0
130.90	519.0
133.80	56.0
134.90	588.0
137.00	628.0
139.00	57.0
140.00	161.0
140.90	3278.0
141.90	317.0
143.00	3080.0
143.90	136.0
144.90	592.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404

145.90	411.0
146.80	252.0
148.00	706.0
149.00	211.0
150.00	300.0
151.90	140.0
152.80	163.0
153.80	168.0
154.90	649.0
156.10	224.0
156.90	434.0
158.00	157.0
159.00	355.0
161.00	297.0
170.60	117.0
172.10	1628.0
173.00	2123.0
174.00	230400.0
175.00	15884.0
176.00	222528.0
177.00	13452.0
178.00	286.0
207.20	78.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404

m/z	Abundance
36.00	1245.0
37.00	6297.0
38.00	5793.0
39.10	2202.0
40.00	357.0
40.70	55.0
42.20	51.0
42.90	70.0
44.00	1509.0
45.10	1191.0
45.90	97.0
47.10	1695.0
47.90	837.0
49.00	5922.0
50.10	26488.0
51.00	7809.0
52.00	350.0
53.10	143.0
55.00	435.0
56.10	2302.0
57.10	3671.0
57.90	133.0
60.00	1443.0
61.00	7136.0
62.10	7044.0
63.10	5798.0
64.10	630.0
65.00	742.0
66.00	77.0
67.10	460.0
68.00	16060.0
69.00	16113.0
70.00	1431.0
72.00	855.0
73.00	7274.0
74.00	27000.0
75.10	79568.0
76.10	6250.0
77.10	970.0
77.90	777.0
79.00	5076.0
80.00	1564.0
80.90	5415.0
82.00	1177.0
83.00	219.0
86.00	277.0
87.00	6747.0
88.00	6563.0
88.90	67.0
91.00	662.0
92.00	5021.0
93.00	6774.0
94.00	19584.0
95.00	166592.0
96.10	10309.0
97.10	304.0
102.90	120.0
103.90	644.0
104.90	230.0
105.90	887.0
106.90	162.0
110.00	101.0
110.90	211.0
111.90	167.0
112.90	164.0
114.80	164.0
115.90	705.0
117.00	1105.0
117.90	557.0
118.90	1128.0
121.90	70.0
123.90	146.0
124.90	61.0
126.90	147.0
128.00	739.0
128.90	380.0
129.90	596.0
130.90	248.0
135.00	433.0
136.90	369.0
139.90	120.0
141.00	1891.0
141.80	230.0
142.90	1907.0
144.10	133.0
145.00	320.0
146.00	230.0
146.90	115.0
147.80	370.0
148.90	141.0
150.00	197.0
151.80	77.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404

153.00	131.0
154.00	133.0
155.00	391.0
156.00	144.0
157.10	327.0
158.10	134.0
159.00	277.0
160.80	184.0
170.70	63.0
172.00	1000.0
173.00	1253.0
174.00	155648.0
175.10	10773.0
176.00	152256.0
177.00	9102.0
178.10	179.0
207.00	95.0
281.30	53.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404

Scan 1637 (11.067 min): VX019429.D
BFB04

m/z	Abundance
38.90	59.0
40.10	367.0
44.00	659.0

Instrument :
MSVOA_X
ClientSampleId :
BFB404