

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111622\
 Data File : VX032866.D
 Acq On : 16 Nov 2022 14:28
 Operator : JC/MD
 Sample : N5614-01DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

Signal : TIC: VX032866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.368	41	46	53	rBV	12431	13992	1.44%	0.172%
2	1.746	104	108	116	rVB	27830	38982	4.01%	0.480%
3	2.337	200	205	213	rBV2	5555	10062	1.03%	0.124%
4	2.782	268	278	282	rBV4	13182	31158	3.20%	0.384%
5	2.825	282	285	290	rVB	9962	17012	1.75%	0.209%
6	3.105	322	331	341	rVB2	27197	62338	6.41%	0.768%
7	3.751	427	437	446	rBV3	8392	29481	3.03%	0.363%
8	4.215	505	513	520	rBV4	5335	15894	1.63%	0.196%
9	4.306	520	528	538	rVB2	14853	42644	4.38%	0.525%
10	5.202	666	675	684	rVB4	4419	14346	1.47%	0.177%
11	5.385	694	705	716	rBV	64046	190104	19.54%	2.341%
12	5.550	722	732	741	rBV	96781	267105	27.45%	3.289%
13	5.824	768	777	789	rVB5	10044	31413	3.23%	0.387%
14	5.958	789	799	805	rBV	69903	183792	18.89%	2.263%
15	6.038	805	812	825	rVV	159971	432426	44.44%	5.324%
16	6.159	825	832	839	rVV6	11526	38191	3.92%	0.470%
17	6.251	839	847	857	rVV2	26713	85495	8.79%	1.053%
18	6.361	857	865	874	rVB4	9117	26163	2.69%	0.322%
19	6.763	921	931	942	rBV	161907	396357	40.73%	4.880%
20	6.848	942	945	960	rVB5	7799	19610	2.02%	0.241%
21	7.171	991	998	1006	rBV3	13009	27729	2.85%	0.341%
22	7.367	1020	1030	1040	rVB5	12932	37559	3.86%	0.462%
23	7.885	1104	1115	1123	rBV8	5853	21183	2.18%	0.261%
24	7.982	1123	1131	1141	rVB2	17187	40138	4.12%	0.494%
25	8.104	1143	1151	1156	rBV	31332	68217	7.01%	0.840%
26	8.141	1156	1157	1162	rVV2	14530	16988	1.75%	0.209%
27	8.190	1162	1165	1175	rVV5	5890	12171	1.25%	0.150%
28	8.312	1178	1185	1190	rBV5	6878	14034	1.44%	0.173%
29	8.507	1212	1217	1225	rVB2	20759	37638	3.87%	0.463%
30	8.604	1225	1233	1235	rBV3	10539	19239	1.98%	0.237%
31	8.647	1235	1240	1249	rVB	356679	552308	56.76%	6.800%
32	8.921	1278	1285	1290	rVV5	5317	10233	1.05%	0.126%
33	9.104	1307	1315	1320	rBV	11185	22030	2.26%	0.271%
34	9.165	1320	1325	1335	rVB	29809	51648	5.31%	0.636%
35	9.427	1364	1368	1370	rBV2	8235	11756	1.21%	0.145%
36	9.458	1370	1373	1377	rVV	19008	28736	2.95%	0.354%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111622\
 Data File : VX032866.D
 Acq On : 16 Nov 2022 14:28
 Operator : JC/MD
 Sample : N5614-01DL 5X
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW-14DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Title : SW846 8260

37	9.500	1377	1380	1387	rVB4	11848	21022	2.16%	0.259%
38	9.762	1415	1423	1431	rBV4	9083	16427	1.69%	0.202%
39	10.055	1466	1471	1476	rBV	336307	441226	45.34%	5.433%
40	10.195	1489	1494	1502	rVB	170072	223974	23.02%	2.758%
41	10.305	1508	1512	1518	rVB	31466	44487	4.57%	0.548%
42	10.586	1548	1558	1562	rBV5	5606	10227	1.05%	0.126%
43	10.963	1615	1620	1626	rBV	76270	95727	9.84%	1.179%
44	11.079	1634	1639	1645	rBV	322368	408587	41.99%	5.031%
45	11.305	1671	1676	1685	rVB	61776	78001	8.02%	0.960%
46	11.402	1685	1692	1696	rBV	17363	25006	2.57%	0.308%
47	11.610	1719	1726	1735	rBV	35591	49017	5.04%	0.604%
48	11.866	1763	1768	1770	rBV	9828	13430	1.38%	0.165%
49	11.890	1770	1772	1778	rVB	13681	15508	1.59%	0.191%
50	12.024	1788	1794	1802	rBV	338431	443884	45.62%	5.465%
51	12.244	1824	1830	1837	rVV2	785195	973104	100.00%	11.981%
52	12.311	1837	1841	1852	rVB2	61431	89164	9.16%	1.098%
53	12.408	1852	1857	1862	rVB2	32075	41939	4.31%	0.516%
54	12.463	1862	1866	1873	rVB2	10237	14876	1.53%	0.183%
55	12.530	1873	1877	1884	rBV2	8350	11152	1.15%	0.137%
56	12.616	1884	1891	1893	rBV	43795	56775	5.83%	0.699%
57	12.646	1893	1896	1900	rVB	67795	78302	8.05%	0.964%
58	12.701	1900	1905	1912	rBV	253857	346718	35.63%	4.269%
59	12.841	1924	1928	1933	rVB2	9287	12379	1.27%	0.152%
60	12.920	1933	1941	1946	rBV	94501	118086	12.13%	1.454%
61	13.024	1953	1958	1967	rBV2	21787	33204	3.41%	0.409%
62	13.134	1967	1976	1978	rBV3	16187	29923	3.08%	0.368%
63	13.170	1978	1982	1991	rVB	139678	172015	17.68%	2.118%
64	13.292	1997	2002	2007	rVV	365617	446922	45.93%	5.503%
65	13.341	2007	2010	2014	rVB3	15148	18418	1.89%	0.227%
66	13.426	2020	2024	2029	rVB	39899	53668	5.52%	0.661%
67	13.506	2032	2037	2039	rBV2	16724	22126	2.27%	0.272%
68	13.542	2039	2043	2046	rVV	59721	82350	8.46%	1.014%
69	13.585	2046	2050	2054	rVV3	44795	71585	7.36%	0.881%
70	13.640	2054	2059	2060	rVV2	30532	41984	4.31%	0.517%
71	13.664	2060	2063	2069	rVB2	51780	79241	8.14%	0.976%
72	13.774	2074	2081	2089	rVV	142428	185349	19.05%	2.282%
73	13.853	2091	2094	2099	rVB2	7744	9754	1.00%	0.120%
74	13.926	2099	2106	2110	rBV2	26282	37690	3.87%	0.464%
75	13.969	2110	2113	2117	rVB	23503	25841	2.66%	0.318%
76	14.079	2126	2131	2136	rBV	44867	58561	6.02%	0.721%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111622\
Data File : VX032866.D
Acq On : 16 Nov 2022 14:28
Operator : JC/MD
Sample : N5614-01DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14DL

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

77	14.219	2148	2154	2164	rBV3	20258	38336	3.94%	0.472%
78	14.323	2167	2171	2175	rVV	20950	30573	3.14%	0.376%
79	14.371	2175	2179	2184	rVB	30775	37849	3.89%	0.466%
80	14.481	2192	2197	2201	rBV2	9417	12905	1.33%	0.159%
81	14.609	2211	2218	2220	rBV3	6233	12473	1.28%	0.154%
82	14.640	2220	2223	2227	rVB	20186	25088	2.58%	0.309%
83	14.780	2241	2246	2251	rBV	37576	48837	5.02%	0.601%




Sum of corrected areas: 8121882

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111622\
Data File : VX032866.D
Acq On : 16 Nov 2022 14:28
Operator : JC/MD
Sample : N5614-01DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

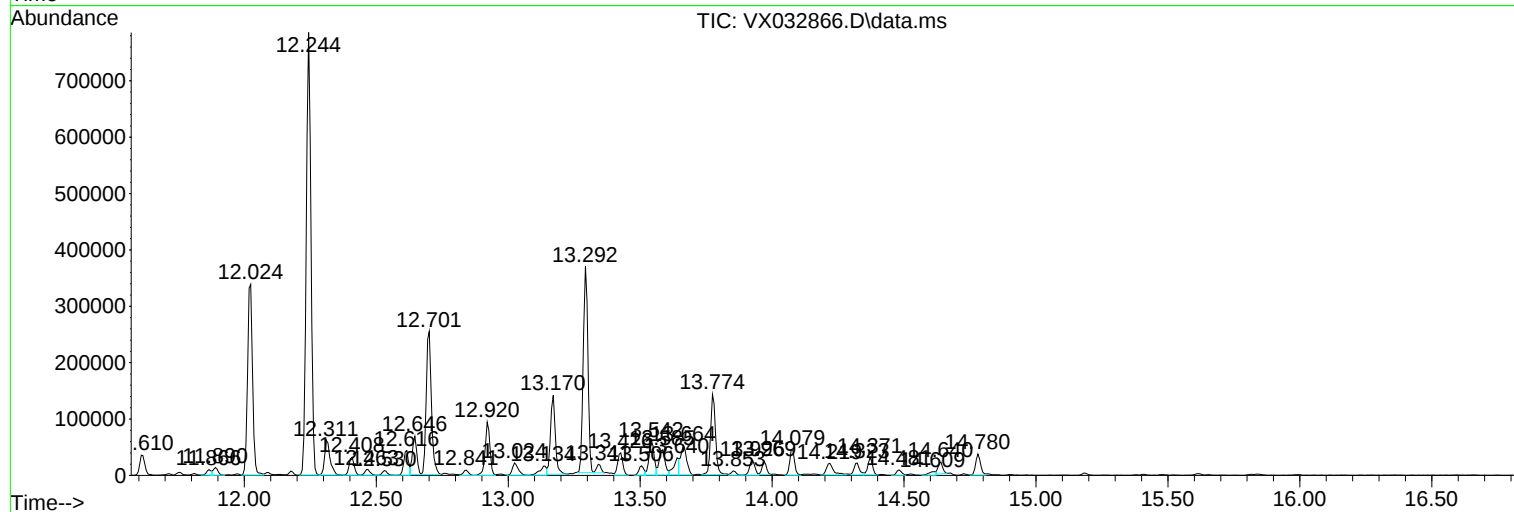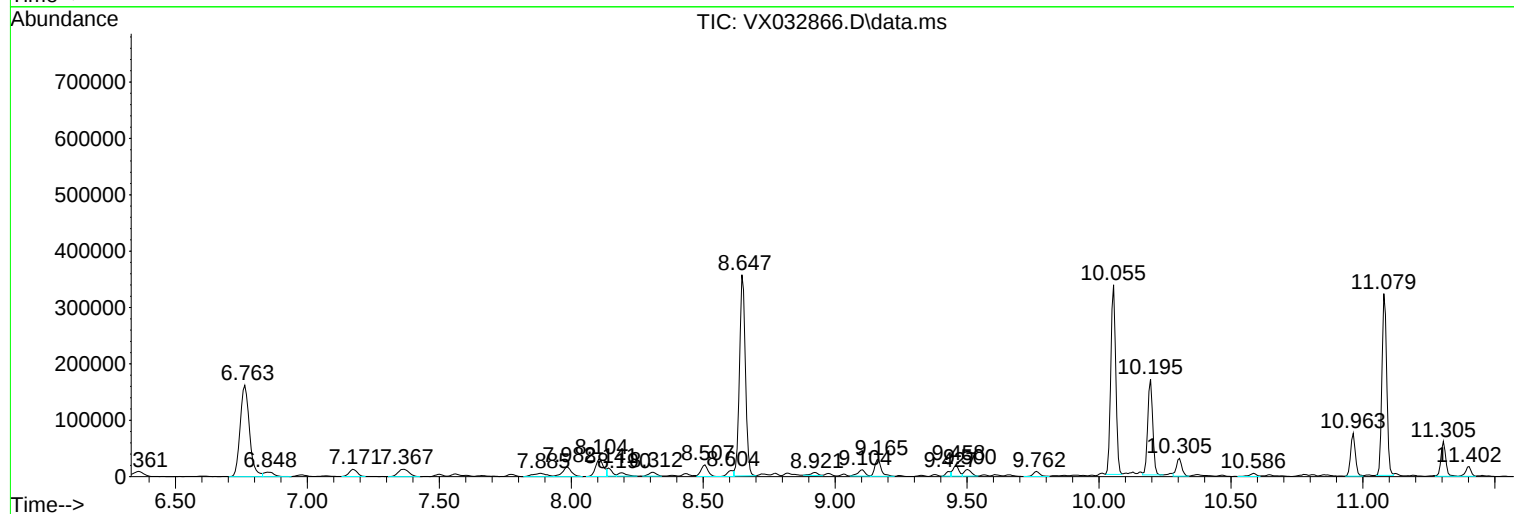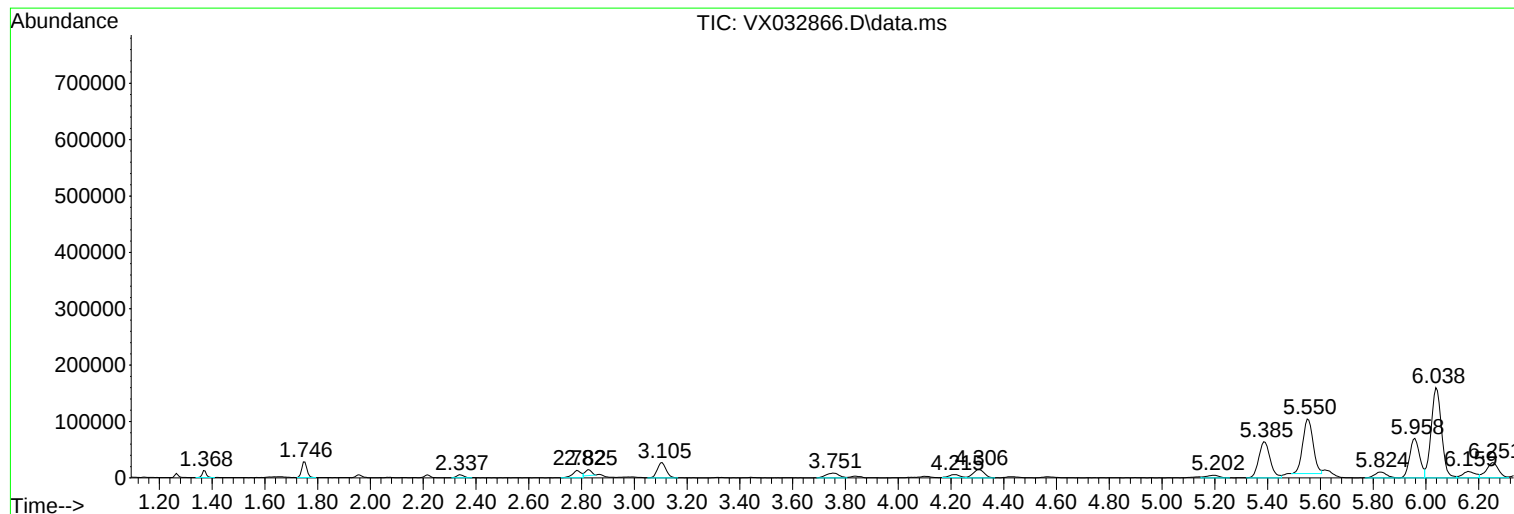

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111622\
Data File : VX032866.D
Acq On : 16 Nov 2022 14:28
Operator : JC/MD
Sample : N5614-01DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111622\
Data File : VX032866.D
Acq On : 16 Nov 2022 14:28
Operator : JC/MD
Sample : N5614-01DL 5X
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW-14DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------