

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111623\
 Data File : VX038856.D
 Acq On : 16 Nov 2023 22:27
 Operator : JC/MD
 Sample : 05357-08
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 BPOW1-8-20231108

Quant Time: Nov 17 03:21:26 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
 Quant Title : SW846 8260
 QLast Update : Thu Nov 16 22:59:22 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.550	168	132788	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	272401	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	280020	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	142803	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	96859	45.268	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	90.540%
35) Dibromofluoromethane	5.385	113	86646	44.042	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	88.080%
50) Toluene-d8	8.647	98	345808	45.941	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.880%#
62) 4-Bromofluorobenzene	11.079	95	149522	49.623	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	99.240%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111623\
Data File : VX038856.D
Acq On : 16 Nov 2023 22:27
Operator : JC/MD
Sample : 05357-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20231108

Quant Time: Nov 17 03:21:26 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260
QLast Update : Thu Nov 16 22:59:22 2023
Response via : Initial Calibration




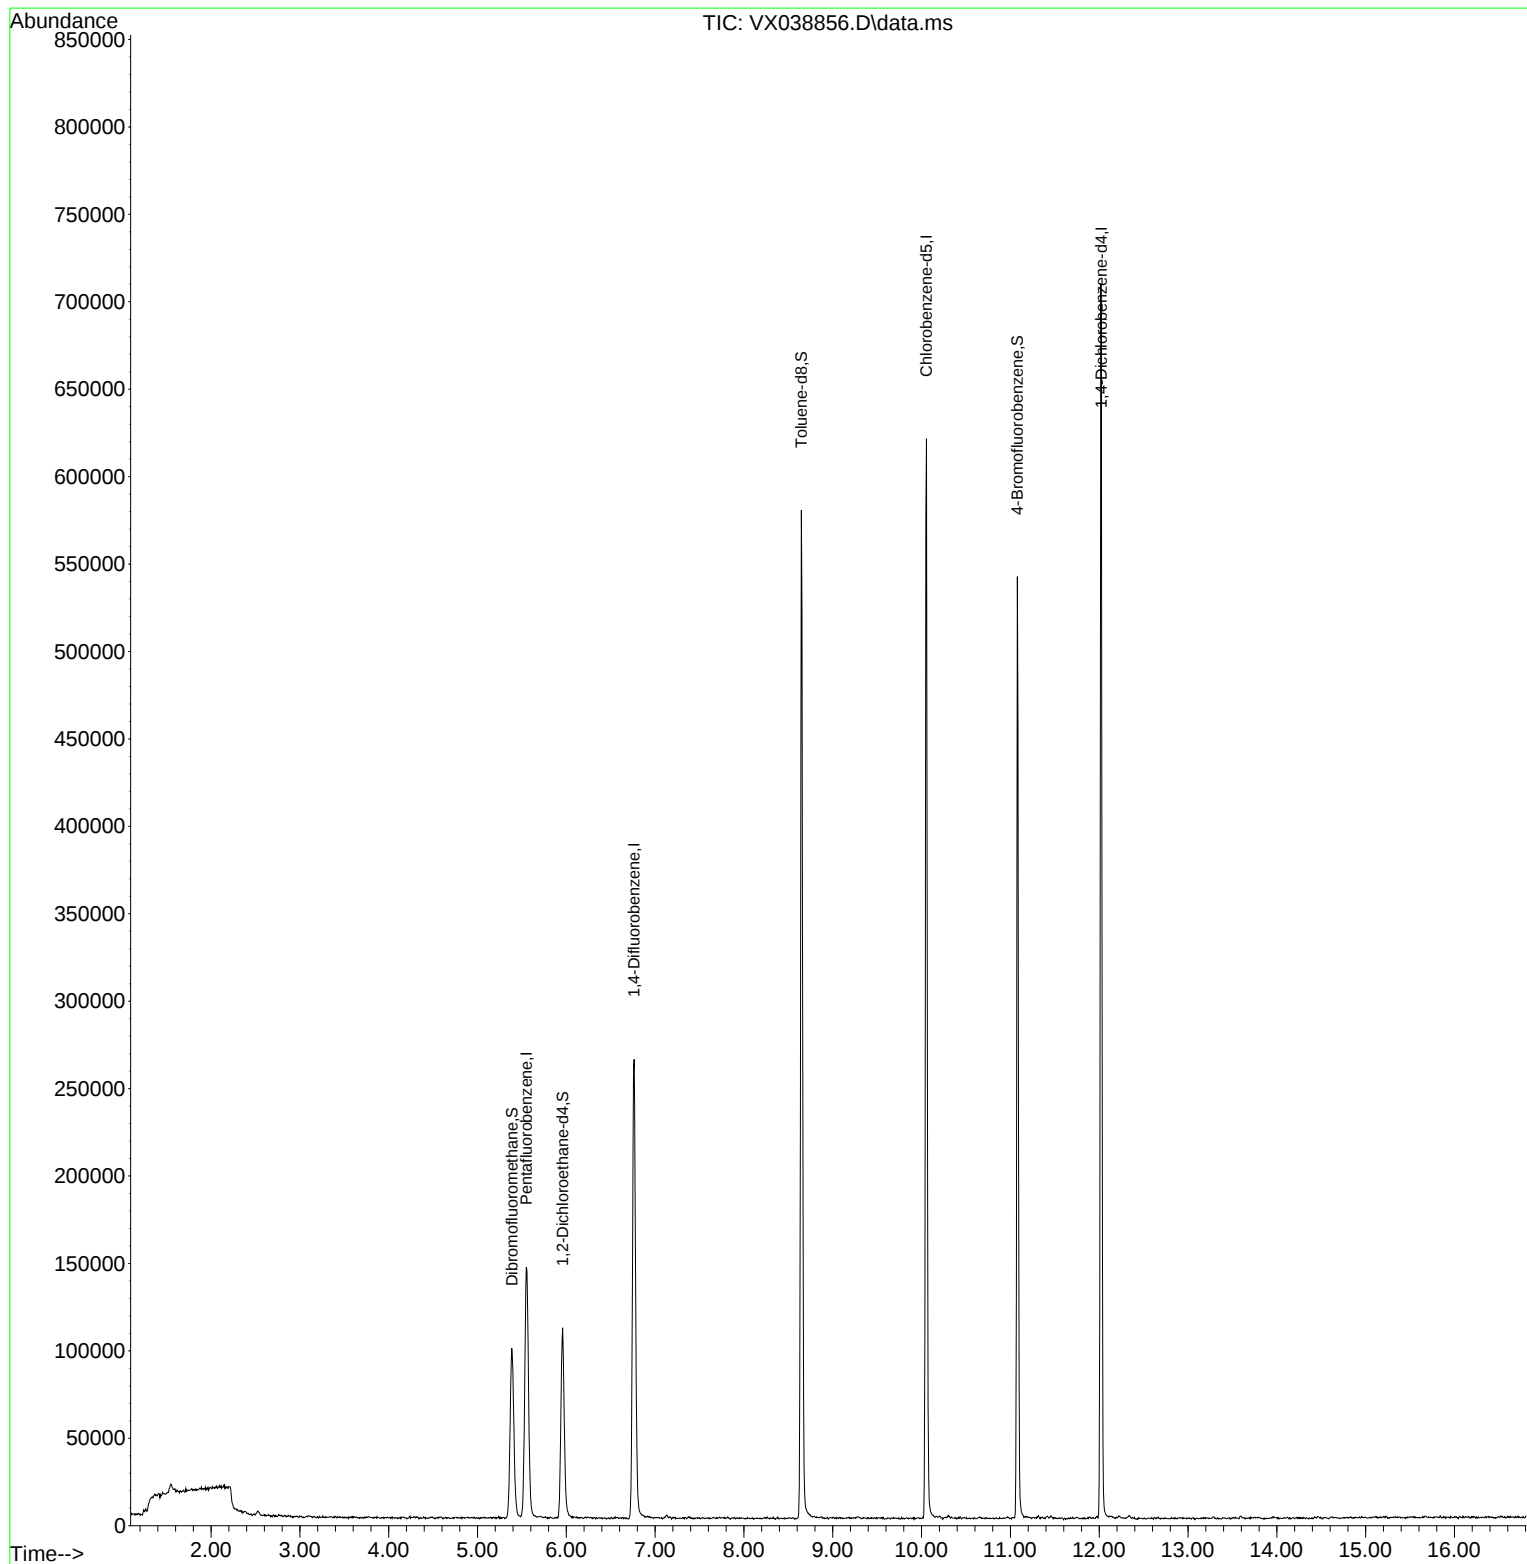




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.550 min Scan# 711
Delta R.T. -0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27




Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20231108


Tgt Ion:168 Resp: 132788
Ion Ratio Lower Upper
168 100
99 64.6 56.6 85.0

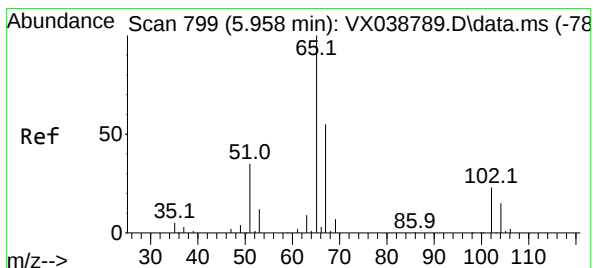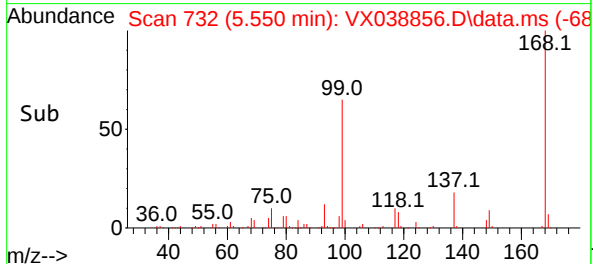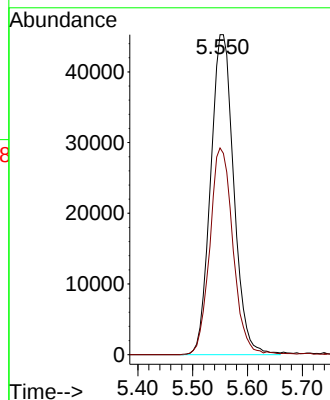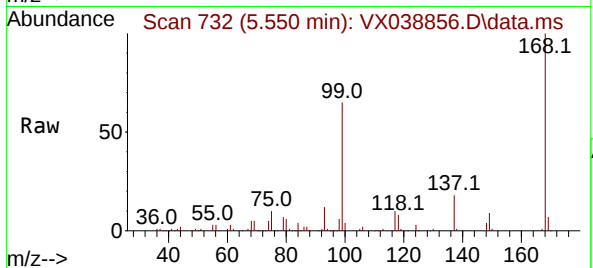

#33
1,2-Dichloroethane-d4
Concen: 45.268 ug/l
RT: 5.958 min Scan# 799
Delta R.T. 0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27

Tgt Ion: 65 Resp: 96859
Ion Ratio Lower Upper
65 100
67 56.5 0.0 100.2


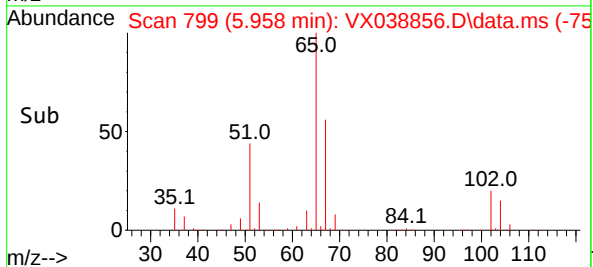
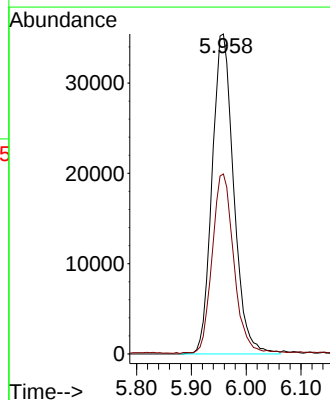
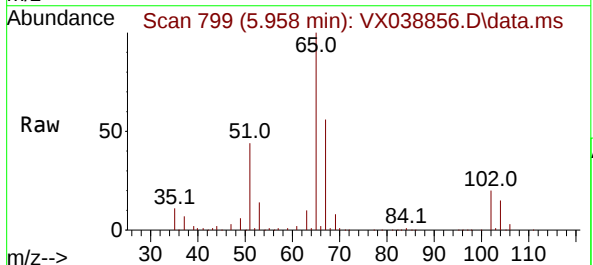


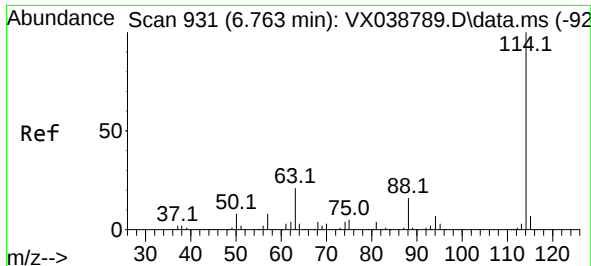

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27




Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20231108


Tgt Ion:114 Resp: 272401
Ion Ratio Lower Upper
114 100
63 20.9 0.0 45.0
88 16.5 0.0 36.6

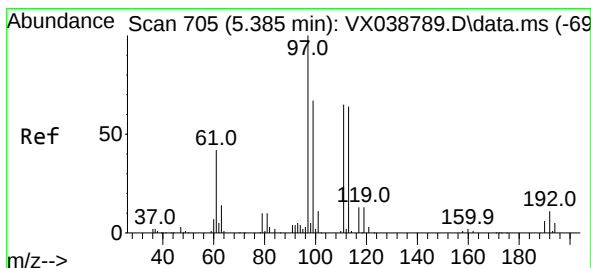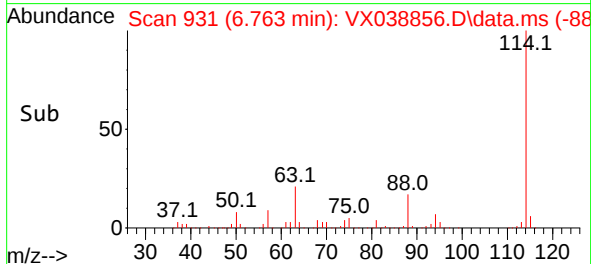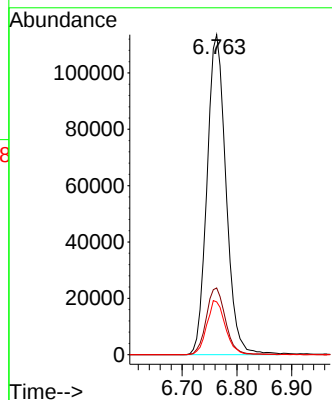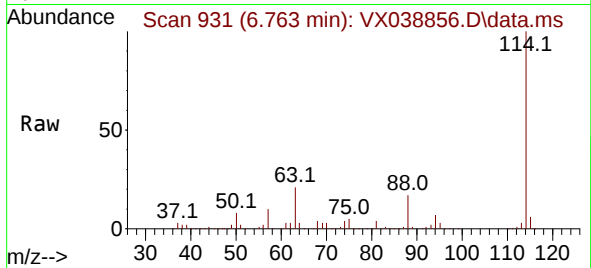

#35
Dibromofluoromethane
Concen: 44.042 ug/l
RT: 5.385 min Scan# 705
Delta R.T. 0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27

Tgt Ion:113 Resp: 86646
Ion Ratio Lower Upper
113 100
111 104.7 82.9 124.3
192 15.9 13.3 19.9


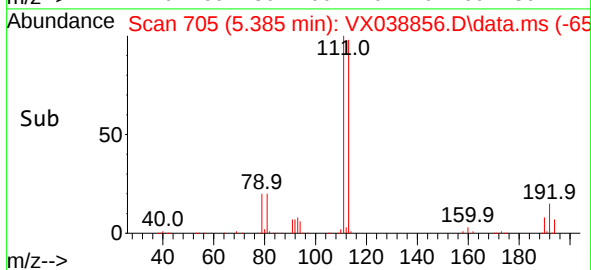
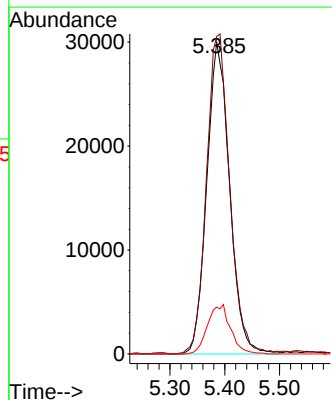
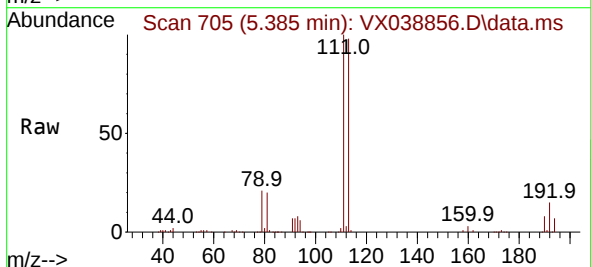


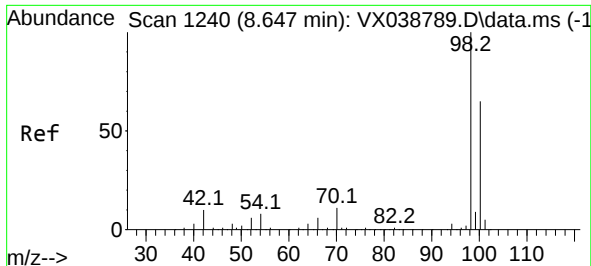

#50
Toluene-d8
Concen: 45.941 ug/l
RT: 8.647 min Scan# 11
Delta R.T. 0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27




Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20231108


Tgt Ion: 98 Resp: 345808
Ion Ratio Lower Upper
98 100
100 63.8 53.1 79.7

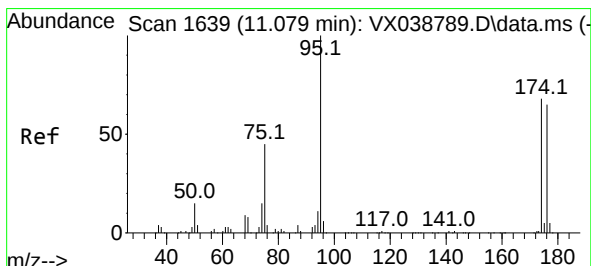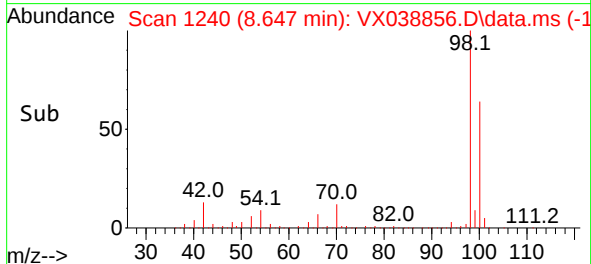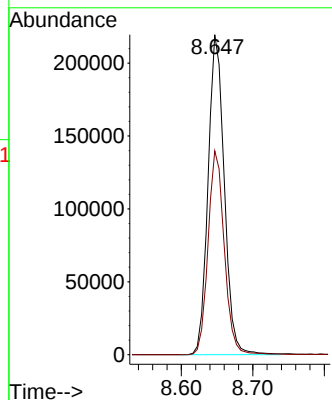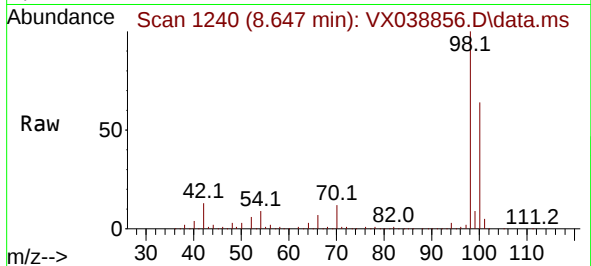

#62
4-Bromofluorobenzene
Concen: 49.623 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27

Tgt Ion: 95 Resp: 149522
Ion Ratio Lower Upper
95 100
174 67.1 0.0 135.6
176 64.3 0.0 131.0


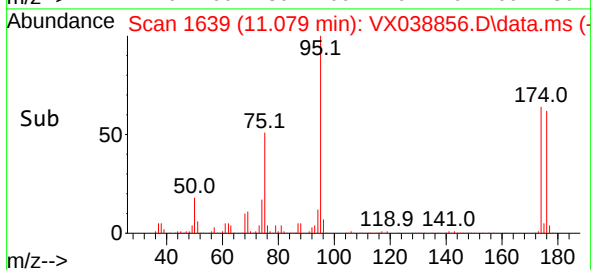
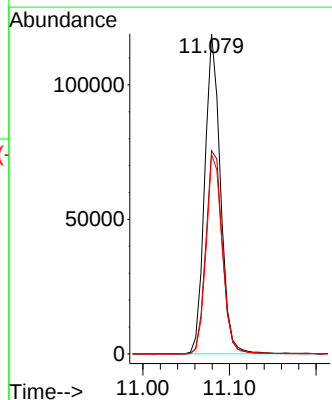
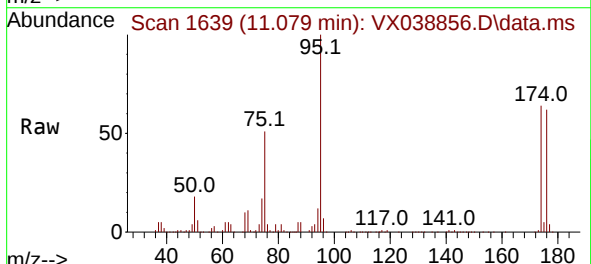


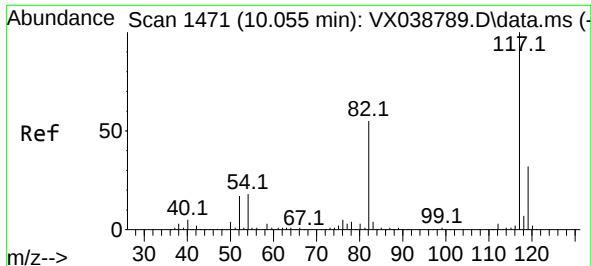

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27

Instrument :
MSVOA_X
ClientSampleId :
BPOW1-8-20231108

Tgt Ion:117 Resp: 280020
Ion Ratio Lower Upper
117 100
82 57.0 46.2 69.4
119 31.6 25.5 38.3

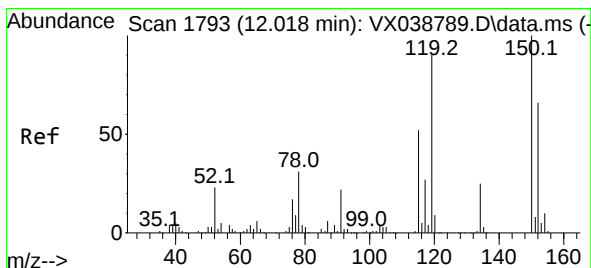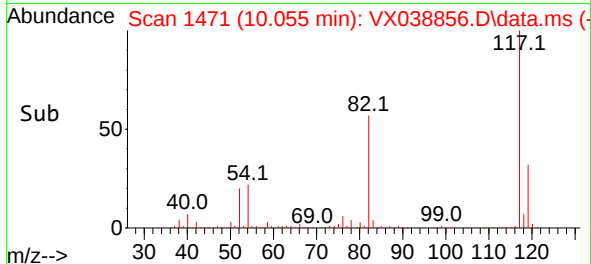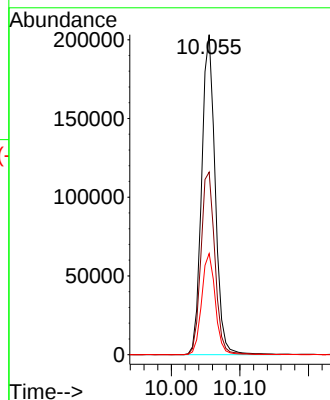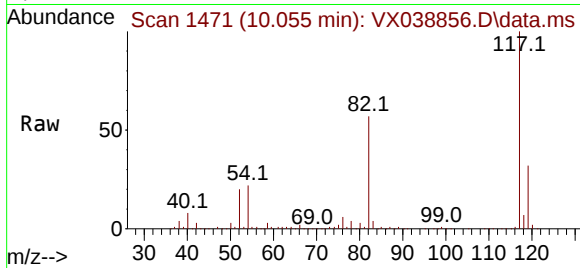

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. 0.006 min
Lab File: VX038856.D
Acq: 16 Nov 2023 22:27

Tgt Ion:152 Resp: 142803
Ion Ratio Lower Upper
152 100
115 65.0 43.3 129.9
150 159.3 0.0 345.0

