

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111623\
 Data File : VX038863.D
 Acq On : 17 Nov 2023 01:09
 Operator : JC/MD
 Sample : 05241-14
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 FSND-EVAL-01S-20231102

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M

Title : SW846 8260

Signal : TIC: VX038863.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.331	32	40	41	rBV7	6108	14897	1.26%	0.225%
2	2.526	229	236	247	rBV	340466	599561	50.89%	9.040%
3	5.385	694	705	718	rBV	95153	279738	23.74%	4.218%
4	5.550	721	732	747	rVB	137700	399154	33.88%	6.018%
5	5.958	789	799	815	rBV	105074	289577	24.58%	4.366%
6	6.763	921	931	949	rBV	257420	624002	52.97%	9.408%
7	7.123	982	990	1006	rBV	540282	1178118	100.00%	17.762%
8	8.647	1233	1240	1258	rBV	557214	879990	74.69%	13.268%
9	10.055	1465	1471	1485	rBV	593091	834400	70.82%	12.580%
10	11.079	1634	1639	1652	rBV	505217	653758	55.49%	9.857%
11	12.018	1788	1793	1804	rBV	667576	879419	74.65%	13.259%




Sum of corrected areas: 6632614

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111623\
Data File : VX038863.D
Acq On : 17 Nov 2023 01:09
Operator : JC/MD
Sample : 05241-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-EVAL-01S-20231102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

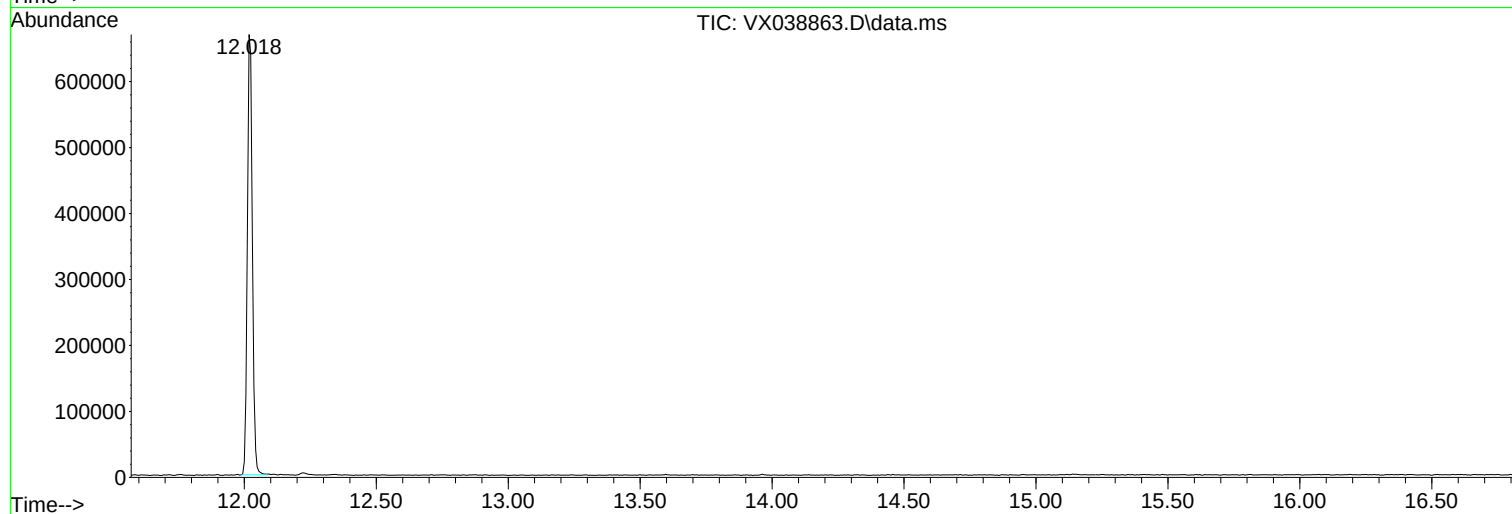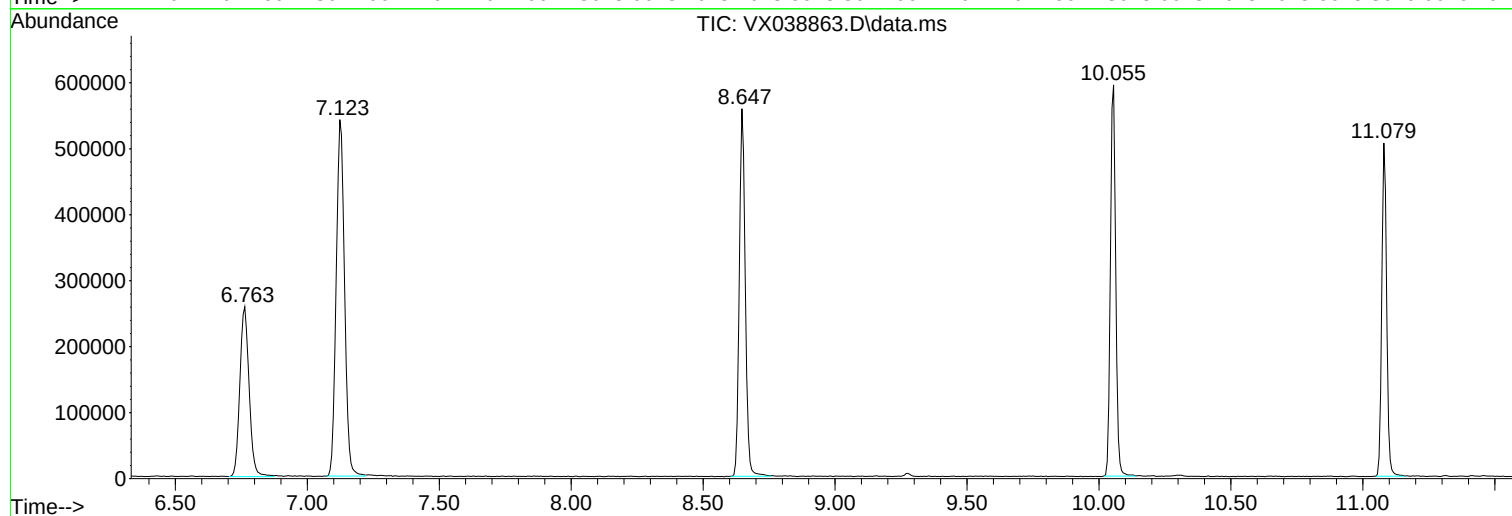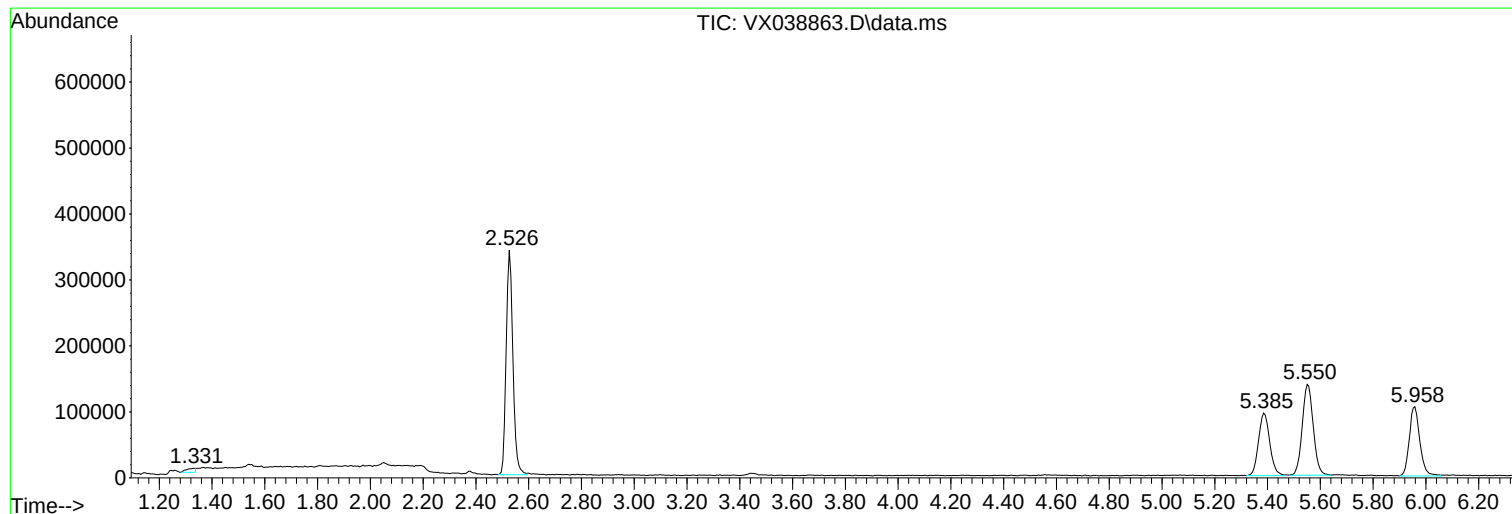

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111623\
Data File : VX038863.D
Acq On : 17 Nov 2023 01:09
Operator : JC/MD
Sample : 05241-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-EVAL-01S-20231102










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.526	75.10 ug/l	599561	Pentafluorobenzene	5.556

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
2			4-Penten-2-ol	86	C5H10O	000625-31-0	9
3			Hydrazine, ethyl-	60	C2H8N2	000624-80-6	9
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			Propanoic acid, 2-hydroxy-, meth...	104	C4H8O3	000547-64-8	9

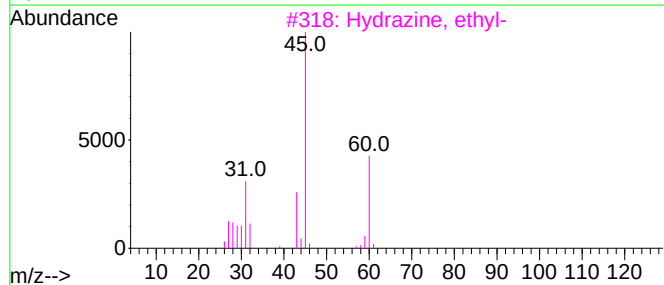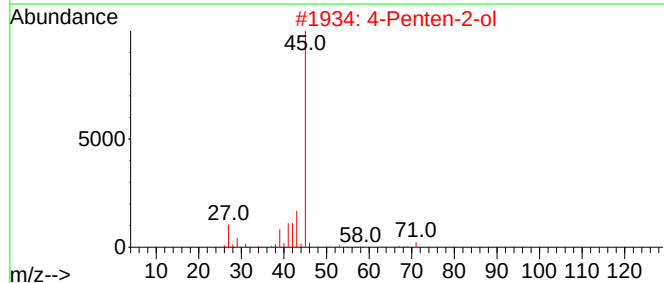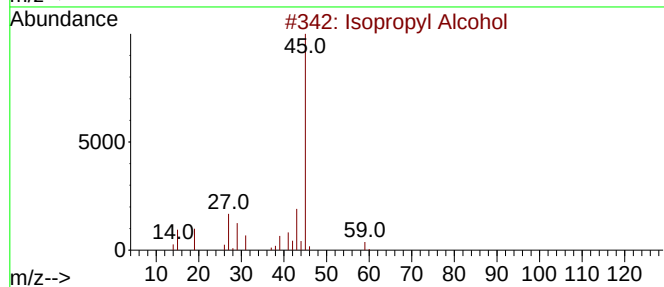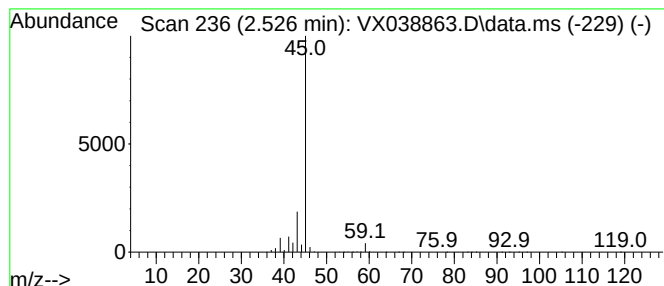

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111623\
Data File : VX038863.D
Acq On : 17 Nov 2023 01:09
Operator : JC/MD
Sample : 05241-14
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
FSND-EVAL-01S-20231102

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.526	75.1	ug/l	599561	1	5.556	399154	50.0