


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111721\
Data File : VX025179.D
Acq On : 17 Nov 2021 09:37
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111721W.M
Title : SW846 8260
Last Update : Wed Nov 17 15:36:16 2021

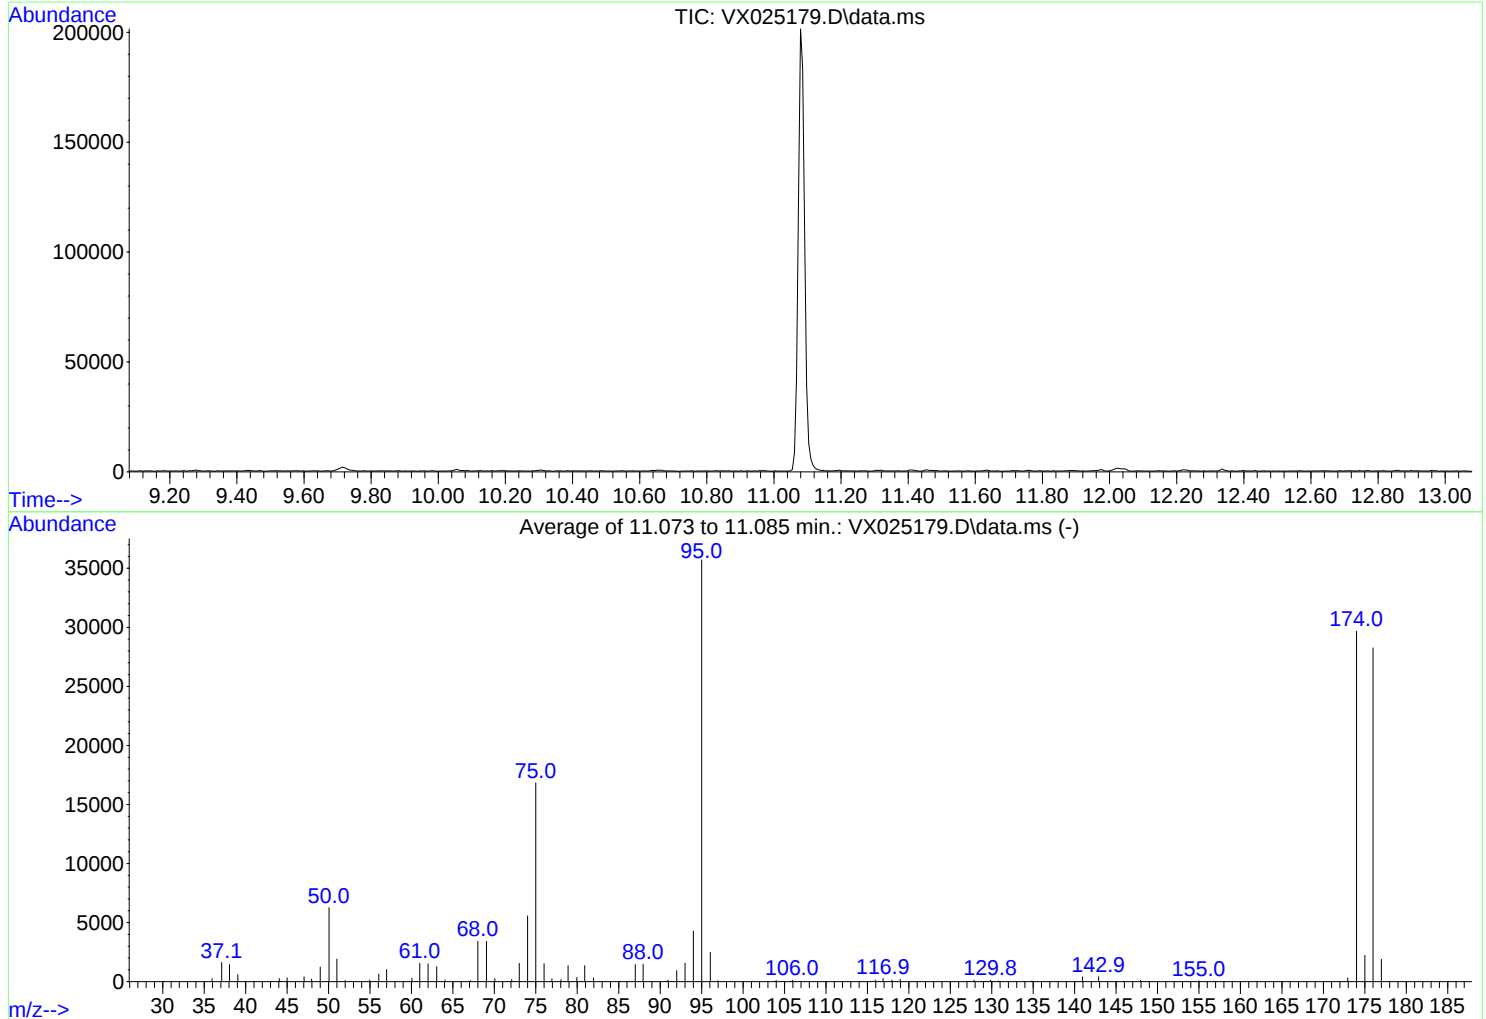

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.5	6267	PASS
75	95	30	60	47.1	16831	PASS
95	95	100	100	100.0	35712	PASS
96	95	5	9	7.0	2483	PASS
173	174	0.00	2	1.1	314	PASS
174	95	50	100	83.1	29669	PASS
175	174	5	9	7.5	2229	PASS
176	174	95	101	95.3	28264	PASS
177	176	5	9	6.7	1880	PASS