

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
 Data File : VX032900.D
 Acq On : 17 Nov 2022 15:16
 Operator : JC/MD
 Sample : N5671-05
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 MW178S-20221115

Quant Time: Nov 18 01:41:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
 Quant Title : SW846 8260
 QLast Update : Thu Oct 27 08:28:06 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	5.556	168	107434	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	177061	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	157725	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.024	152	73827	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.958	65	77227	51.734	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	103.460%
35) Dibromofluoromethane	5.385	113	61912	49.020	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.040%
50) Toluene-d8	8.646	98	219992	50.093	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	100.180%
62) 4-Bromofluorobenzene	11.079	95	84465	49.236	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	98.480%
Target Compounds						
						Qvalue
19) Methyl tert-butyl Ether	3.111	73	4761	1.257	ug/l	97
44) Trichloroethene	7.128	130	1231	0.879	ug/l	99
52) Toluene	8.720	92	2461	0.758	ug/l	99
64) Tetrachloroethene	9.281	164	410	0.355	ug/l #	73

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032900.D
Acq On : 17 Nov 2022 15:16
Operator : JC/MD
Sample : N5671-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115

Quant Time: Nov 18 01:41:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260
QLast Update : Thu Oct 27 08:28:06 2022
Response via : Initial Calibration




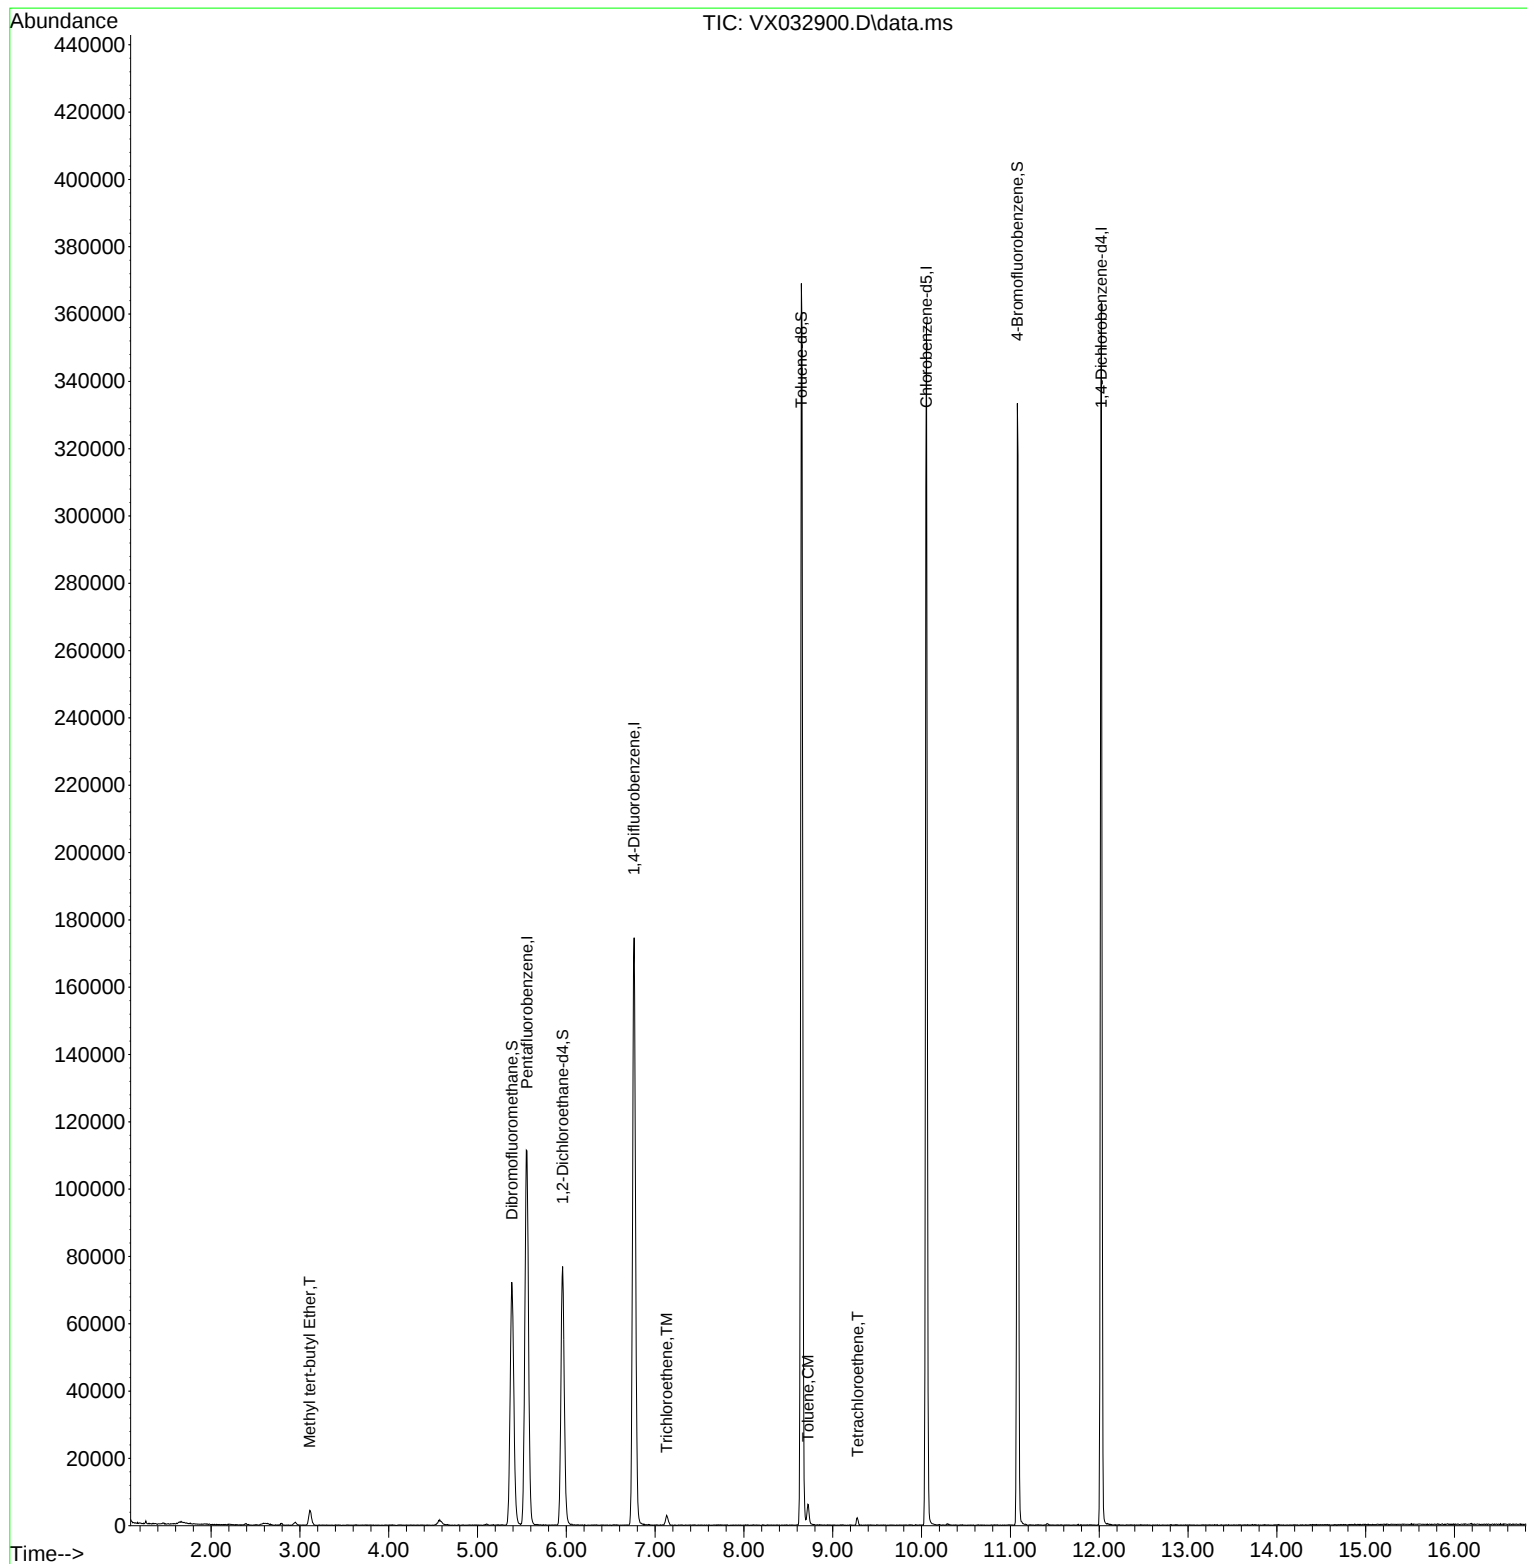




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.556 min Scan# 733
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16




Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115


Tgt Ion:168 Resp: 107434
Ion Ratio Lower Upper
168 100
99 54.8 46.1 69.1

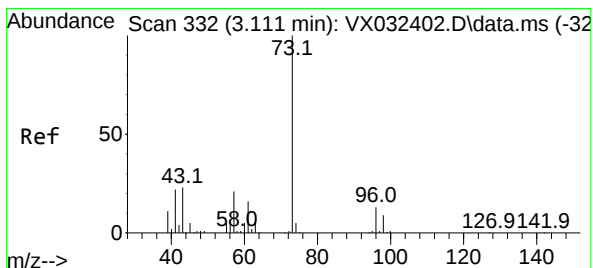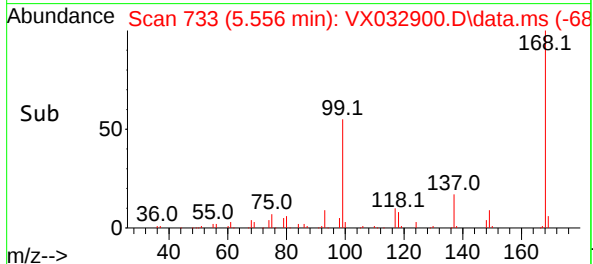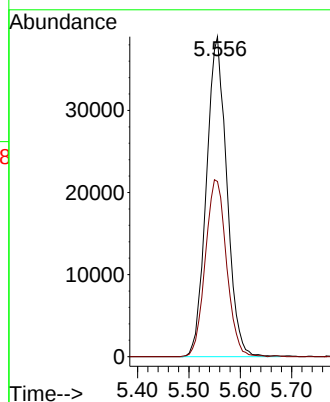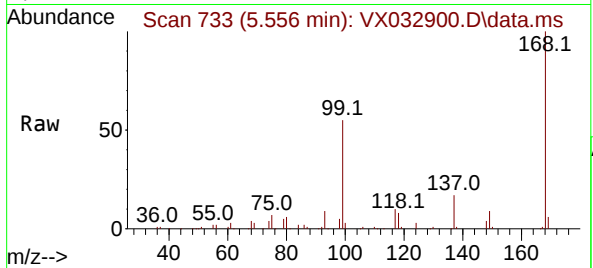

#19
Methyl tert-butyl Ether
Concen: 1.257 ug/l
RT: 3.111 min Scan# 332
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16

Tgt Ion: 73 Resp: 4761
Ion Ratio Lower Upper
73 100
57 22.4 16.6 25.0

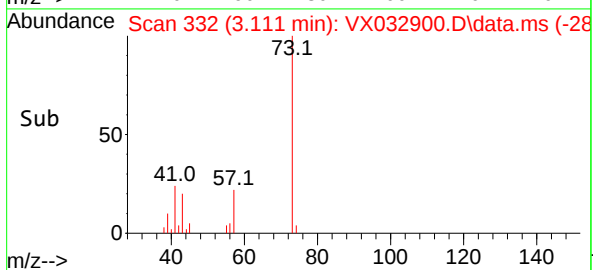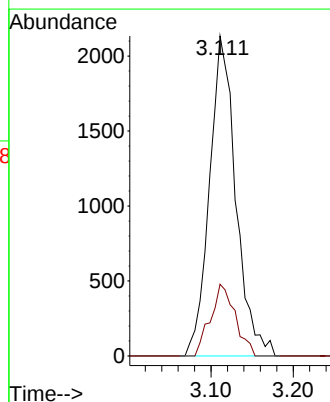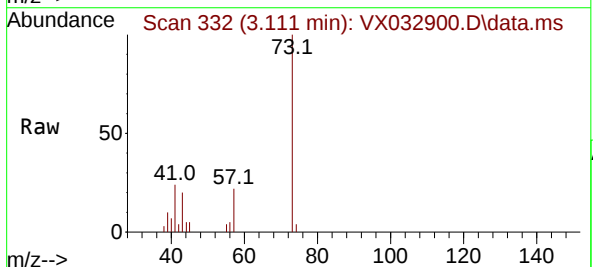

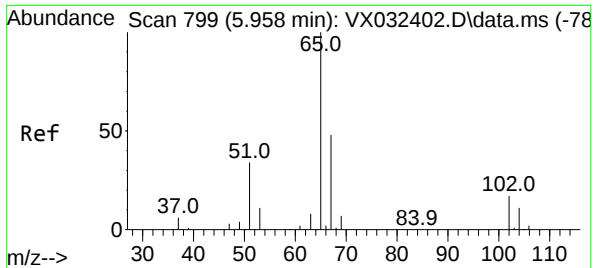

#33

1,2-Dichloroethane-d4

Concen: 51.734 ug/l

RT: 5.958 min Scan# 799

Delta R.T. -0.000 min

Lab File: VX032900.D

Acq: 17 Nov 2022 15:16

Instrument :

MSVOA_X

ClientSampleId :





MW178S-20221115

Tgt Ion: 65 Resp: 77227

Ion Ratio Lower Upper

65 100

67 49.5 0.0 101.8

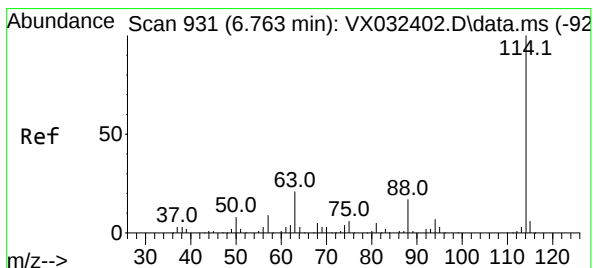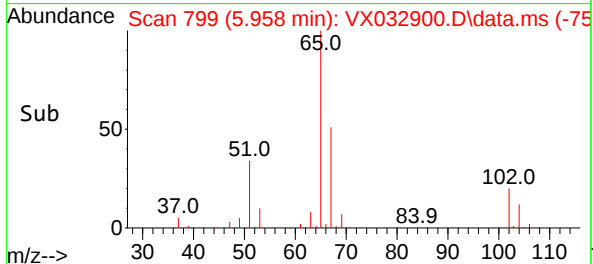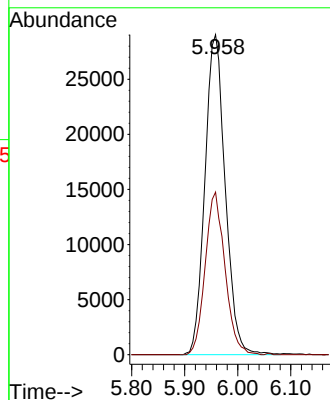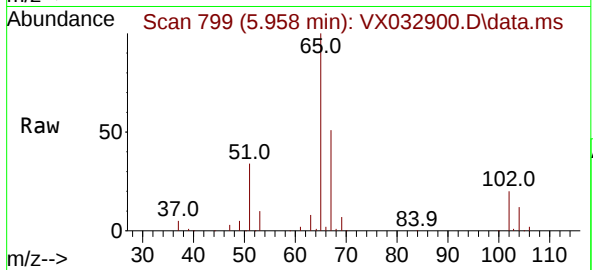

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.763 min Scan# 931

Delta R.T. -0.000 min

Lab File: VX032900.D

Acq: 17 Nov 2022 15:16




Tgt Ion: 114 Resp: 177061

Ion Ratio Lower Upper

114 100

63 18.9 0.0 41.6

88 15.0 0.0 33.4


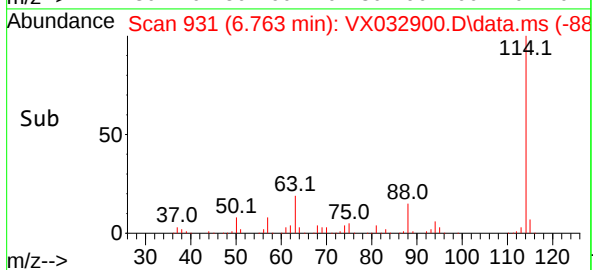
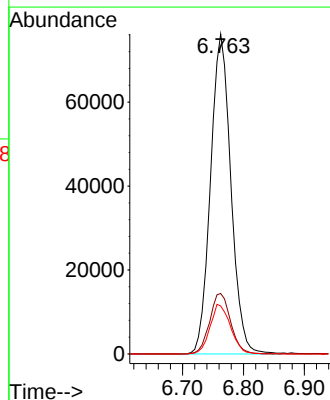
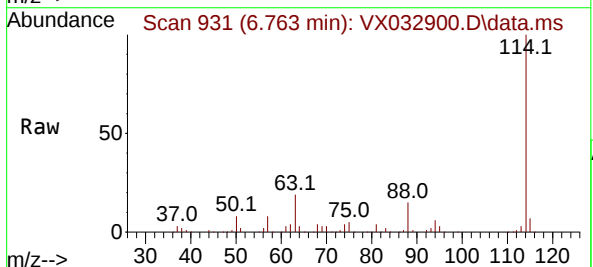




#35
Dibromofluoromethane
Concen: 49.020 ug/l
RT: 5.385 min Scan# 705
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16




Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115


Tgt Ion:113 Resp: 61912
Ion Ratio Lower Upper
113 100
111 101.7 82.4 123.6
192 19.6 15.4 23.2

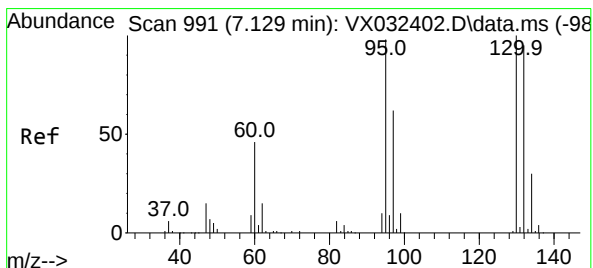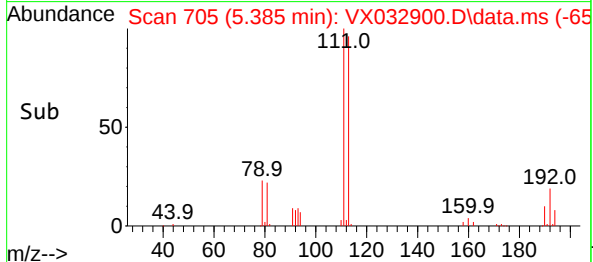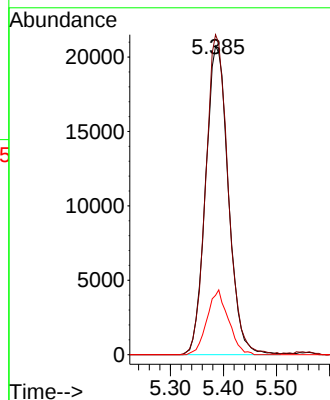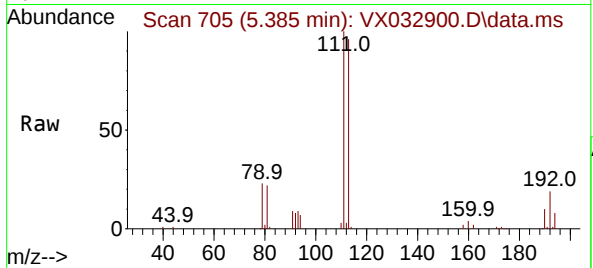

#44
Trichloroethene
Concen: 0.879 ug/l
RT: 7.128 min Scan# 991
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16

Tgt Ion:130 Resp: 1231
Ion Ratio Lower Upper
130 100
95 96.9 0.0 195.2

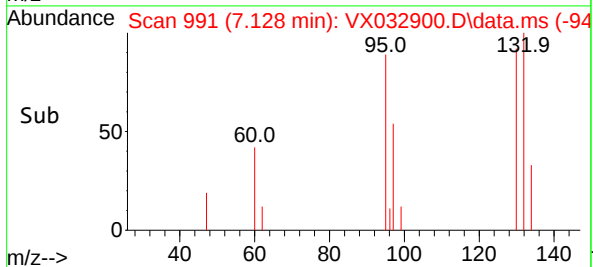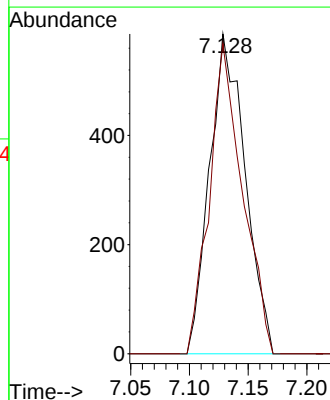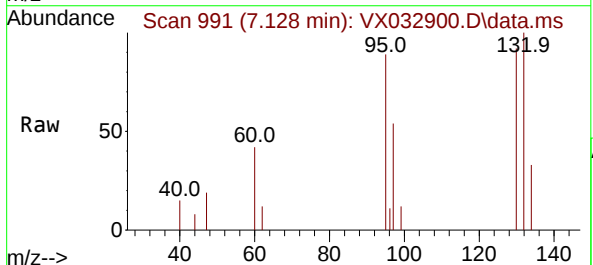

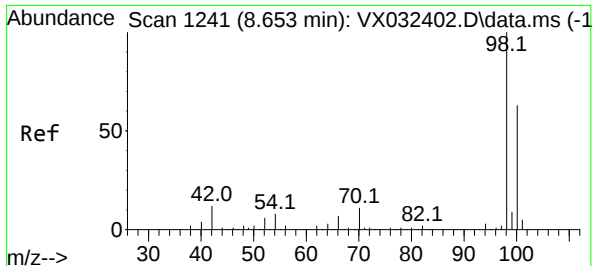

#50

Toluene-d8

Concen: 50.093 ug/l

RT: 8.646 min Scan# 1

Delta R.T. -0.006 min

Lab File: VX032900.D

Acq: 17 Nov 2022 15:16

Instrument :

MSVOA_X

ClientSampleId :





MW178S-20221115

Tgt Ion: 98 Resp: 219992

Ion Ratio Lower Upper

98 100

100 64.0 50.9 76.3

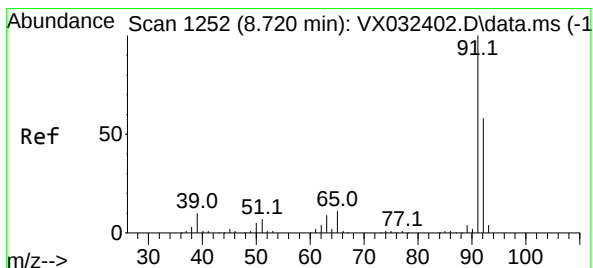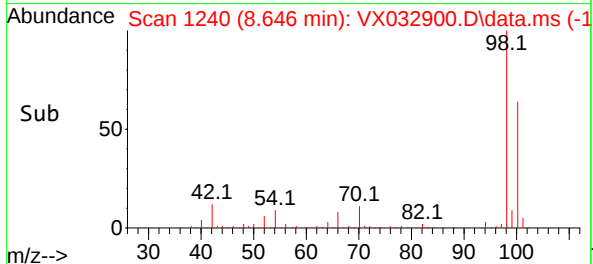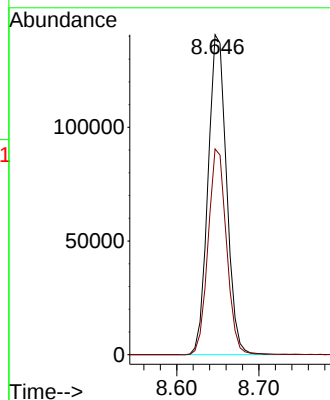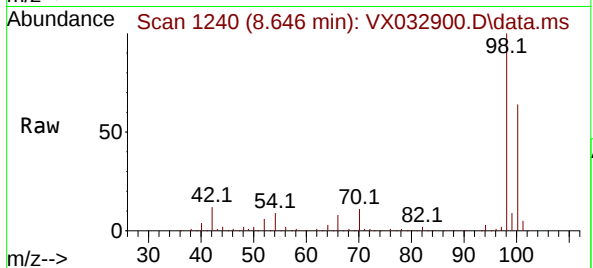

#52

Toluene

Concen: 0.758 ug/l

RT: 8.720 min Scan# 1252

Delta R.T. -0.000 min

Lab File: VX032900.D




Acq: 17 Nov 2022 15:16


Tgt Ion: 92 Resp: 2461

Ion Ratio Lower Upper

92 100

91 174.3 138.3 207.5


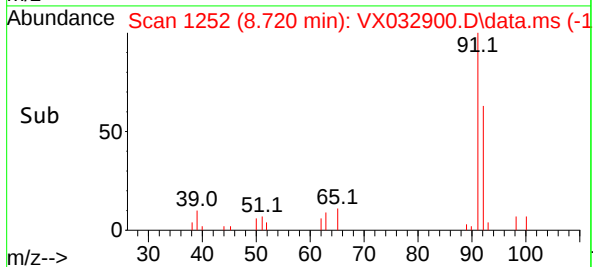
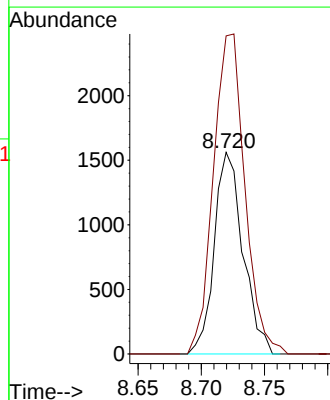
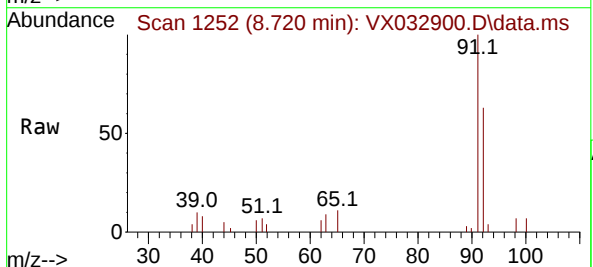


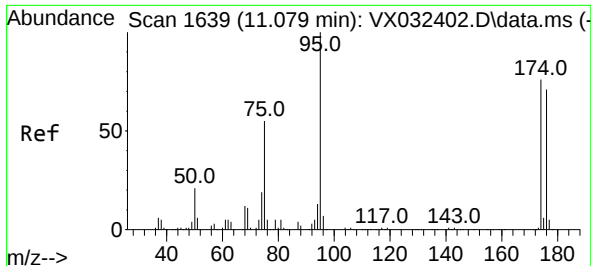

#62
4-Bromofluorobenzene
Concen: 49.236 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16




Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115


Tgt Ion: 95 Resp: 84465
Ion Ratio Lower Upper
95 100
174 82.7 0.0 164.0
176 80.3 0.0 154.4

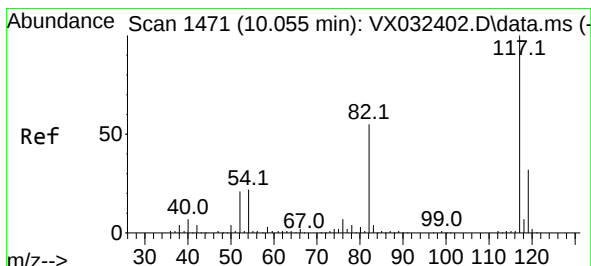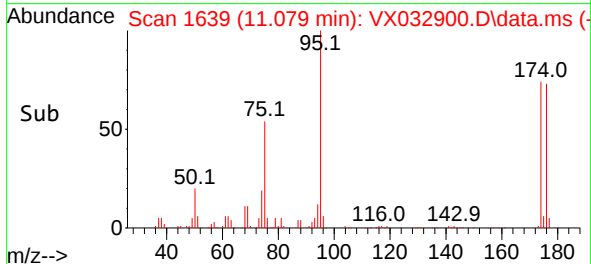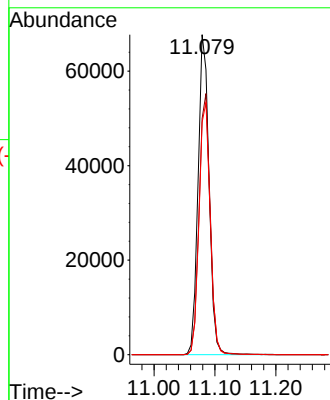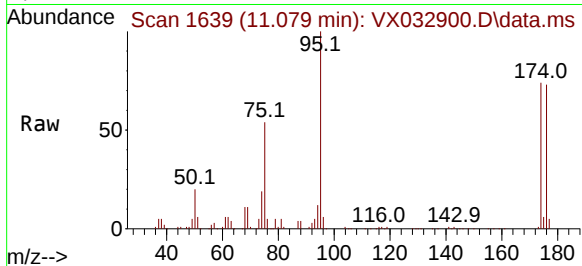

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16

Tgt Ion: 117 Resp: 157725
Ion Ratio Lower Upper
117 100
82 54.8 44.3 66.5
119 32.5 25.7 38.5


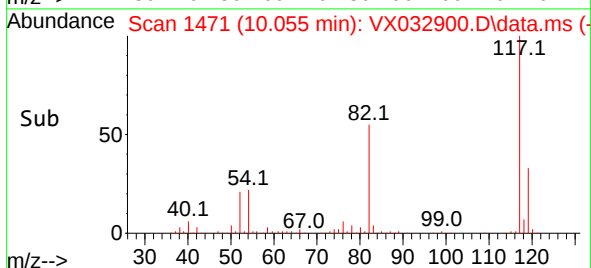
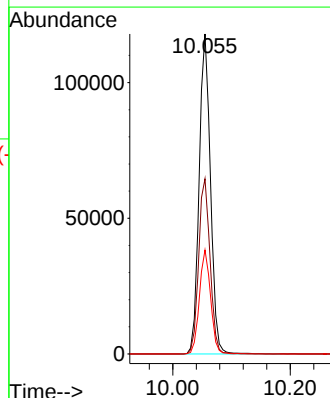
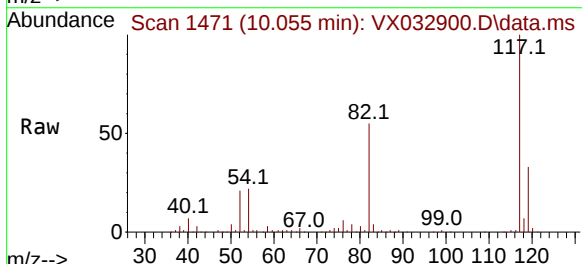


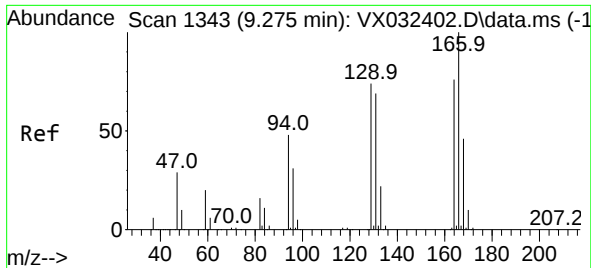

#64
Tetrachloroethene
Concen: 0.355 ug/l
RT: 9.281 min Scan# 11
Delta R.T. 0.006 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115

Tgt Ion:164 Resp: 410
Ion Ratio Lower Upper
164 100
166 105.2 105.4 158.2#
129 60.1 78.2 117.2#
131 70.5 72.5 108.7#

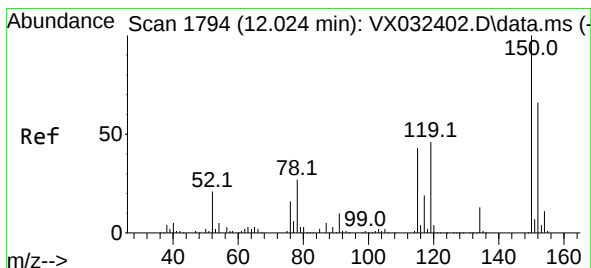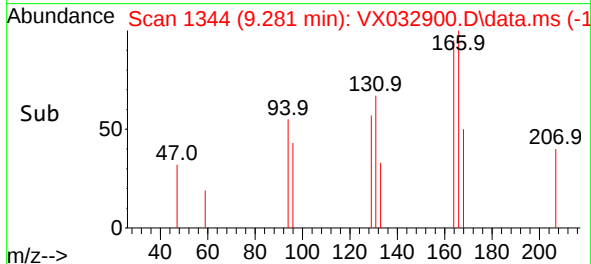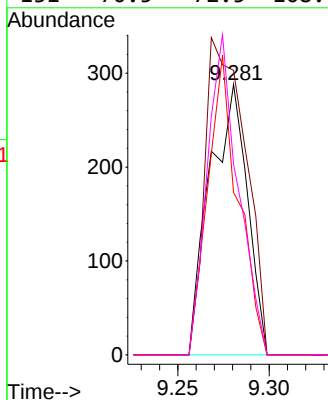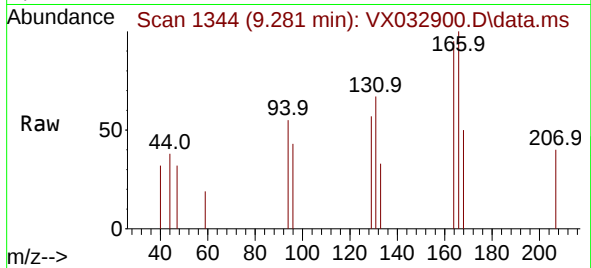

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.024 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VX032900.D
Acq: 17 Nov 2022 15:16

Tgt Ion:152 Resp: 73827
Ion Ratio Lower Upper
152 100
115 59.0 44.0 132.0
150 156.9 0.0 351.8

