

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032900.D
Acq On : 17 Nov 2022 15:16
Operator : JC/MD
Sample : N5671-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Title : SW846 8260

Signal : TIC: VX032900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.111	323	332	344	rVB2	4461	10550	1.82%	0.340%
2	5.385	694	705	721	rBV2	72145	207771	35.92%	6.690%
3	5.549	721	732	750	rVB	111311	316421	54.70%	10.189%
4	5.958	788	799	814	rBV	76835	201473	34.83%	6.488%
5	6.763	920	931	947	rBV	174548	411694	71.17%	13.257%
6	7.128	986	991	999	rVB3	2958	6014	1.04%	0.194%
7	8.646	1234	1240	1248	rBV	368913	578442	100.00%	18.627%
8	8.720	1248	1252	1262	rVB	6107	11068	1.91%	0.356%
9	10.055	1465	1471	1482	rBV	357299	479780	82.94%	15.450%
10	11.079	1634	1639	1653	rBV	333369	429462	74.24%	13.829%
11	12.024	1789	1794	1804	rBV	363119	452789	78.28%	14.580%




Sum of corrected areas: 3105464

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032900.D
Acq On : 17 Nov 2022 15:16
Operator : JC/MD
Sample : N5671-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

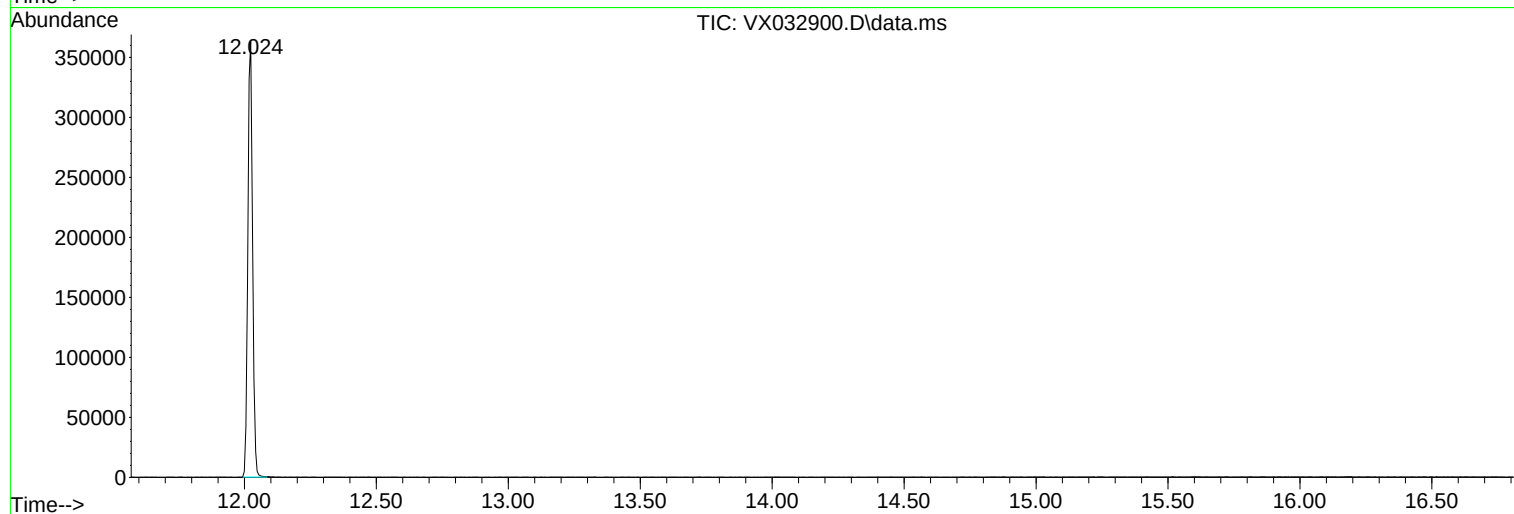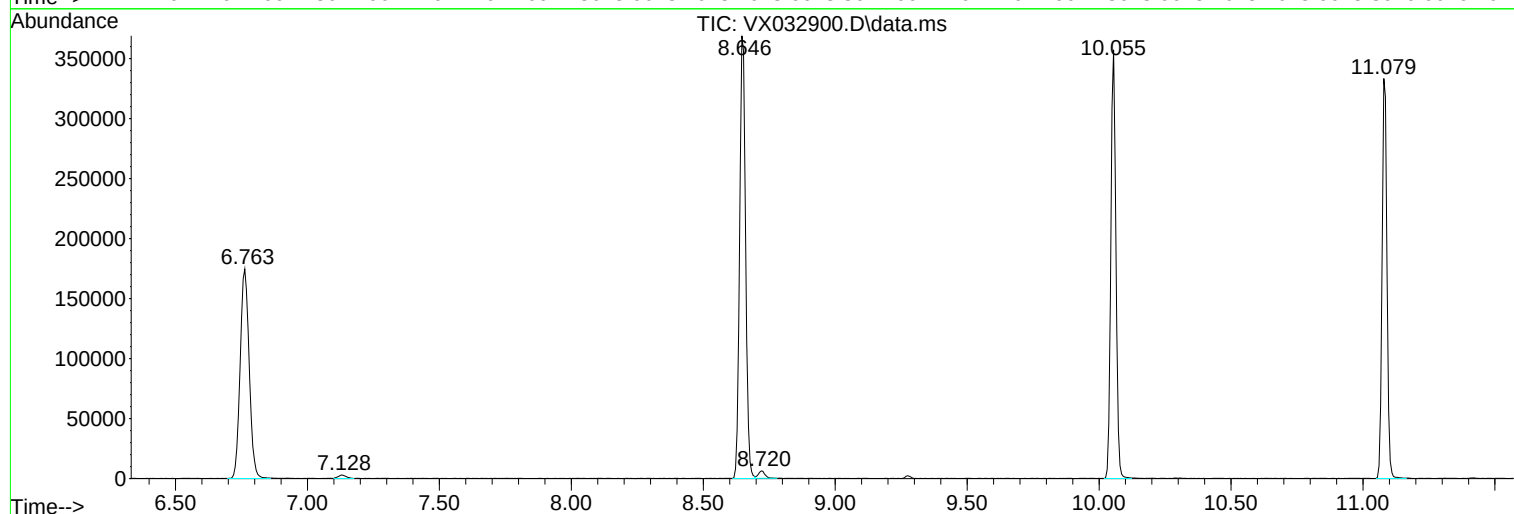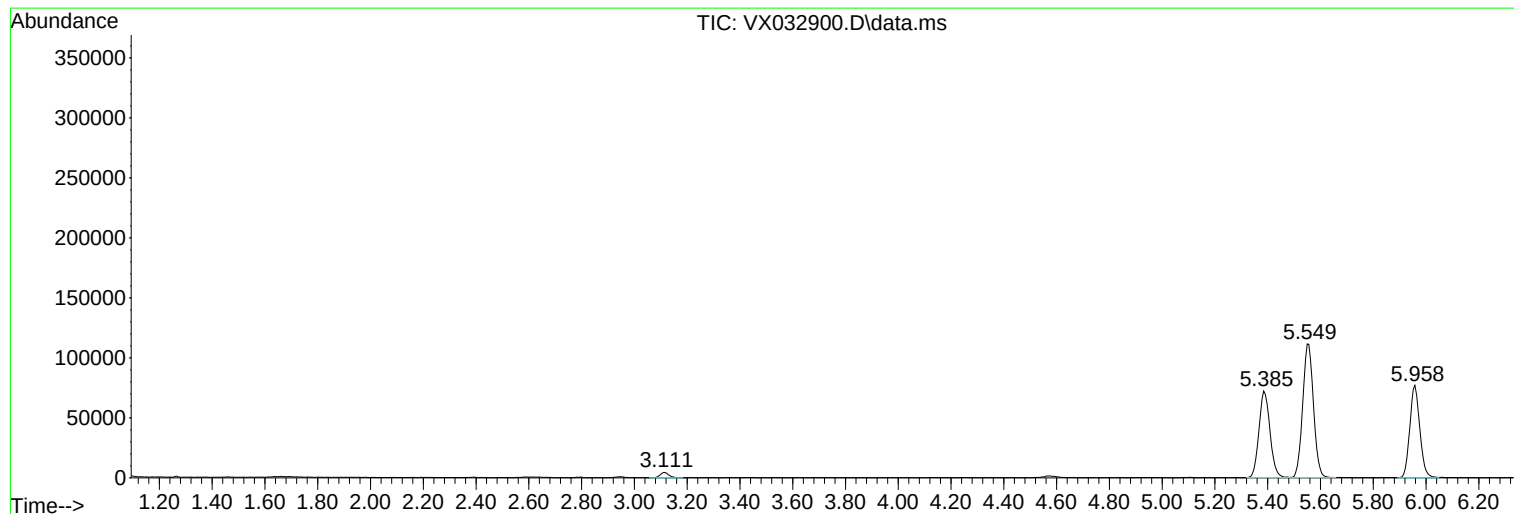

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032900.D
Acq On : 17 Nov 2022 15:16
Operator : JC/MD
Sample : N5671-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032900.D
Acq On : 17 Nov 2022 15:16
Operator : JC/MD
Sample : N5671-05
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
MW178S-20221115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------