

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032903.D
Acq On : 17 Nov 2022 16:25
Operator : JC/MD
Sample : N5671-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20221115

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032903.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.330	195	204	221	rBV	2176964	4098891	100.00%	40.286%
2	5.391	690	706	719	rBV	77308	225197	5.49%	2.213%
3	5.549	721	732	747	rVV	121423	343522	8.38%	3.376%
4	5.958	789	799	811	rBV	82382	217961	5.32%	2.142%
5	6.763	919	931	945	rBV	189447	447666	10.92%	4.400%
6	7.122	981	990	1004	rBV	669320	1469477	35.85%	14.443%
7	8.646	1234	1240	1248	rBV	402185	635915	15.51%	6.250%
8	9.274	1336	1343	1355	rVB	837392	1196598	29.19%	11.761%
9	10.055	1465	1471	1486	rBV	399799	540200	13.18%	5.309%
10	11.079	1634	1639	1652	rBV	370110	481633	11.75%	4.734%
11	12.024	1788	1794	1806	rBV	410430	517313	12.62%	5.084%




Sum of corrected areas: 10174373

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032903.D
Acq On : 17 Nov 2022 16:25
Operator : JC/MD
Sample : N5671-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20221115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

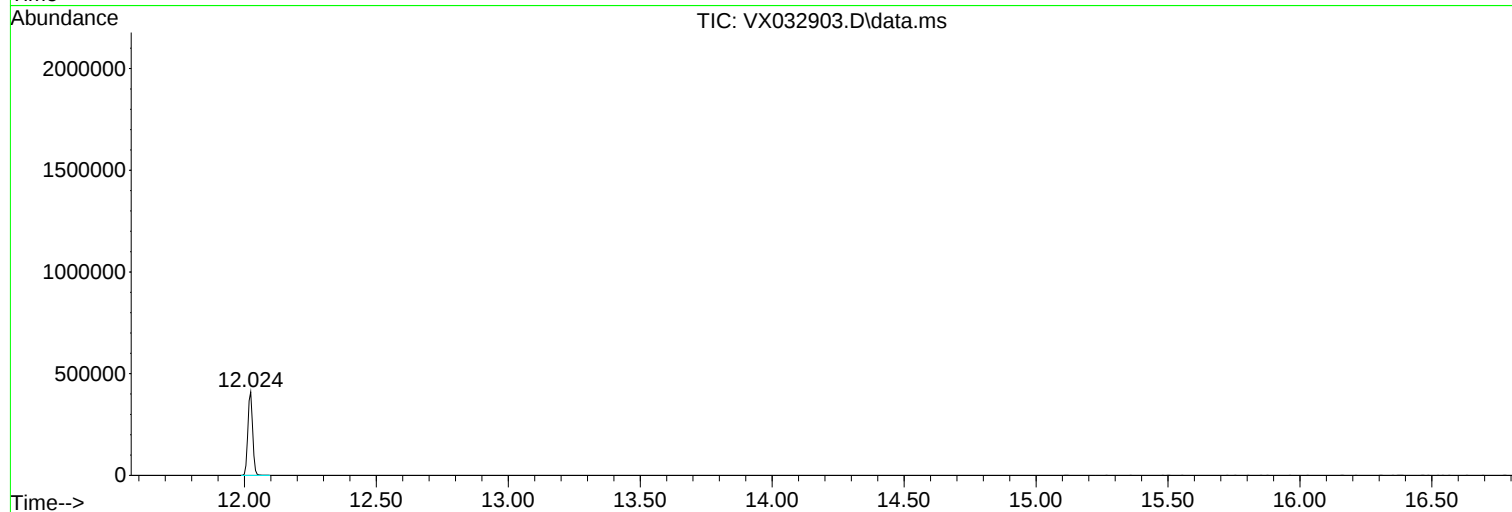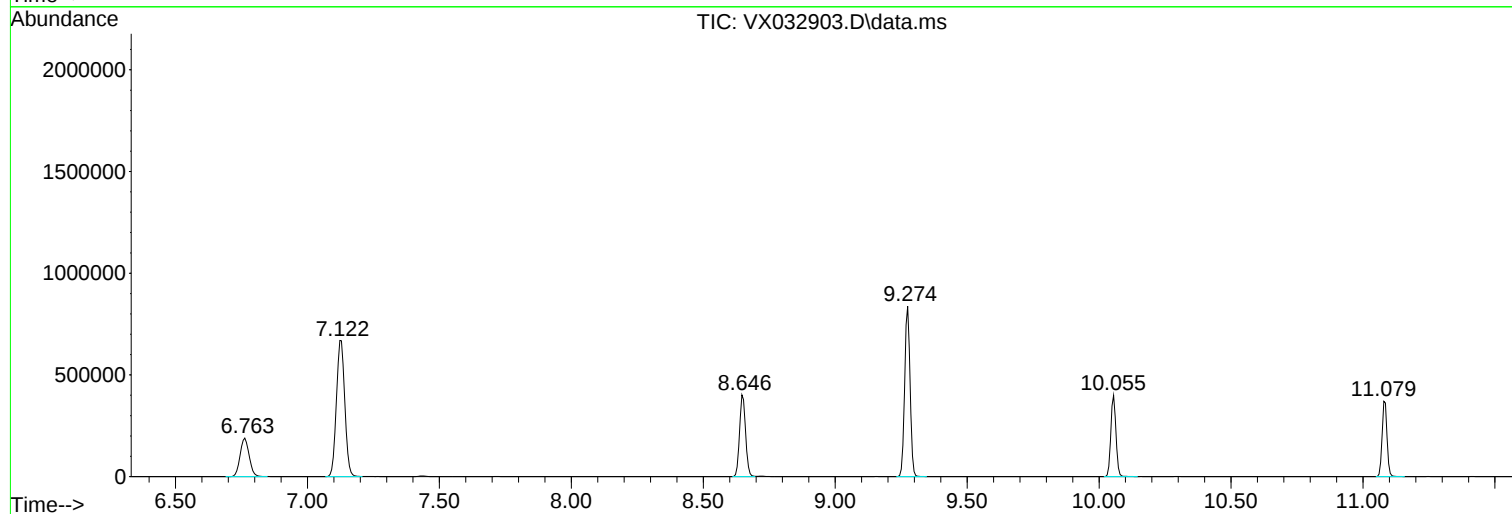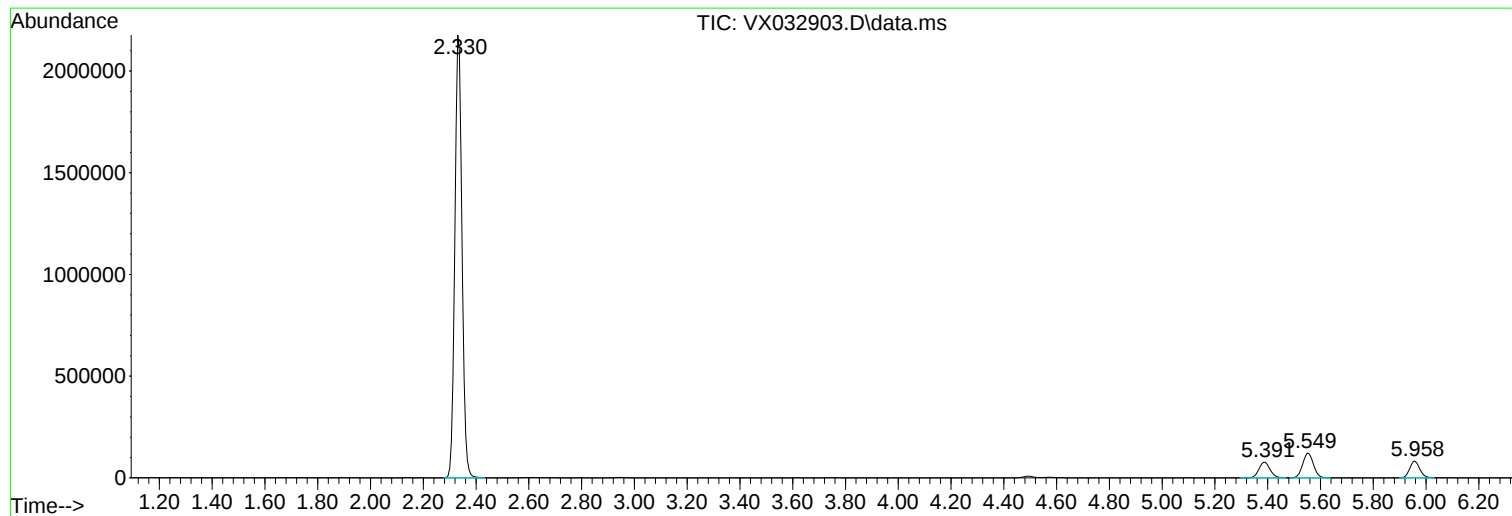

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032903.D
Acq On : 17 Nov 2022 16:25
Operator : JC/MD
Sample : N5671-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20221115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032903.D
Acq On : 17 Nov 2022 16:25
Operator : JC/MD
Sample : N5671-08
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE134D3-20221115

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------