

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
 Data File : VX032908.D
 Acq On : 17 Nov 2022 18:21
 Operator : JC/MD
 Sample : N5672-03
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 RE125D3-20221116

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M

Title : SW846 8260

Signal : TIC: VX032908.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.331	196	204	218	rBV	348499	655077	60.87%	13.336%
2	5.385	695	705	721	rBV2	69801	203902	18.95%	4.151%
3	5.550	721	732	748	rVV	109914	310347	28.84%	6.318%
4	5.958	788	799	814	rBV	74917	200153	18.60%	4.075%
5	6.763	921	931	948	rBV	167723	406382	37.76%	8.273%
6	7.123	980	990	1006	rBV	490313	1076275	100.00%	21.911%
7	8.647	1234	1240	1249	rBV	373708	575779	53.50%	11.722%
8	9.275	1337	1343	1351	rBV	74868	107981	10.03%	2.198%
9	10.055	1465	1471	1480	rBV	366965	485857	45.14%	9.891%
10	11.079	1634	1639	1650	rBV	341231	430961	40.04%	8.774%
11	12.024	1788	1794	1801	rBV	364212	459348	42.68%	9.351%




Sum of corrected areas: 4912062

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032908.D
Acq On : 17 Nov 2022 18:21
Operator : JC/MD
Sample : N5672-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20221116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

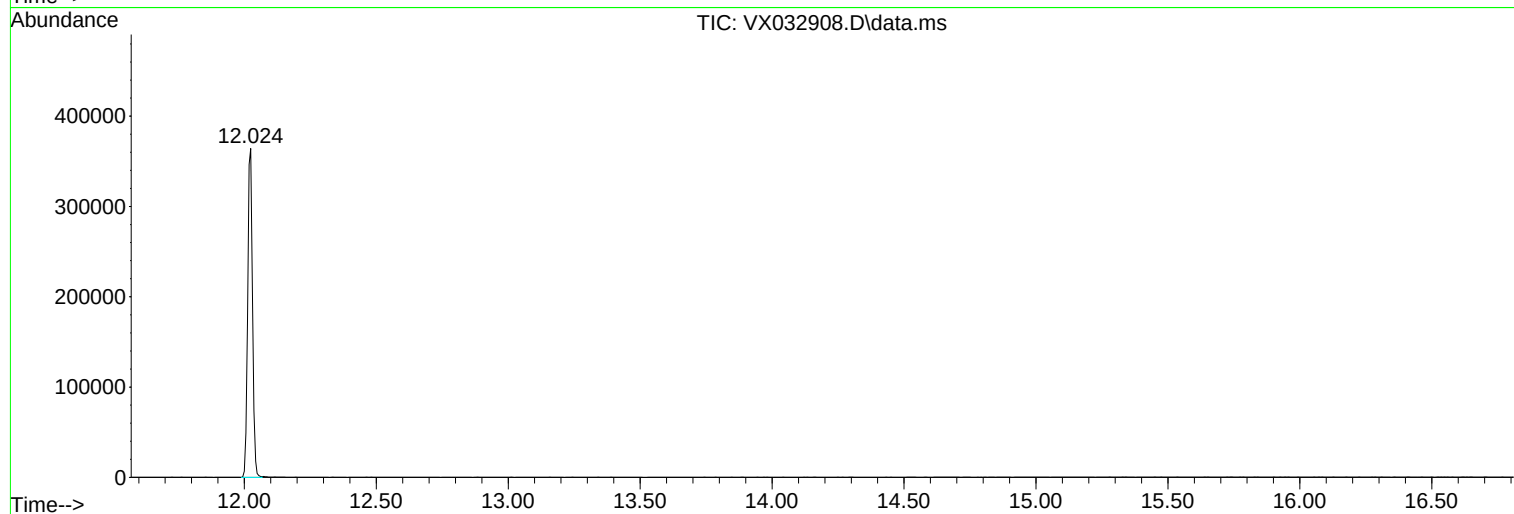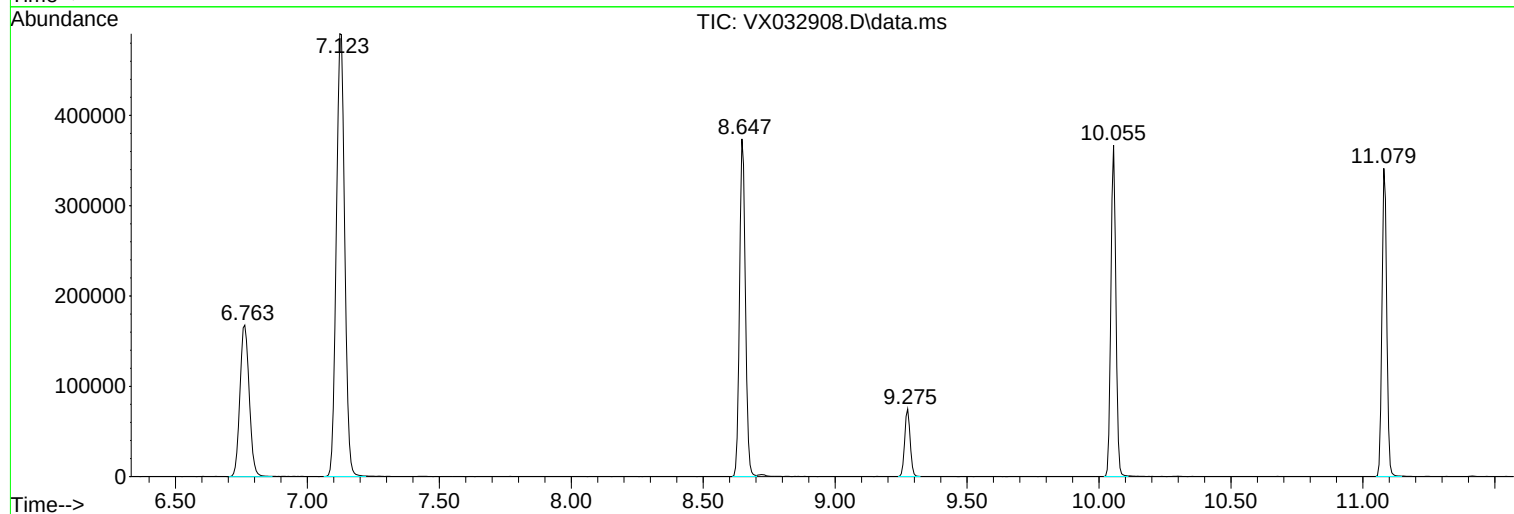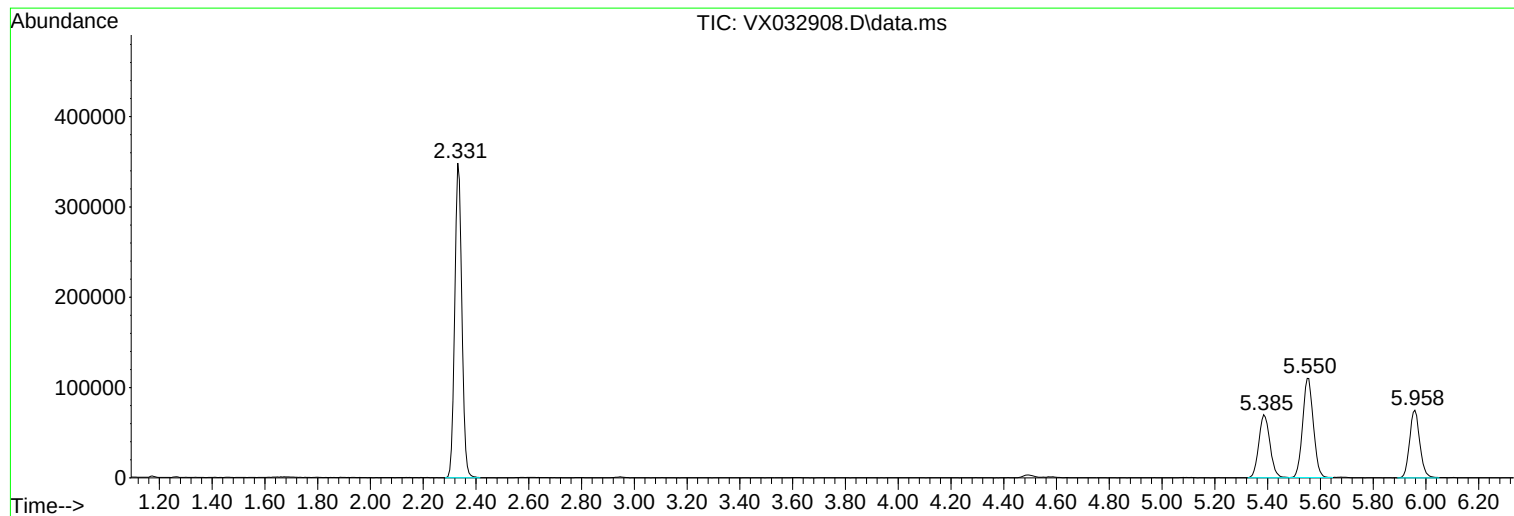

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032908.D
Acq On : 17 Nov 2022 18:21
Operator : JC/MD
Sample : N5672-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20221116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111722\
Data File : VX032908.D
Acq On : 17 Nov 2022 18:21
Operator : JC/MD
Sample : N5672-03
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
RE125D3-20221116

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X102622W.M
Quant Title : SW846 8260

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------