
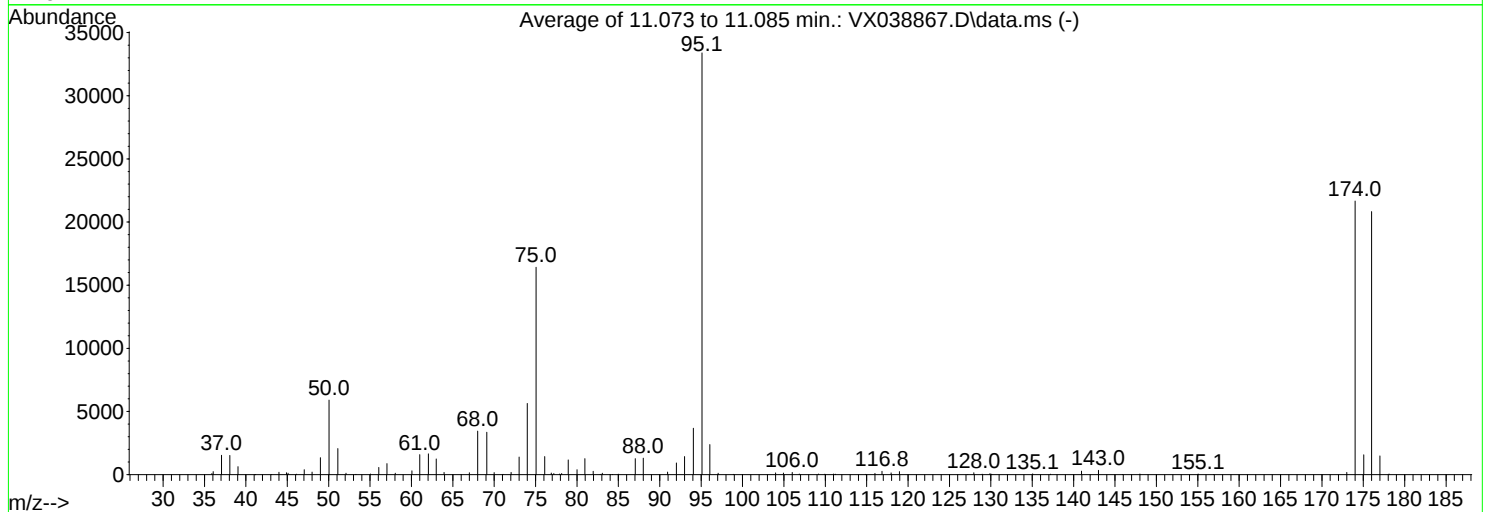


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX111723\
Data File : VX038867.D
Acq On : 17 Nov 2023 08:36
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X111623W.M
Title : SW846 8260
Last Update : Thu Nov 16 22:59:22 2023

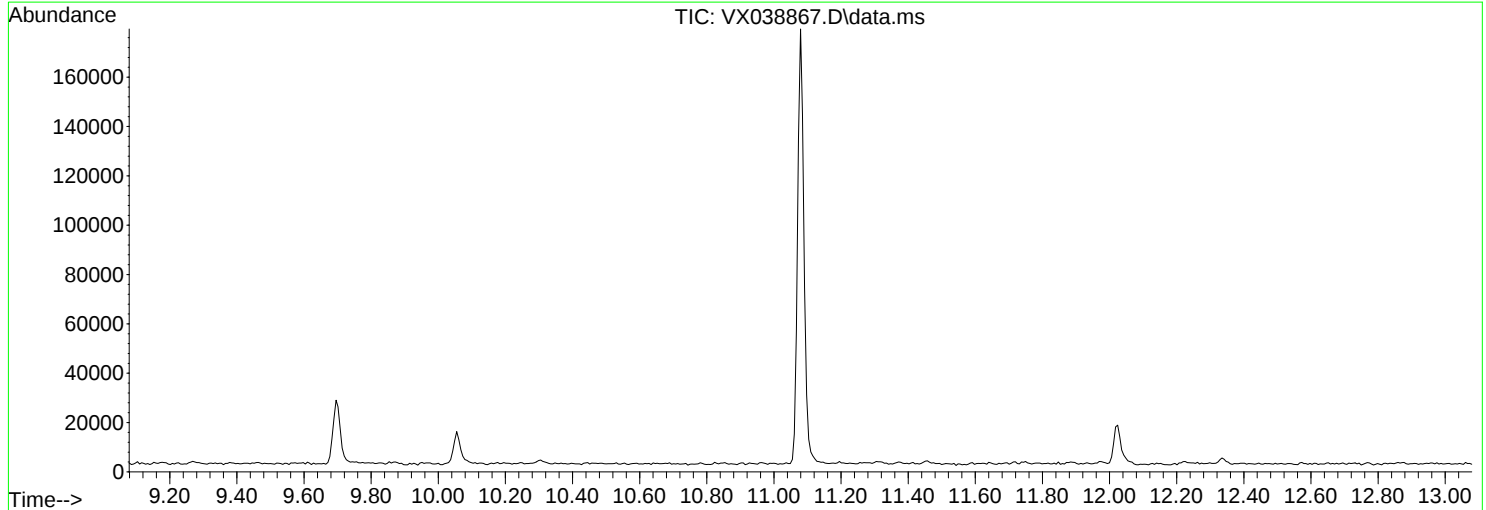

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1631

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	5904	PASS
75	95	30	60	49.2	16422	PASS
95	95	100	100	100.0	33397	PASS
96	95	5	9	7.2	2388	PASS
173	174	0.00	2	0.8	173	PASS
174	95	50	100	64.9	21664	PASS
175	174	5	9	7.2	1566	PASS
176	174	95	101	96.1	20826	PASS
177	176	5	9	7.1	1486	PASS